
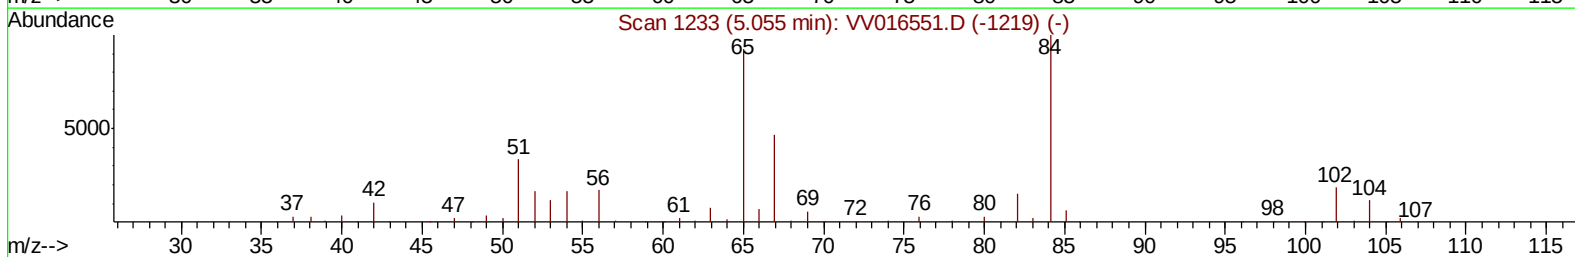
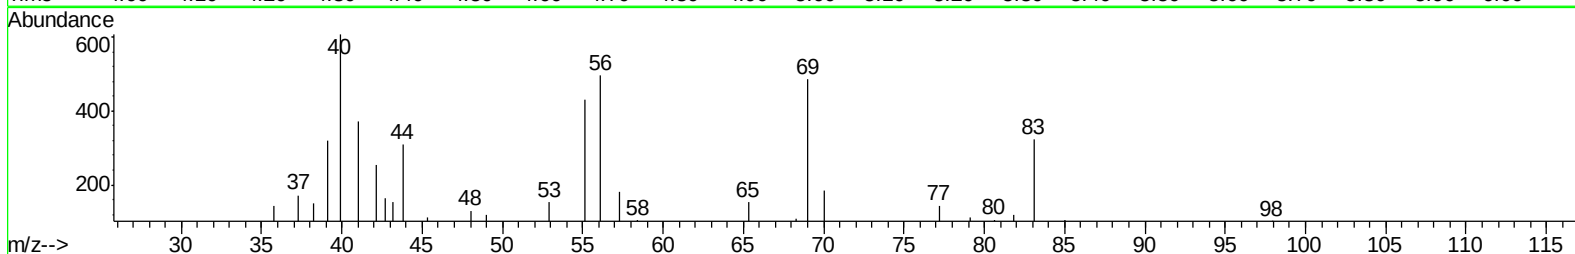


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV060520\
 Data File : VV016547.D
 Acq On : 05 Jun 2020 19:39
 Operator : SY/MD
 Sample : L2861-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Quant Time: Jun 06 08:25:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 06 06:28:49 2020
 Response via : Initial Calibration

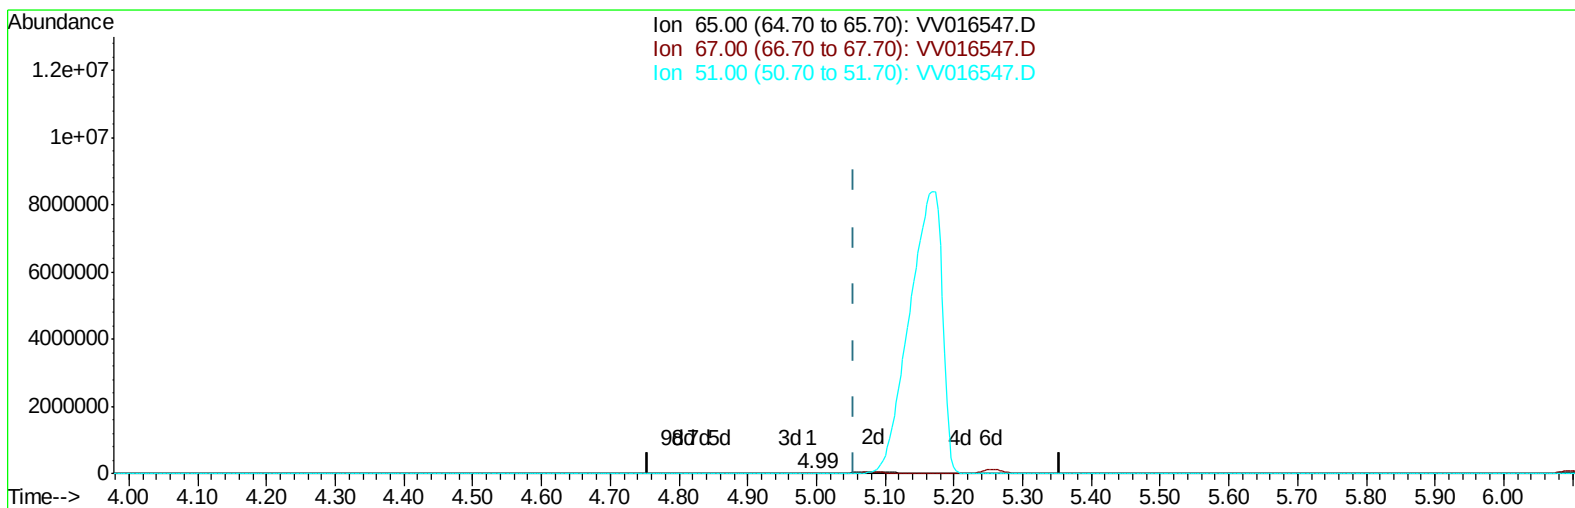

TIC: VV016547.D

(26) 1,2-Dichloroethane-d4 (S)

4.994min (-0.061) 0.04ug/L

response 151

Ion	Exp%	Act%
65.00	100	100
67.00	52.20	54.30
51.00	37.30	47.68
0.00	0.00	0.00