

Quantitation Report (QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060520\
 Data File : VV016565.D
 Acq On : 06 Jun 2020 03:40
 Operator : SY/MD
 Sample : L2862-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D97

Quant Time: Jun 06 07:27:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 06 06:28:49 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sam
 6/6/2020 11:33:24 AM

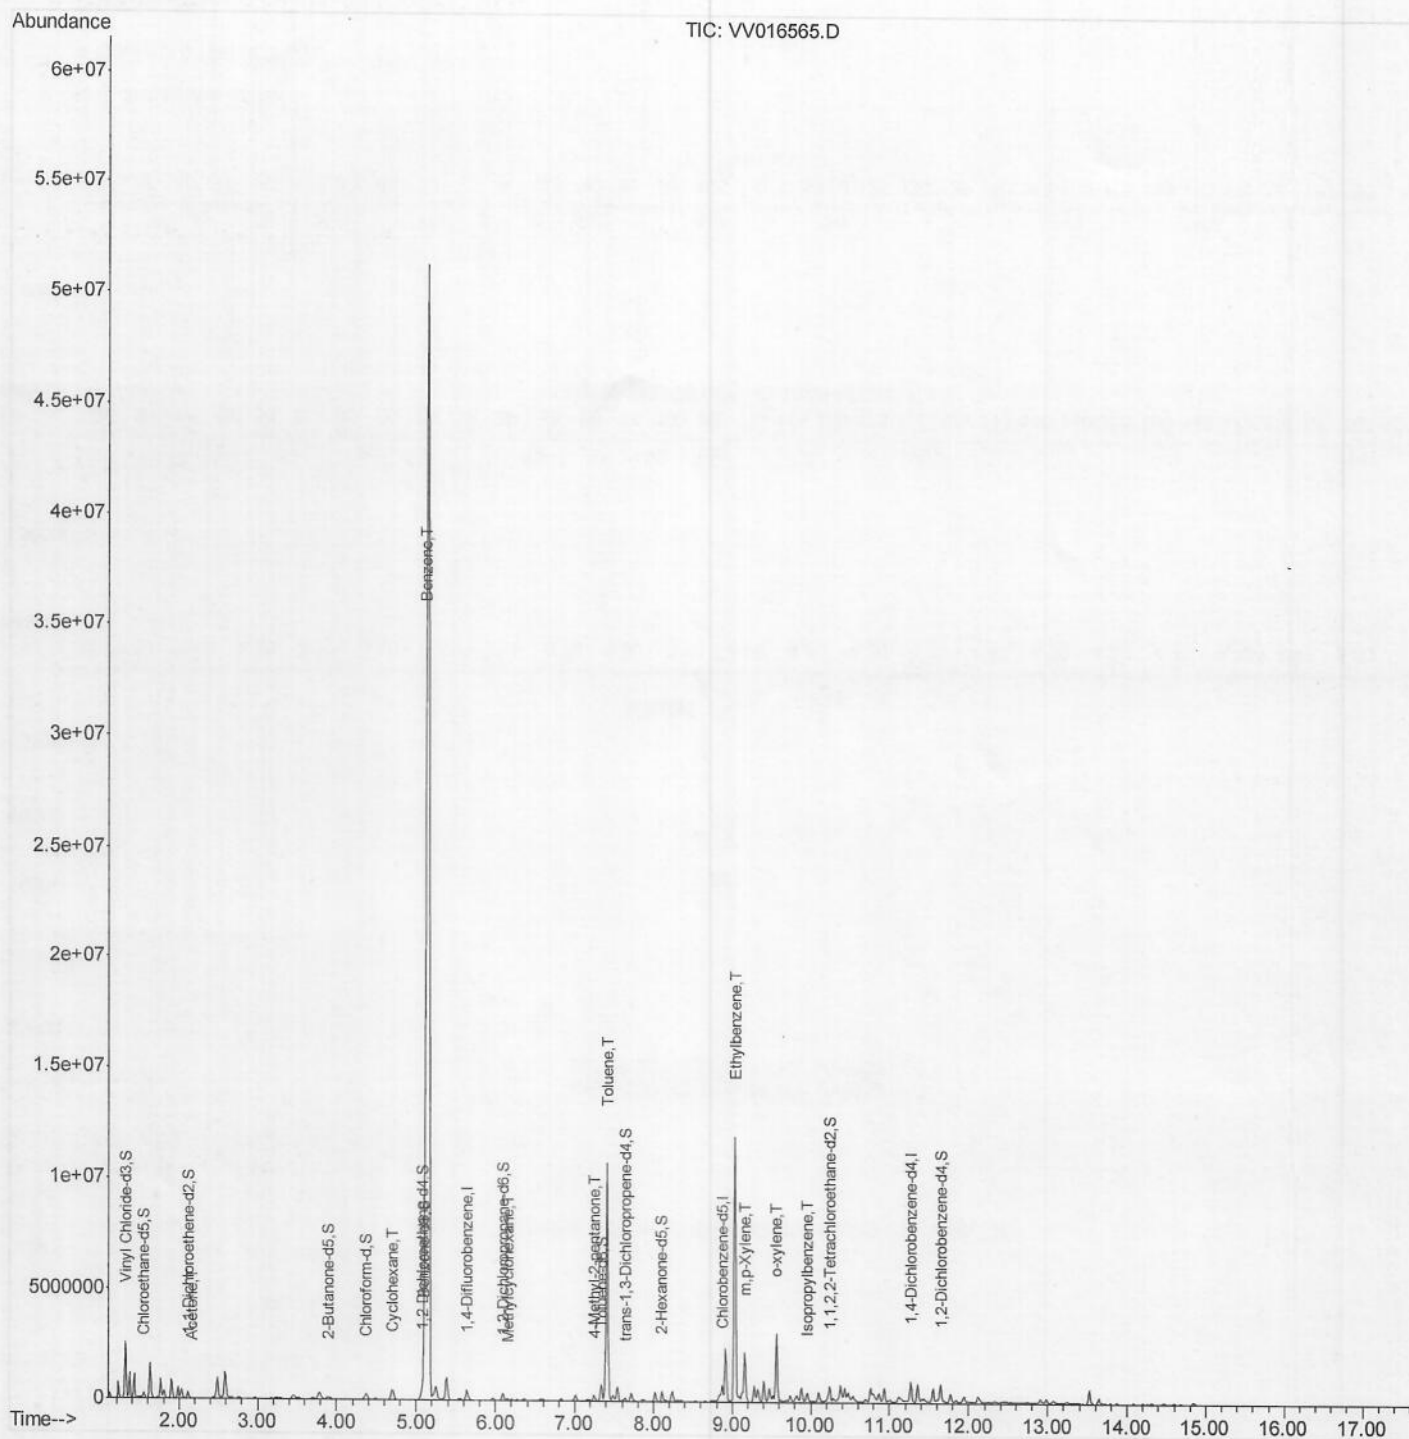

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060520\
 Data File : VV016565.D
 Acq On : 06 Jun 2020 03:40
 Operator : SY/MD
 Sample : L2862-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 F9D97

Quant Time: Jun 06 06:32:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 06 06:28:49 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sam
 6/6/2020 11:33:24 AM

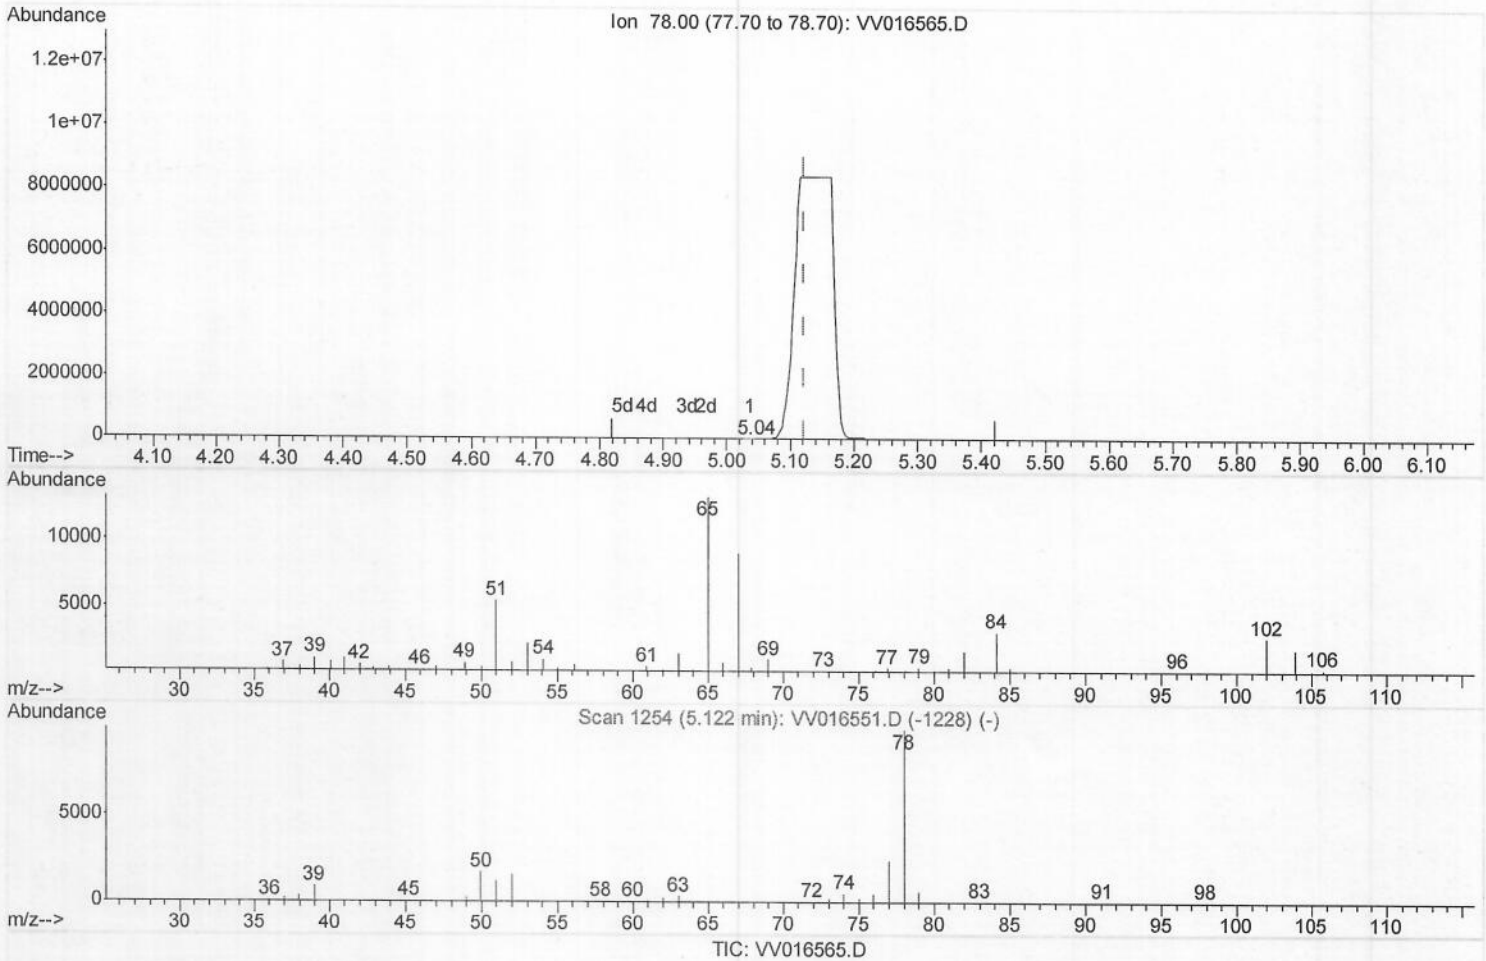

(33) Benzene (T)

5.039min (-0.084) 0.01ug/L

response 136

Ion	Exp%	Act%
78.00	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060520\
 Data File : VV016565.D
 Acq On : 06 Jun 2020 03:40
 Operator : SY/MD
 Sample : L2862-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D97

Manual Integrations
 APPROVED

sam
 6/6/2020 11:33:24 AM

Quant Time: Jun 06 06:32:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 06 06:28:49 2020
 Response via : Initial Calibration

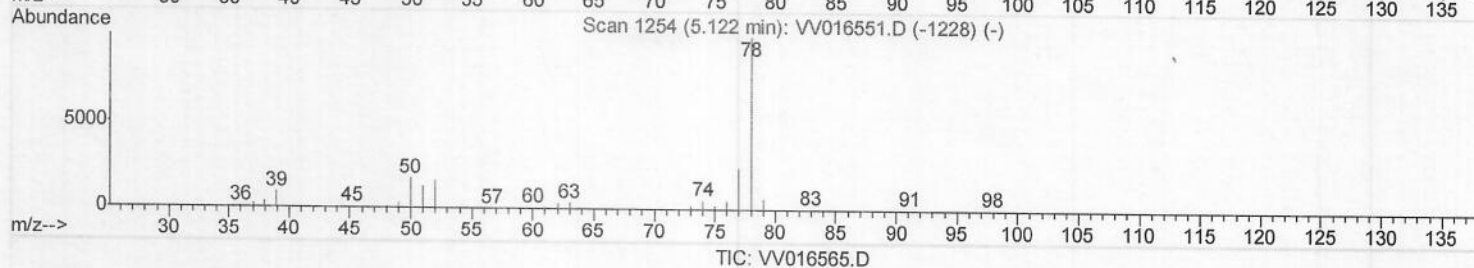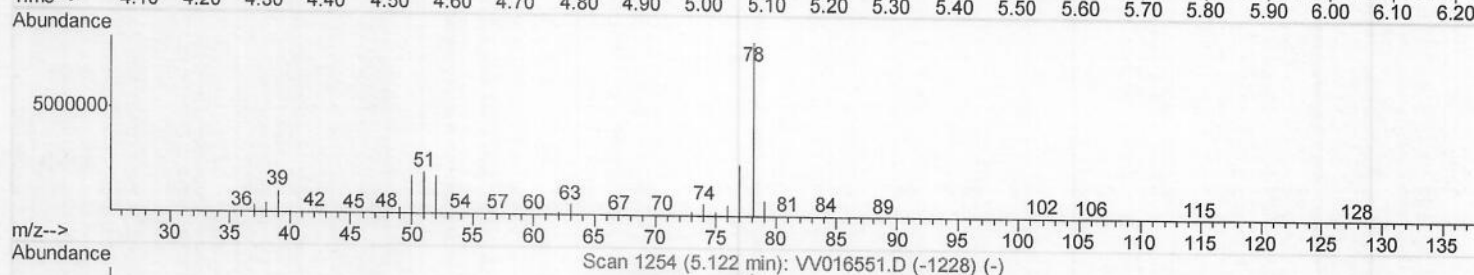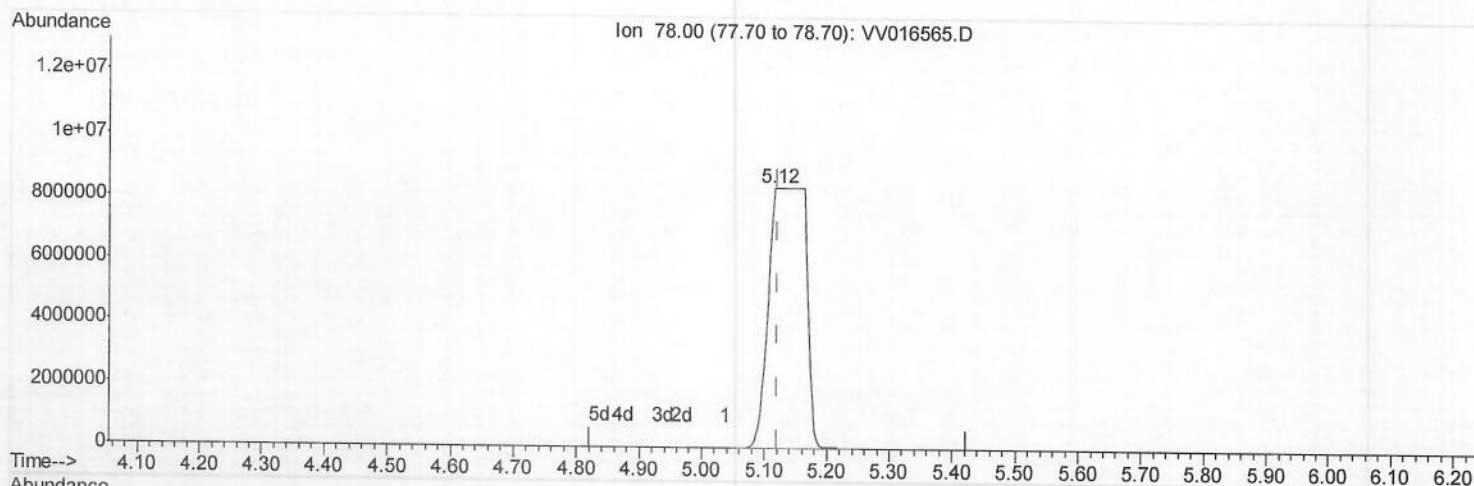

(33) Benzene (T)

5.116min (-0.007) 3179.40ug/L m

response 34612669

Ion	Exp%	Act%
78.00	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

M.D
 6/6/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060520\
 Data File : VV016565.D
 Acq On : 06 Jun 2020 03:40
 Operator : SY/MD
 Sample : L2862-11
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D97

Manual Integrations
 APPROVED

sam
 6/6/2020 11:33:24 AM

Quant Time: Jun 06 07:27:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 06 06:28:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	387314	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	370167	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	181945	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.31	65	118802	43.31	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery =	86.62%		
7) Chloroethane-d5	1.56	69	86422	43.64	ug/L	-0.02
Spiked Amount 50.000	Range 70	- 130	Recovery =	87.28%		
11) 1,1-Dichloroethene-d2	2.12	63	161478	33.21	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery =	66.42%		
21) 2-Butanone-d5	3.90	46	194101	110.66	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery =	110.66%		
24) Chloroform-d	4.37	84	247068	47.99	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	95.98%		
26) 1,2-Dichloroethane-d4	5.06	65	180632	52.40	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	104.80%		
32) Benzene-d6	5.08	84	498381	50.26	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	100.52%		
36) 1,2-Dichloropropane-d6	6.09	67	152028	49.21	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery =	98.42%		
41) Toluene-d8	7.34	98	463024	51.42	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	102.84%		
43) trans-1,3-Dichloropropene-	7.64	79	73747	48.98	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery =	97.96%		
47) 2-Hexanone-d5	8.11	63	152842	115.51	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery =	115.51%		
57) 1,1,2,2-Tetrachloroethane-	10.24	84	193993	46.30	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery =	92.60%		
64) 1,2-Dichlorobenzene-d4	11.65	152	185575	54.27	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	108.54%		
Target Compounds						
13) Acetone	2.17	43	8018	4.891	ug/L	98
29) Cyclohexane	4.70	56	253681	57.741	ug/L	99
33) Benzene	5.12	78	34612669m	3179.397	ug/L	
35) Methylcyclohexane	6.15	83	16419	4.004	ug/L	89
40) 4-Methyl-2-pentanone	7.25	43	150123	38.450	ug/L	99
42) Toluene	7.41	91	7397321	641.245	ug/L	97
52) Ethylbenzene	9.04	91	7970109	634.792	ug/L	98
53) m,p-Xylene	9.16	106	570179	120.437	ug/L	100
54) o-xylene	9.57	106	777896	169.658	ug/L	98
56) Isopropylbenzene	9.95	105	207300	17.406	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

M.D
 06/08/20