

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016526.D
 Acq On : 05 Jun 2020 11:23
 Operator : SY/MD
 Sample : L2836-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	192298	193494	12.78%	1.695%
2	1.563	140	147	163	rVB	133587	162147	10.71%	1.420%
3	2.116	310	319	341	rVB	307499	455058	30.05%	3.985%
4	2.412	409	411	414	rBV5	1358	640	0.04%	0.006%
5	2.663	485	489	490	rBV3	1333	810	0.05%	0.007%
6	2.859	548	550	553	rBV3	984	517	0.03%	0.005%
7	3.187	649	652	656	rVB2	1273	859	0.06%	0.008%
8	3.206	656	658	660	rBV3	1075	446	0.03%	0.004%
9	3.219	660	662	667	rBV6	1039	986	0.07%	0.009%
10	3.280	679	681	686	rVB6	1486	818	0.05%	0.007%
11	3.331	695	697	699	rBV3	873	552	0.04%	0.005%
12	3.482	741	744	746	rBV3	1171	944	0.06%	0.008%
13	3.563	767	769	773	rVV4	1262	842	0.06%	0.007%
14	3.582	773	775	777	rVB3	1684	672	0.04%	0.006%
15	3.605	777	782	784	rBV3	1804	1505	0.10%	0.013%
16	3.708	810	814	815	rBV3	1375	1100	0.07%	0.010%
17	3.730	819	821	826	rVB7	1154	693	0.05%	0.006%
18	3.749	826	827	831	rBV4	923	509	0.03%	0.004%
19	3.894	860	872	896	rBV	123352	319960	21.13%	2.802%
20	4.309	999	1001	1003	rBV3	940	458	0.03%	0.004%
21	4.373	1006	1021	1040	rVV	243780	592478	39.13%	5.189%
22	4.849	1166	1169	1170	rBV3	1223	568	0.04%	0.005%
23	4.952	1199	1201	1206	rVB5	1602	1023	0.07%	0.009%
24	4.997	1213	1215	1217	rBV3	1406	840	0.06%	0.007%
25	5.071	1220	1238	1264	rVV2	586400	1514267	100.00%	13.262%
26	5.492	1366	1369	1370	rBV2	1516	805	0.05%	0.007%
27	5.640	1400	1415	1440	rBV	452304	907958	59.96%	7.952%
28	5.916	1497	1501	1503	rBV4	2865	2541	0.17%	0.022%
29	6.029	1533	1536	1537	rVB3	1369	685	0.05%	0.006%
30	6.093	1543	1556	1575	rBV	338579	683388	45.13%	5.985%
31	6.203	1587	1590	1592	rBV4	1724	1421	0.09%	0.012%
32	6.341	1631	1633	1637	rVB5	1584	877	0.06%	0.008%
33	6.376	1642	1644	1651	rBV8	1249	1268	0.08%	0.011%
34	6.598	1711	1713	1717	rBV5	1403	869	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016526.D
 Acq On : 05 Jun 2020 11:23
 Operator : SY/MD
 Sample : L2836-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.646	1724	1728	1731	rBV6	2330	2050	0.14%	0.018%
36	6.730	1752	1754	1757	rBV4	1092	517	0.03%	0.005%
37	6.826	1782	1784	1787	rBV4	1125	670	0.04%	0.006%
38	7.006	1829	1840	1862	rBV	194167	343965	22.71%	3.012%
39	7.338	1931	1943	1960	rBV	698955	1193810	78.84%	10.455%
40	7.640	2027	2037	2057	rBV	134386	232837	15.38%	2.039%
41	7.891	2112	2115	2116	rBV3	1163	753	0.05%	0.007%
42	7.942	2129	2131	2134	rVB4	1994	935	0.06%	0.008%
43	7.968	2134	2139	2143	rBV6	2899	2796	0.18%	0.024%
44	7.987	2143	2145	2146	rBV2	1149	601	0.04%	0.005%
45	8.055	2165	2166	2167	rBV	1270	468	0.03%	0.004%
46	8.106	2172	2182	2212	rVV	449150	750180	49.54%	6.570%
47	8.781	2390	2392	2395	rBV4	1265	614	0.04%	0.005%
48	8.875	2408	2421	2439	rBV	680418	1092619	72.15%	9.569%
49	9.276	2544	2546	2548	rBV2	1148	494	0.03%	0.004%
50	9.408	2584	2587	2592	rVB7	1861	1631	0.11%	0.014%
51	9.440	2593	2597	2601	rBV6	1605	1466	0.10%	0.013%
52	9.460	2601	2603	2605	rBV4	1329	479	0.03%	0.004%
53	9.646	2658	2661	2662	rBV3	1243	610	0.04%	0.005%
54	9.765	2695	2698	2699	rBV3	1388	716	0.05%	0.006%
55	9.842	2720	2722	2723	rBV2	1124	599	0.04%	0.005%
56	9.871	2729	2731	2733	rVB3	1220	420	0.03%	0.004%
57	9.920	2744	2746	2748	rBV3	1008	431	0.03%	0.004%
58	10.010	2771	2774	2776	rBV3	1113	821	0.05%	0.007%
59	10.183	2826	2828	2831	rBV3	1714	1176	0.08%	0.010%
60	10.238	2833	2845	2862	rVV	457266	716088	47.29%	6.272%
61	10.338	2873	2876	2878	rBV4	1823	1189	0.08%	0.010%
62	10.547	2937	2941	2947	rBV9	1936	2344	0.15%	0.021%
63	10.688	2983	2985	2987	rBV2	1190	794	0.05%	0.007%
64	10.984	3075	3077	3081	rVB4	1392	811	0.05%	0.007%
65	11.032	3089	3092	3094	rBV4	1224	785	0.05%	0.007%
66	11.270	3155	3166	3186	rBV	685853	1045917	69.07%	9.160%
67	11.431	3214	3216	3218	rBV3	1485	621	0.04%	0.005%
68	11.505	3237	3239	3243	rVB5	1346	901	0.06%	0.008%
69	11.524	3243	3245	3246	rBV2	1255	649	0.04%	0.006%
70	11.601	3267	3269	3271	rBV2	826	516	0.03%	0.005%
71	11.646	3271	3283	3300	rVV	725041	1136922	75.08%	9.957%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016526.D
 Acq On : 05 Jun 2020 11:23
 Operator : SY/MD
 Sample : L2836-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.759	3314	3318	3321	rBV6	1221	1037	0.07%	0.009%
73	12.035	3402	3404	3406	rBV3	1110	413	0.03%	0.004%
74	12.077	3414	3417	3419	rBV3	881	521	0.03%	0.005%
75	12.119	3427	3430	3432	rBV2	1859	1042	0.07%	0.009%
76	12.183	3449	3450	3453	rBV3	951	475	0.03%	0.004%
77	12.225	3461	3463	3465	rBV3	914	468	0.03%	0.004%
78	12.273	3474	3478	3481	rBV4	1393	1269	0.08%	0.011%
79	12.505	3547	3550	3551	rBV3	1692	843	0.06%	0.007%
80	12.595	3574	3578	3581	rBV6	1133	822	0.05%	0.007%
81	12.736	3619	3622	3625	rBV4	1361	1122	0.07%	0.010%
82	12.839	3652	3654	3656	rBV3	1019	472	0.03%	0.004%
83	12.887	3667	3669	3672	rBV	1036	429	0.03%	0.004%
84	12.907	3672	3675	3679	rVB4	1905	1355	0.09%	0.012%
85	12.929	3679	3682	3684	rBV3	1390	857	0.06%	0.008%
86	13.035	3712	3715	3717	rBV4	785	578	0.04%	0.005%
87	13.099	3734	3735	3737	rBV2	1016	490	0.03%	0.004%
88	13.189	3762	3763	3767	rVB3	1632	924	0.06%	0.008%
89	13.209	3767	3769	3773	rVB3	1385	924	0.06%	0.008%
90	13.254	3782	3783	3786	rBV3	820	413	0.03%	0.004%
91	13.360	3813	3816	3821	rBV5	1886	1111	0.07%	0.010%
92	13.460	3844	3847	3848	rBV2	1145	523	0.03%	0.005%
93	13.469	3848	3850	3851	rBV2	1278	622	0.04%	0.005%
94	13.530	3863	3869	3874	rBV8	3913	5567	0.37%	0.049%
95	13.607	3891	3893	3896	rBV3	1469	866	0.06%	0.008%
96	13.659	3907	3909	3911	rVB2	1277	522	0.03%	0.005%
97	14.125	4051	4054	4057	rVV4	1353	798	0.05%	0.007%
98	14.543	4180	4184	4185	rBV2	1873	1375	0.09%	0.012%
99	14.710	4234	4236	4237	rBV2	1317	478	0.03%	0.004%
100	15.164	4375	4377	4378	rBV2	1463	575	0.04%	0.005%


Sum of corrected areas: 11418084

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016526.D
Acq On : 05 Jun 2020 11:23
Operator : SY/MD
Sample : L2836-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

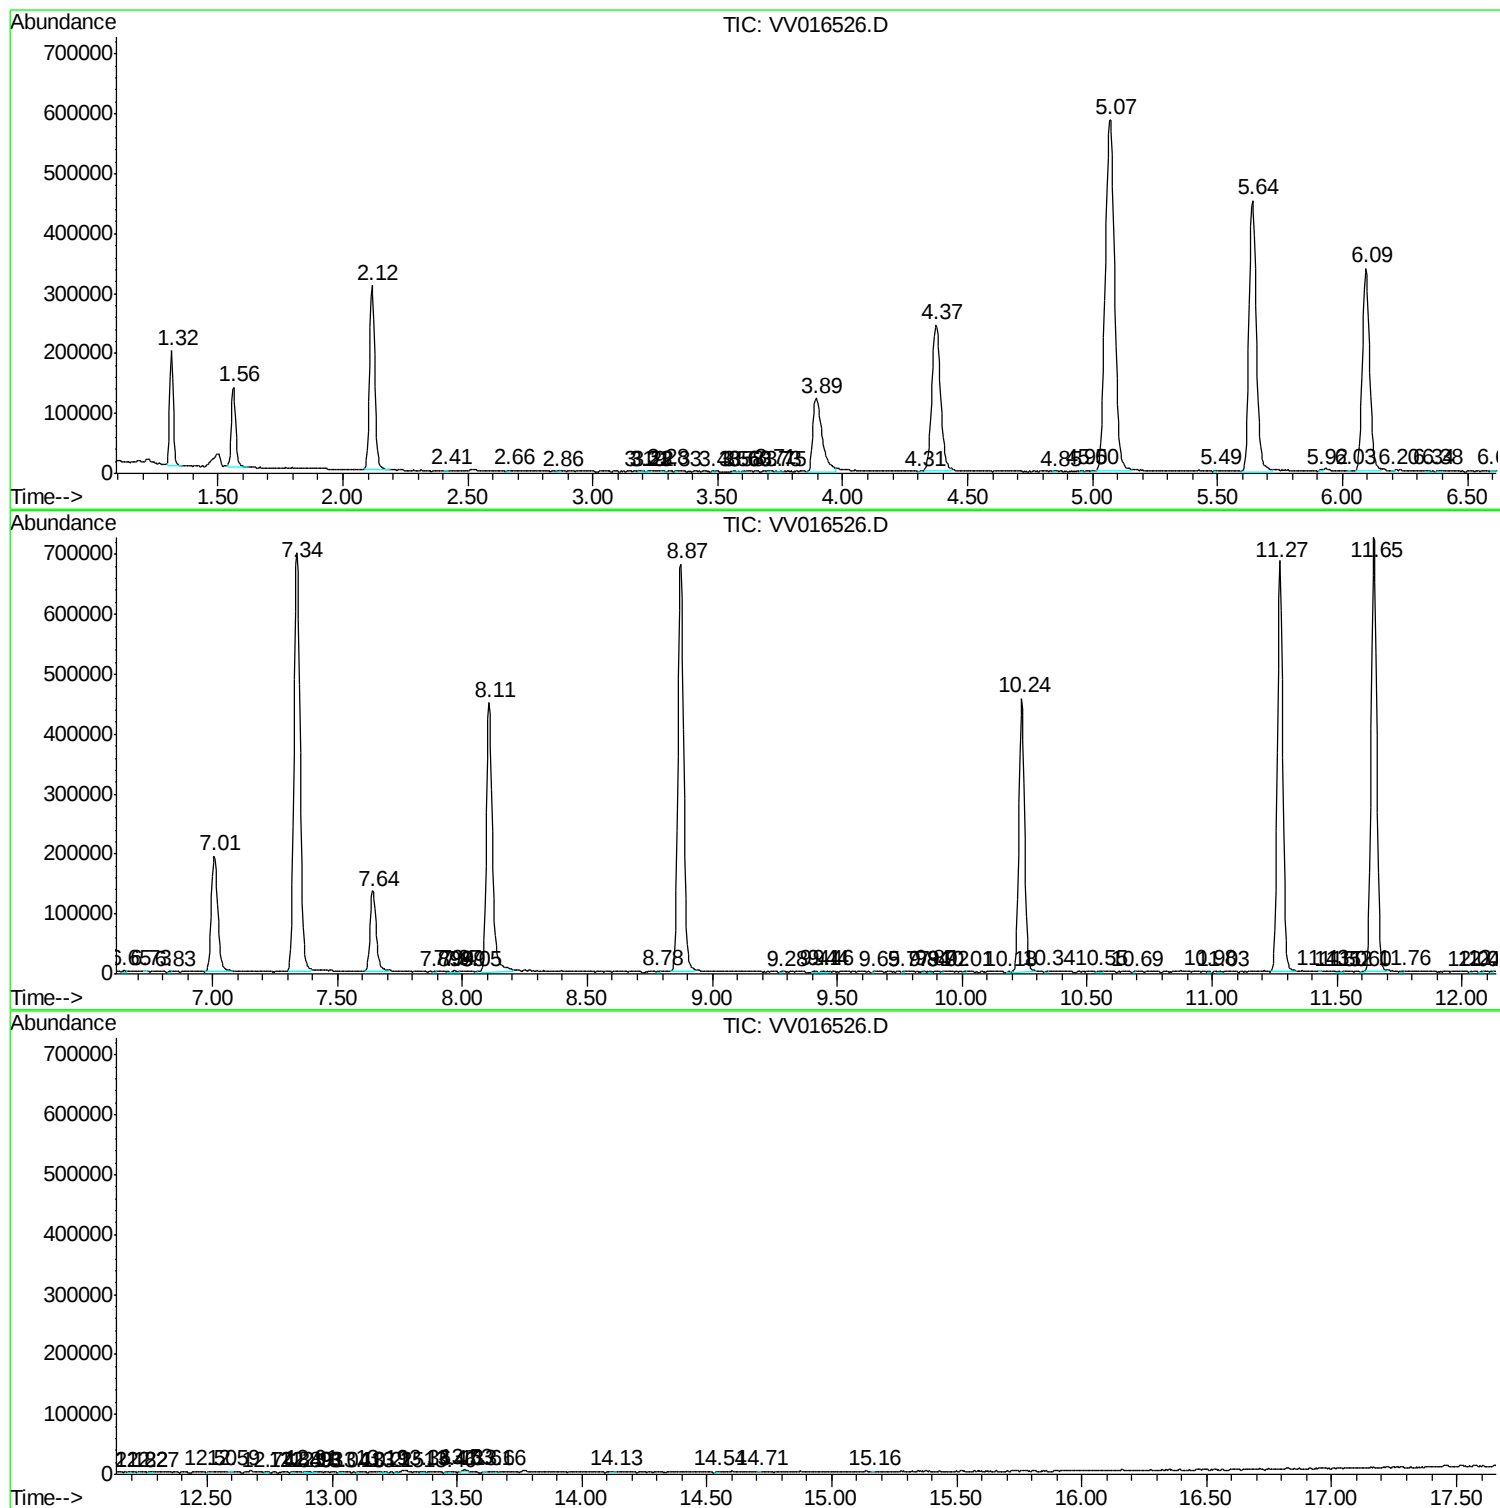

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016526.D
Acq On : 05 Jun 2020 11:23
Operator : SY/MD
Sample : L2836-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016526.D
Acq On : 05 Jun 2020 11:23
Operator : SY/MD
Sample : L2836-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
