

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016527.D
 Acq On : 05 Jun 2020 11:45
 Operator : SY/MD
 Sample : L2844-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	79	rVB	180500	182031	12.41%	1.631%
2	1.566	141	148	158	rVB	124105	148781	10.15%	1.333%
3	2.119	310	320	340	rVB	289947	443811	30.26%	3.976%
4	2.296	372	375	381	rBV7	2501	2356	0.16%	0.021%
5	2.470	428	429	432	rVB2	1511	771	0.05%	0.007%
6	2.524	439	446	455	rBV10	4201	7240	0.49%	0.065%
7	2.952	577	579	582	rVB4	1348	745	0.05%	0.007%
8	3.016	596	599	600	rBV2	1061	585	0.04%	0.005%
9	3.344	696	701	703	rBV6	1511	1453	0.10%	0.013%
10	3.470	738	740	745	rVB5	1560	1193	0.08%	0.011%
11	3.505	749	751	756	rBV5	864	852	0.06%	0.008%
12	3.720	815	818	820	rBV4	1199	934	0.06%	0.008%
13	3.756	827	829	833	rBV3	1079	569	0.04%	0.005%
14	3.814	845	847	852	rVB6	1503	873	0.06%	0.008%
15	3.839	852	855	859	rBV3	1145	1077	0.07%	0.010%
16	3.897	863	873	898	rVV	111475	293755	20.03%	2.632%
17	4.193	963	965	966	rBV2	1201	549	0.04%	0.005%
18	4.216	970	972	975	rVV4	1249	632	0.04%	0.006%
19	4.376	1007	1022	1044	rBV	233789	562404	38.35%	5.038%
20	4.534	1068	1071	1075	rBV5	1236	974	0.07%	0.009%
21	4.595	1086	1090	1093	rBV6	1131	1198	0.08%	0.011%
22	4.836	1161	1165	1169	rBV6	1908	2115	0.14%	0.019%
23	4.881	1176	1179	1183	rBV5	1468	1119	0.08%	0.010%
24	4.913	1186	1189	1190	rBV3	1437	714	0.05%	0.006%
25	4.981	1208	1210	1212	rBV3	1327	625	0.04%	0.006%
26	4.994	1212	1214	1220	rVB5	1132	633	0.04%	0.006%
27	5.071	1220	1238	1262	rBV2	571310	1466431	100.00%	13.137%
28	5.470	1360	1362	1365	rBV3	953	713	0.05%	0.006%
29	5.515	1373	1376	1378	rBV3	1334	828	0.06%	0.007%
30	5.540	1382	1384	1387	rBV3	1648	1187	0.08%	0.011%
31	5.640	1403	1415	1440	rBV	452277	899754	61.36%	8.061%
32	5.855	1480	1482	1485	rBV3	1382	649	0.04%	0.006%
33	5.872	1485	1487	1488	rBV2	1158	602	0.04%	0.005%
34	5.917	1498	1501	1502	rBV3	2307	1399	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016527.D
 Acq On : 05 Jun 2020 11:45
 Operator : SY/MD
 Sample : L2844-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.093	1543	1556	1583	rBV	327961	661409	45.10%	5.925%
36	6.341	1630	1633	1635	rBV3	930	650	0.04%	0.006%
37	6.460	1667	1670	1674	rVB5	1418	888	0.06%	0.008%
38	6.592	1709	1711	1714	rVB4	1505	670	0.05%	0.006%
39	6.627	1714	1722	1723	rBV8	2297	2335	0.16%	0.021%
40	6.814	1777	1780	1783	rBV5	905	617	0.04%	0.006%
41	6.849	1789	1791	1794	rVB3	1641	720	0.05%	0.006%
42	6.900	1805	1807	1810	rBV3	1373	825	0.06%	0.007%
43	7.010	1829	1841	1859	rBV	185639	333666	22.75%	2.989%
44	7.338	1931	1943	1960	rBV	689278	1166372	79.54%	10.449%
45	7.643	2028	2038	2054	rBV	129896	217092	14.80%	1.945%
46	7.791	2082	2084	2088	rBV5	1519	989	0.07%	0.009%
47	8.106	2171	2182	2207	rBV	426740	712295	48.57%	6.381%
48	8.553	2317	2321	2322	rBV4	1130	700	0.05%	0.006%
49	8.765	2384	2387	2389	rBV3	840	599	0.04%	0.005%
50	8.875	2409	2421	2446	rBV	685975	1107269	75.51%	9.920%
51	9.135	2499	2502	2504	rBV2	1354	985	0.07%	0.009%
52	9.293	2549	2551	2554	rBV4	1176	584	0.04%	0.005%
53	9.347	2566	2568	2574	rBV6	1351	1220	0.08%	0.011%
54	9.662	2662	2666	2668	rBV4	2031	1455	0.10%	0.013%
55	9.752	2692	2694	2696	rBV2	1601	1036	0.07%	0.009%
56	9.794	2704	2707	2710	rBV4	1303	1080	0.07%	0.010%
57	9.846	2719	2723	2724	rBV3	1998	1311	0.09%	0.012%
58	9.913	2742	2744	2750	rVB7	905	627	0.04%	0.006%
59	9.952	2750	2756	2760	rBV8	3678	4045	0.28%	0.036%
60	10.084	2793	2797	2805	rBV9	1438	1726	0.12%	0.015%
61	10.119	2805	2808	2810	rVB3	1342	816	0.06%	0.007%
62	10.238	2834	2845	2860	rBV	441966	685555	46.75%	6.142%
63	10.482	2918	2921	2923	rBV3	999	646	0.04%	0.006%
64	10.508	2927	2929	2931	rBV3	1329	675	0.05%	0.006%
65	10.637	2967	2969	2971	rBV3	1301	772	0.05%	0.007%
66	10.849	3033	3035	3038	rVB4	1215	583	0.04%	0.005%
67	10.926	3056	3059	3060	rBV2	1371	869	0.06%	0.008%
68	10.981	3072	3076	3078	rBV4	1892	1615	0.11%	0.014%
69	11.080	3105	3107	3110	rVB5	1179	617	0.04%	0.006%
70	11.270	3154	3166	3187	rBV	700656	1069665	72.94%	9.583%
71	11.582	3261	3263	3268	rVB5	2639	1825	0.12%	0.016%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016527.D
 Acq On : 05 Jun 2020 11:45
 Operator : SY/MD
 Sample : L2844-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.646	3268	3283	3298	rBV	716005	1120461	76.41%	10.038%
73	11.852	3345	3347	3348	rBV2	1191	574	0.04%	0.005%
74	12.003	3392	3394	3398	rVB5	1671	962	0.07%	0.009%
75	12.026	3399	3401	3408	rVB6	1758	1643	0.11%	0.015%
76	12.061	3408	3412	3413	rBV4	1330	835	0.06%	0.007%
77	12.100	3422	3424	3427	rBV4	1186	668	0.05%	0.006%
78	12.157	3438	3442	3446	rBV4	974	978	0.07%	0.009%
79	12.177	3446	3448	3451	rVB3	1856	932	0.06%	0.008%
80	12.238	3461	3467	3468	rBV4	1003	839	0.06%	0.008%
81	12.315	3487	3491	3493	rBV5	874	595	0.04%	0.005%
82	12.563	3566	3568	3570	rBV3	1696	825	0.06%	0.007%
83	12.727	3615	3619	3621	rBV4	1471	1219	0.08%	0.011%
84	12.768	3629	3632	3633	rBV3	853	584	0.04%	0.005%
85	12.833	3649	3652	3658	rVB7	1614	1482	0.10%	0.013%
86	12.871	3661	3664	3666	rBV4	1189	764	0.05%	0.007%
87	13.003	3702	3705	3709	rBV4	1996	1445	0.10%	0.013%
88	13.029	3709	3713	3716	rVB5	1547	978	0.07%	0.009%
89	13.109	3736	3738	3740	rBV3	969	599	0.04%	0.005%
90	13.238	3775	3778	3785	rBV7	1122	1187	0.08%	0.011%
91	13.280	3786	3791	3795	rBV7	3402	3764	0.26%	0.034%
92	13.585	3883	3886	3889	rVB5	1276	719	0.05%	0.006%
93	13.604	3889	3892	3893	rBV3	1564	703	0.05%	0.006%
94	13.649	3904	3906	3908	rBV3	872	562	0.04%	0.005%
95	13.759	3938	3940	3942	rBV2	1374	734	0.05%	0.007%
96	13.955	3998	4001	4005	rVB5	1491	996	0.07%	0.009%
97	14.032	4022	4025	4027	rBV4	1217	662	0.05%	0.006%
98	14.132	4054	4056	4058	rBV3	1215	623	0.04%	0.006%
99	14.341	4118	4121	4123	rBV4	1227	744	0.05%	0.007%
100	14.392	4135	4137	4141	rBV4	1158	761	0.05%	0.007%


Sum of corrected areas: 11162193

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016527.D
Acq On : 05 Jun 2020 11:45
Operator : SY/MD
Sample : L2844-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

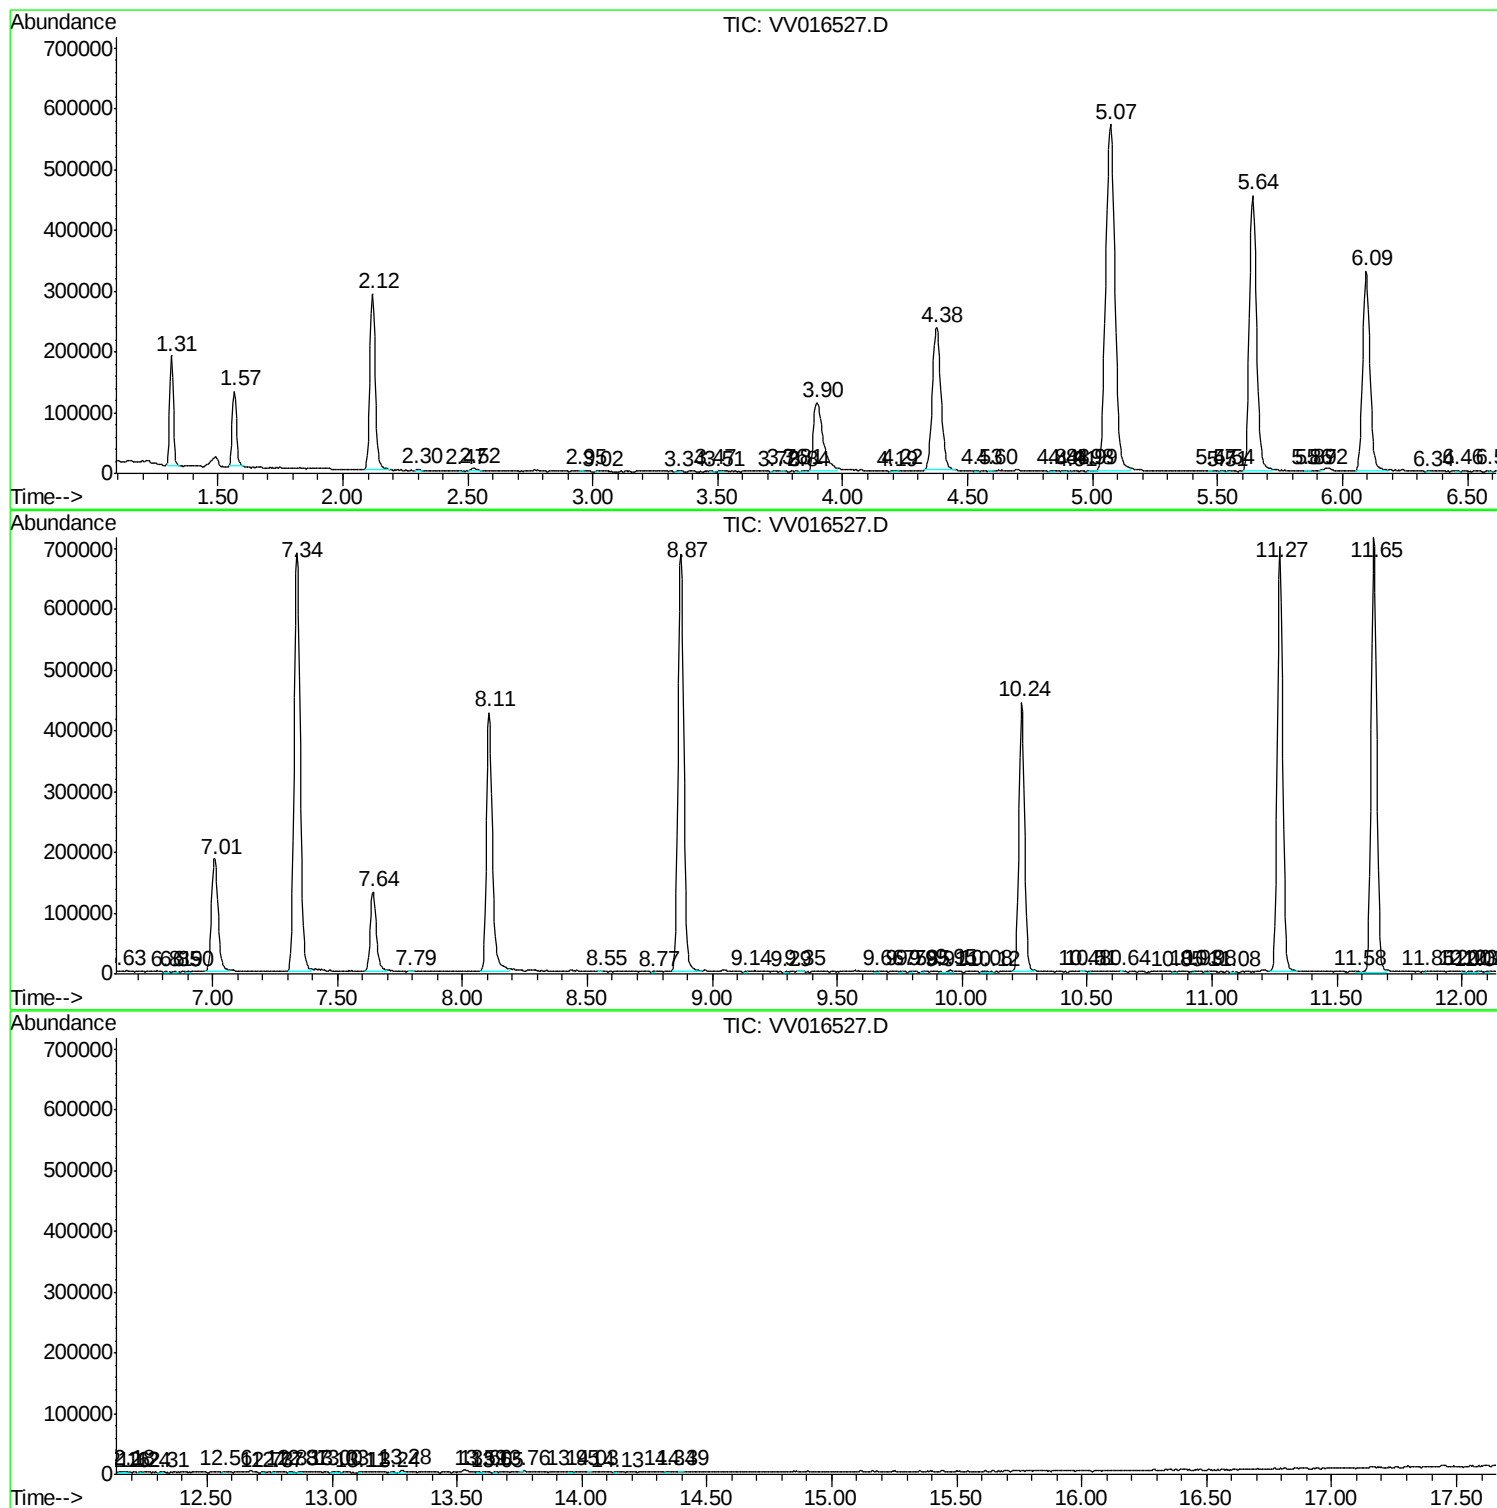

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016527.D
Acq On : 05 Jun 2020 11:45
Operator : SY/MD
Sample : L2844-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016527.D
Acq On : 05 Jun 2020 11:45
Operator : SY/MD
Sample : L2844-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc