

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016528.D
 Acq On : 05 Jun 2020 12:09
 Operator : SY/MD
 Sample : L2868-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	85	rVB	186116	188837	13.07%	1.726%
2	1.563	140	147	163	rVB	128290	157916	10.93%	1.443%
3	2.116	310	319	342	rVB	295433	445196	30.80%	4.068%
4	2.489	433	435	437	rBV3	1149	498	0.03%	0.005%
5	2.740	510	513	517	rBV6	1316	1079	0.07%	0.010%
6	2.904	561	564	565	rBV3	740	365	0.03%	0.003%
7	2.949	577	578	579	rBV	1160	430	0.03%	0.004%
8	3.132	633	635	638	rVB4	1295	642	0.04%	0.006%
9	3.319	691	693	696	rBV4	749	518	0.04%	0.005%
10	3.335	696	698	701	rVV4	1093	568	0.04%	0.005%
11	3.386	711	714	717	rBV5	1166	880	0.06%	0.008%
12	3.431	726	728	729	rBV2	930	314	0.02%	0.003%
13	3.473	739	741	743	rBV3	949	449	0.03%	0.004%
14	3.524	754	757	760	rBV4	1813	1466	0.10%	0.013%
15	3.630	788	790	791	rBV2	1195	493	0.03%	0.005%
16	3.708	810	814	817	rVB4	1456	1039	0.07%	0.009%
17	3.733	820	822	825	rVV3	1270	940	0.07%	0.009%
18	3.765	829	832	834	rBV3	980	510	0.04%	0.005%
19	3.778	834	836	838	rBV3	869	416	0.03%	0.004%
20	3.791	838	840	844	rVB5	1448	793	0.05%	0.007%
21	3.827	849	851	853	rVB3	1057	325	0.02%	0.003%
22	3.839	853	855	856	rBV2	1629	694	0.05%	0.006%
23	3.894	862	872	902	rBV	111762	302607	20.94%	2.765%
24	4.203	966	968	969	rBV2	768	305	0.02%	0.003%
25	4.373	1007	1021	1042	rVB	229382	544415	37.67%	4.975%
26	4.592	1087	1089	1094	rBV5	1864	1219	0.08%	0.011%
27	5.071	1218	1238	1261	rBV2	558819	1445325	100.00%	13.208%
28	5.470	1360	1362	1366	rVB4	2326	1575	0.11%	0.014%
29	5.502	1366	1372	1373	rBV5	2522	2609	0.18%	0.024%
30	5.540	1378	1384	1387	rVV8	1895	1953	0.14%	0.018%
31	5.640	1403	1415	1436	rBV	442272	870182	60.21%	7.952%
32	6.093	1544	1556	1579	rVB	318881	637420	44.10%	5.825%
33	6.421	1656	1658	1664	rVB6	1591	1493	0.10%	0.014%
34	6.598	1711	1713	1714	rBV	874	334	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016528.D
 Acq On : 05 Jun 2020 12:09
 Operator : SY/MD
 Sample : L2868-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.621	1718	1720	1722	rBV2	1030	585	0.04%	0.005%
36	6.817	1780	1781	1782	rBV	859	304	0.02%	0.003%
37	7.006	1829	1840	1855	rBV	181818	322021	22.28%	2.943%
38	7.129	1876	1878	1885	rVB7	2139	1632	0.11%	0.015%
39	7.338	1928	1943	1961	rBV	672008	1153647	79.82%	10.542%
40	7.547	2006	2008	2010	rBV3	1186	591	0.04%	0.005%
41	7.608	2022	2027	2028	rBV5	2088	1833	0.13%	0.017%
42	7.640	2028	2037	2053	rVV2	128404	215403	14.90%	1.968%
43	7.826	2094	2095	2097	rBV2	1098	339	0.02%	0.003%
44	7.907	2116	2120	2121	rBV5	1515	1182	0.08%	0.011%
45	8.064	2167	2169	2171	rBV4	943	598	0.04%	0.005%
46	8.106	2172	2182	2205	rVV	416435	705483	48.81%	6.447%
47	8.511	2307	2308	2312	rVB4	1422	558	0.04%	0.005%
48	8.714	2369	2371	2373	rBV3	949	524	0.04%	0.005%
49	8.807	2397	2400	2403	rBV5	1483	1154	0.08%	0.011%
50	8.875	2408	2421	2442	rBV	662541	1082359	74.89%	9.891%
51	9.161	2508	2510	2513	rBV3	2539	1454	0.10%	0.013%
52	9.344	2563	2567	2570	rBV4	1497	1214	0.08%	0.011%
53	9.412	2585	2588	2590	rBV3	1066	667	0.05%	0.006%
54	9.440	2595	2597	2599	rBV3	1165	619	0.04%	0.006%
55	9.514	2617	2620	2621	rBV3	864	403	0.03%	0.004%
56	9.807	2708	2711	2715	rBV4	1884	1694	0.12%	0.015%
57	9.871	2729	2731	2734	rVV4	1107	516	0.04%	0.005%
58	9.897	2737	2739	2743	rBV3	1323	605	0.04%	0.006%
59	10.112	2802	2806	2808	rBV3	1459	899	0.06%	0.008%
60	10.238	2831	2845	2860	rBV	436173	684295	47.35%	6.253%
61	10.929	3056	3060	3062	rBV4	1805	1497	0.10%	0.014%
62	11.051	3095	3098	3100	rBV4	1648	817	0.06%	0.007%
63	11.090	3108	3110	3111	rBV2	695	303	0.02%	0.003%
64	11.116	3116	3118	3122	rVB4	1276	747	0.05%	0.007%
65	11.270	3155	3166	3189	rBV	678153	1043393	72.19%	9.535%
66	11.485	3231	3233	3234	rBV2	951	271	0.02%	0.002%
67	11.511	3239	3241	3243	rVB	1089	388	0.03%	0.004%
68	11.547	3250	3252	3254	rBV3	926	380	0.03%	0.003%
69	11.646	3272	3283	3301	rBV	693935	1078314	74.61%	9.854%
70	11.781	3322	3325	3327	rBV3	1686	947	0.07%	0.009%
71	11.836	3339	3342	3345	rBV4	1421	991	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016528.D
 Acq On : 05 Jun 2020 12:09
 Operator : SY/MD
 Sample : L2868-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.910	3363	3365	3367	rBV3	959	521	0.04%	0.005%
73	12.003	3391	3394	3397	rBV3	1230	782	0.05%	0.007%
74	12.055	3408	3410	3413	rBV4	1173	439	0.03%	0.004%
75	12.157	3440	3442	3444	rBV3	909	386	0.03%	0.004%
76	12.264	3472	3475	3476	rBV3	1624	1061	0.07%	0.010%
77	12.321	3491	3493	3494	rBV2	1353	542	0.04%	0.005%
78	12.485	3542	3544	3547	rBV2	1459	971	0.07%	0.009%
79	12.620	3584	3586	3587	rBV2	1575	594	0.04%	0.005%
80	12.733	3618	3621	3625	rBV4	1601	962	0.07%	0.009%
81	12.855	3657	3659	3661	rBV3	2471	1234	0.09%	0.011%
82	13.093	3731	3733	3737	rVB4	1743	1023	0.07%	0.009%
83	13.167	3754	3756	3758	rBV	864	445	0.03%	0.004%
84	13.180	3758	3760	3762	rBV3	885	466	0.03%	0.004%
85	13.193	3762	3764	3767	rBV5	1391	915	0.06%	0.008%
86	13.231	3772	3776	3777	rBV3	1437	815	0.06%	0.007%
87	13.611	3891	3894	3898	rBV5	1213	854	0.06%	0.008%
88	13.942	3995	3997	4000	rBV4	1540	1061	0.07%	0.010%
89	13.997	4012	4014	4016	rBV2	915	459	0.03%	0.004%
90	14.061	4032	4034	4037	rBV2	1056	531	0.04%	0.005%
91	14.196	4073	4076	4077	rBV2	1162	571	0.04%	0.005%
92	14.398	4136	4139	4143	rVB5	2667	1842	0.13%	0.017%
93	14.633	4210	4212	4214	rBV3	1122	653	0.05%	0.006%
94	14.707	4233	4235	4238	rVB4	1352	531	0.04%	0.005%
95	14.726	4238	4241	4245	rBV3	1442	1528	0.11%	0.014%
96	15.029	4331	4335	4336	rBV4	1550	1273	0.09%	0.012%


Sum of corrected areas: 10942891

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016528.D
Acq On : 05 Jun 2020 12:09
Operator : SY/MD
Sample : L2868-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

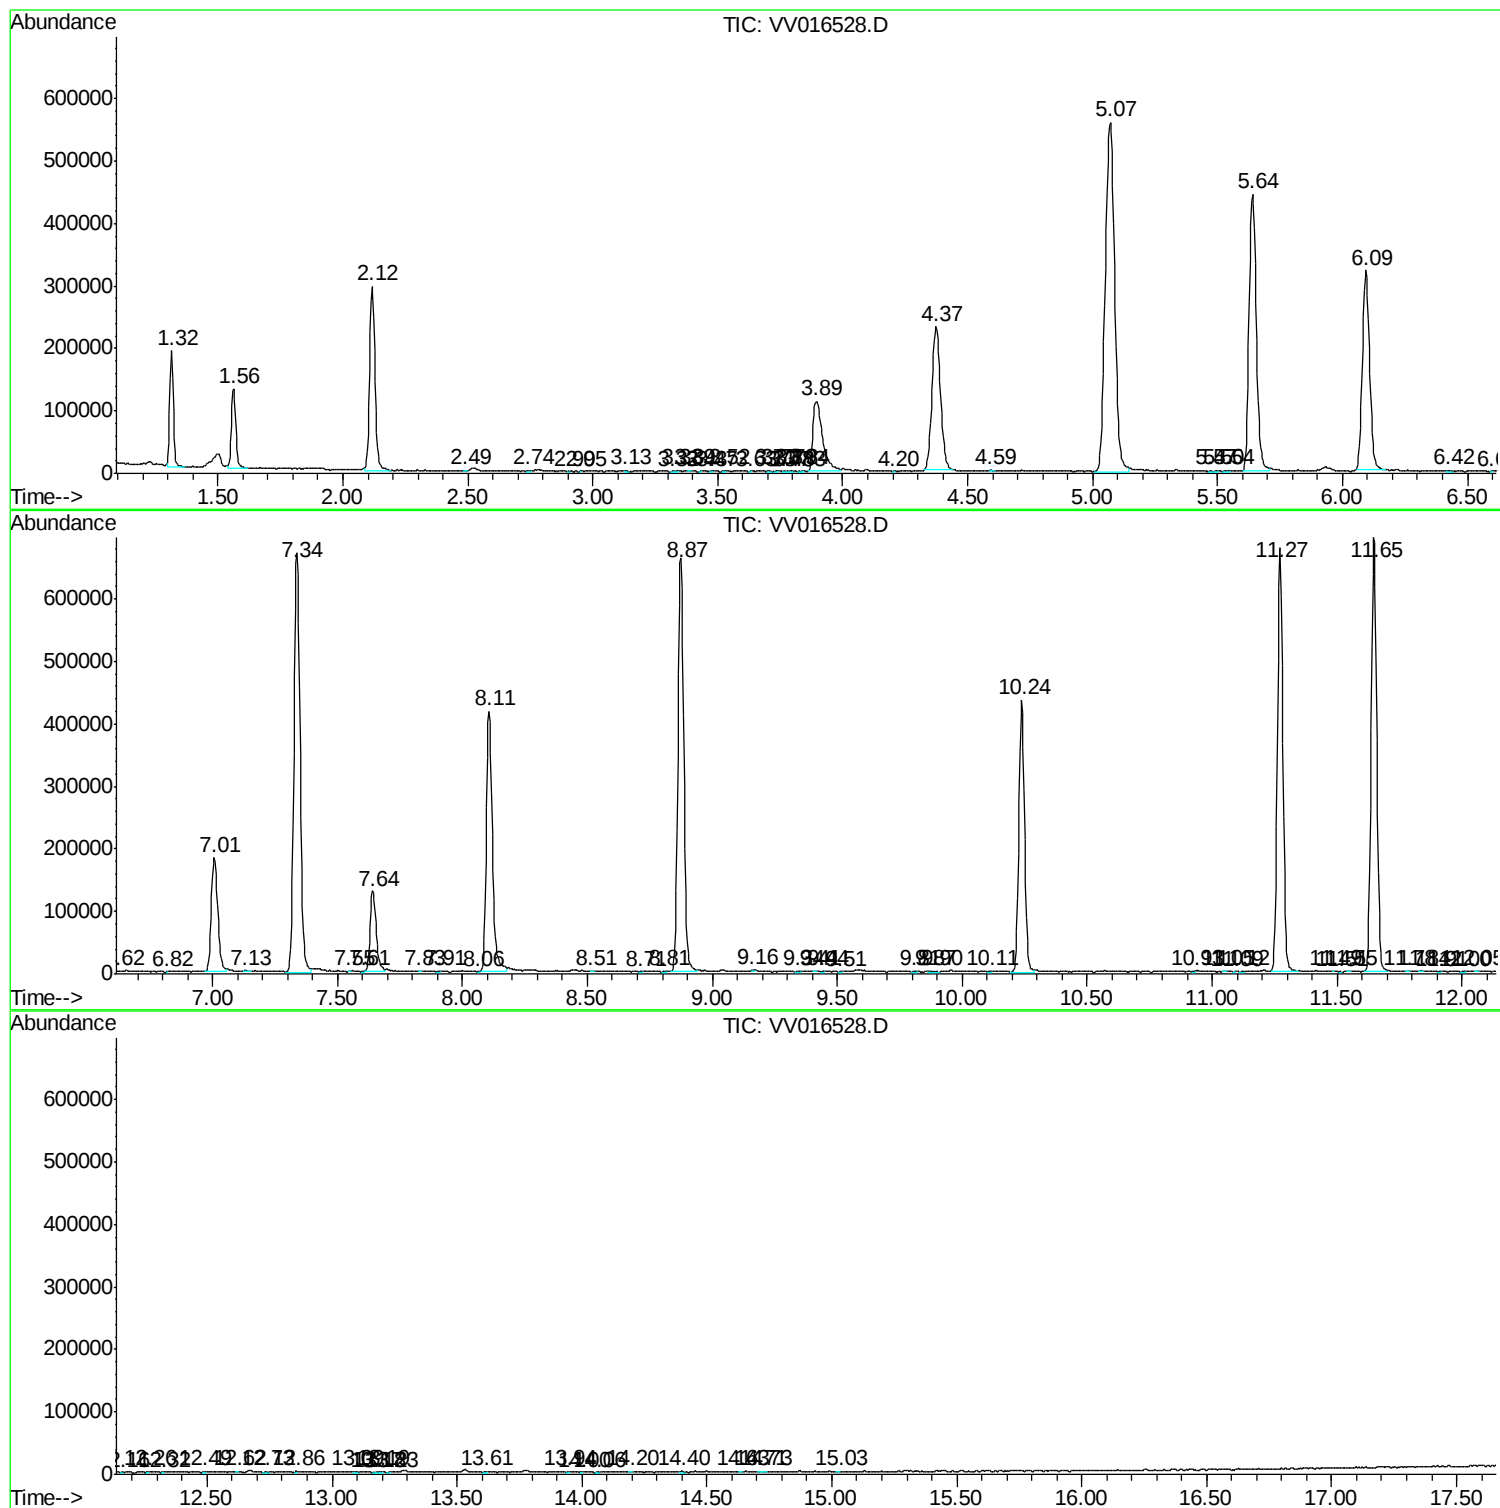

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016528.D
Acq On : 05 Jun 2020 12:09
Operator : SY/MD
Sample : L2868-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016528.D
Acq On : 05 Jun 2020 12:09
Operator : SY/MD
Sample : L2868-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc