

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016531.D
 Acq On : 05 Jun 2020 13:21
 Operator : SY/MD
 Sample : L2861-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	81	rVB	186965	183366	13.50%	1.729%
2	1.560	140	146	164	rVB	123128	152800	11.25%	1.441%
3	2.116	309	319	334	rBV	280528	417711	30.76%	3.939%
4	2.505	438	440	441	rBV3	1459	628	0.05%	0.006%
5	2.833	539	542	544	rBV4	1824	838	0.06%	0.008%
6	2.946	574	577	578	rBV3	1133	667	0.05%	0.006%
7	2.975	584	586	593	rVB6	1777	1601	0.12%	0.015%
8	3.007	593	596	599	rBV5	1629	1130	0.08%	0.011%
9	3.042	604	607	608	rBV3	1036	591	0.04%	0.006%
10	3.168	643	646	649	rBV4	1922	1339	0.10%	0.013%
11	3.364	703	707	713	rBV6	1646	1651	0.12%	0.016%
12	3.460	735	737	739	rBV3	1201	609	0.04%	0.006%
13	3.479	739	743	747	rVB5	1175	897	0.07%	0.008%
14	3.508	749	752	755	rVB5	1037	678	0.05%	0.006%
15	3.550	763	765	766	rBV2	1253	600	0.04%	0.006%
16	3.576	771	773	778	rVB5	823	604	0.04%	0.006%
17	3.611	781	784	786	rBV4	1054	807	0.06%	0.008%
18	3.711	812	815	819	rBV4	1309	1204	0.09%	0.011%
19	3.788	837	839	841	rVB3	1376	595	0.04%	0.006%
20	3.894	862	872	902	rBV	103304	275018	20.25%	2.593%
21	4.286	991	994	995	rBV2	1210	690	0.05%	0.007%
22	4.373	1004	1021	1042	rBV	217656	533348	39.27%	5.029%
23	4.489	1055	1057	1059	rBV3	1754	823	0.06%	0.008%
24	4.846	1167	1168	1170	rBV2	1304	670	0.05%	0.006%
25	4.958	1201	1203	1208	rVB4	1333	883	0.07%	0.008%
26	5.013	1217	1220	1221	rBV2	1068	623	0.05%	0.006%
27	5.071	1221	1238	1259	rBV2	531784	1358019	100.00%	12.806%
28	5.640	1402	1415	1437	rBV	470828	935182	68.86%	8.818%
29	5.833	1472	1475	1478	rVB3	1766	1208	0.09%	0.011%
30	5.856	1478	1482	1484	rBV5	1230	912	0.07%	0.009%
31	5.987	1521	1523	1525	rBV3	1633	788	0.06%	0.007%
32	6.093	1544	1556	1579	rVB	300730	601579	44.30%	5.673%
33	6.553	1696	1699	1701	rBV3	1254	835	0.06%	0.008%
34	6.621	1718	1720	1722	rBV3	1474	796	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016531.D
 Acq On : 05 Jun 2020 13:21
 Operator : SY/MD
 Sample : L2861-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.804	1775	1777	1779	rBV2	1043	686	0.05%	0.006%
36	7.007	1830	1840	1866	rVB	159751	282912	20.83%	2.668%
37	7.235	1906	1911	1914	rBV7	1514	1445	0.11%	0.014%
38	7.338	1931	1943	1962	rBV	625011	1072810	79.00%	10.116%
39	7.643	2028	2038	2055	rBV	111566	192677	14.19%	1.817%
40	7.878	2107	2111	2112	rBV3	1018	746	0.05%	0.007%
41	7.891	2113	2115	2118	rVB4	1524	706	0.05%	0.007%
42	8.003	2146	2150	2155	rVB7	2358	2354	0.17%	0.022%
43	8.106	2171	2182	2215	rBV	381700	664878	48.96%	6.270%
44	8.646	2347	2350	2351	rBV2	1389	804	0.06%	0.008%
45	8.704	2365	2368	2372	rVB6	1854	1223	0.09%	0.012%
46	8.727	2372	2375	2377	rBV4	1213	745	0.05%	0.007%
47	8.778	2388	2391	2393	rBV3	1122	619	0.05%	0.006%
48	8.875	2410	2421	2435	rBV	696665	1118487	82.36%	10.547%
49	9.154	2504	2508	2510	rBV4	1086	802	0.06%	0.008%
50	9.167	2510	2512	2516	rVV4	1650	1200	0.09%	0.011%
51	9.196	2519	2521	2526	rVB4	1037	836	0.06%	0.008%
52	9.219	2526	2528	2532	rVB4	1873	1142	0.08%	0.011%
53	9.238	2532	2534	2538	rVB5	1474	988	0.07%	0.009%
54	9.261	2538	2541	2542	rBV3	1474	967	0.07%	0.009%
55	9.354	2567	2570	2572	rBV4	881	723	0.05%	0.007%
56	9.598	2643	2646	2648	rBV3	1525	963	0.07%	0.009%
57	9.704	2677	2679	2681	rBV4	1617	791	0.06%	0.007%
58	9.820	2712	2715	2716	rBV2	2077	1162	0.09%	0.011%
59	9.852	2723	2725	2730	rVB6	1589	993	0.07%	0.009%
60	9.936	2749	2751	2753	rBV2	1256	610	0.04%	0.006%
61	9.965	2753	2760	2763	rBV8	1531	1817	0.13%	0.017%
62	10.106	2801	2804	2808	rVB4	1742	1030	0.08%	0.010%
63	10.164	2821	2822	2826	rBV3	1339	996	0.07%	0.009%
64	10.238	2834	2845	2861	rVB	405324	621756	45.78%	5.863%
65	10.441	2904	2908	2913	rVB7	1770	1419	0.10%	0.013%
66	10.463	2913	2915	2920	rBV5	1504	1040	0.08%	0.010%
67	10.605	2957	2959	2964	rBV5	988	746	0.05%	0.007%
68	10.724	2994	2996	2997	rBV	1434	606	0.04%	0.006%
69	10.836	3027	3031	3033	rBV3	815	727	0.05%	0.007%
70	10.875	3040	3043	3045	rBV5	1419	1021	0.08%	0.010%
71	10.913	3053	3055	3059	rBV4	902	635	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016531.D
 Acq On : 05 Jun 2020 13:21
 Operator : SY/MD
 Sample : L2861-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.984	3074	3077	3081	rBV4	1572	1193	0.09%	0.011%
73	11.270	3154	3166	3185	rBV	712195	1095121	80.64%	10.327%
74	11.476	3228	3230	3234	rVB4	1682	692	0.05%	0.007%
75	11.592	3263	3266	3271	rBV7	1103	1051	0.08%	0.010%
76	11.646	3271	3283	3300	rBV	642708	1018822	75.02%	9.607%
77	12.019	3396	3399	3402	rBV4	1790	1160	0.09%	0.011%
78	12.058	3408	3411	3416	rBV6	1702	1819	0.13%	0.017%
79	12.222	3461	3462	3466	rBV4	1027	684	0.05%	0.006%
80	12.286	3479	3482	3484	rBV3	1992	1165	0.09%	0.011%
81	12.344	3497	3500	3503	rBV5	1357	847	0.06%	0.008%
82	12.428	3522	3526	3529	rBV2	1739	1604	0.12%	0.015%
83	12.646	3591	3594	3597	rVB4	1189	708	0.05%	0.007%
84	12.666	3598	3600	3602	rBV3	1203	715	0.05%	0.007%
85	12.801	3640	3642	3644	rBV3	1557	635	0.05%	0.006%
86	12.823	3646	3649	3651	rBV3	1003	627	0.05%	0.006%
87	12.842	3651	3655	3657	rBV2	1406	722	0.05%	0.007%
88	12.871	3661	3664	3667	rBV5	1643	1321	0.10%	0.012%
89	12.997	3700	3703	3705	rVB5	1203	611	0.04%	0.006%
90	13.010	3705	3707	3709	rBV3	1569	796	0.06%	0.008%
91	13.045	3715	3718	3721	rBV4	2125	1709	0.13%	0.016%
92	13.222	3768	3773	3775	rBV5	1454	1160	0.09%	0.011%
93	13.312	3799	3801	3805	rBV5	1608	1006	0.07%	0.009%
94	13.344	3808	3811	3813	rBV4	1368	646	0.05%	0.006%
95	13.392	3823	3826	3827	rBV2	1070	620	0.05%	0.006%
96	13.601	3888	3891	3896	rBV6	1731	1167	0.09%	0.011%
97	13.829	3958	3962	3965	rBV4	1439	918	0.07%	0.009%
98	13.920	3988	3990	3993	rVB2	1496	631	0.05%	0.006%
99	14.035	4024	4026	4030	rBV5	1781	1687	0.12%	0.016%
100	14.199	4074	4077	4079	rBV4	1886	1339	0.10%	0.013%


Sum of corrected areas: 10604928

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016531.D
Acq On : 05 Jun 2020 13:21
Operator : SY/MD
Sample : L2861-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

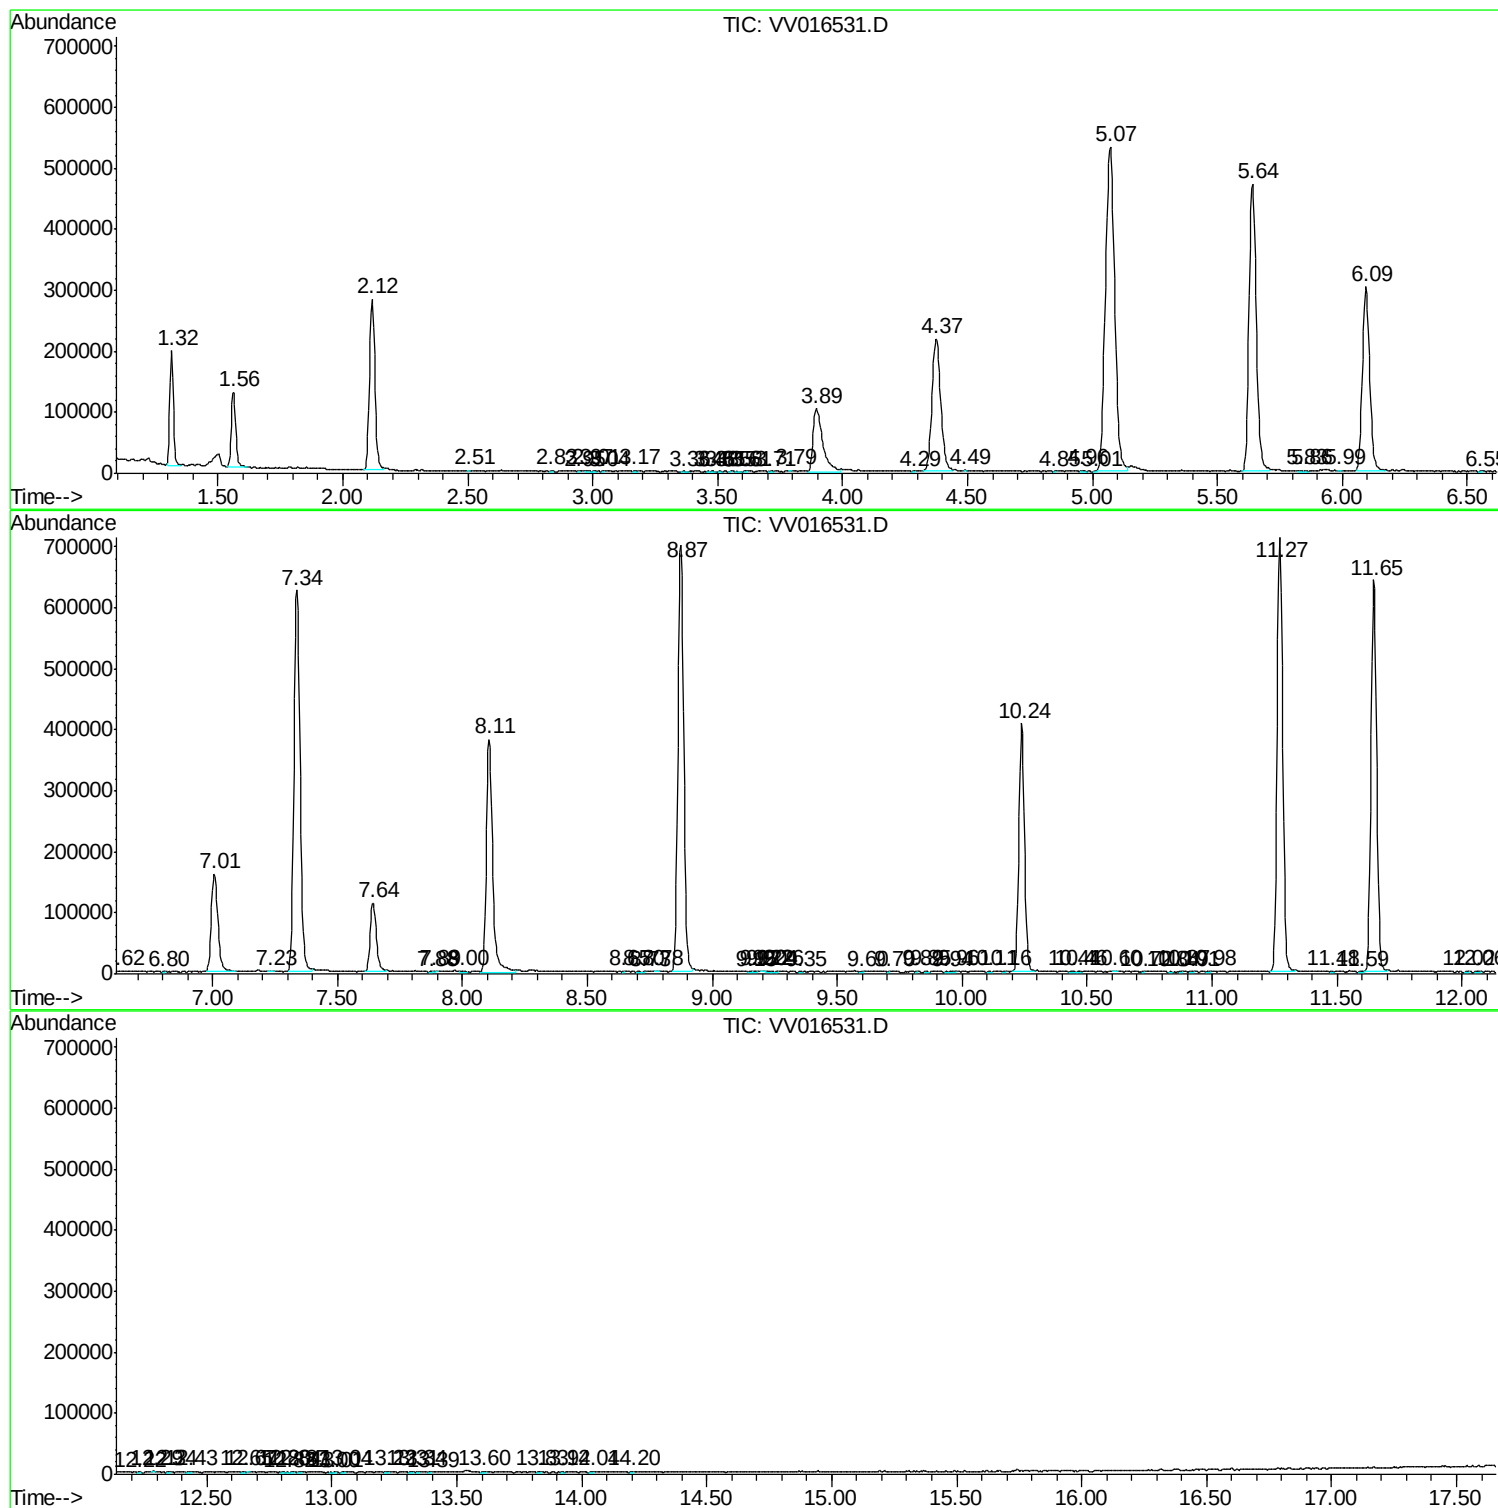

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016531.D
Acq On : 05 Jun 2020 13:21
Operator : SY/MD
Sample : L2861-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060520\
Data File : VV016531.D
Acq On : 05 Jun 2020 13:21
Operator : SY/MD
Sample : L2861-02
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
F9D76

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc