

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016532.D
 Acq On : 05 Jun 2020 13:44
 Operator : SY/MD
 Sample : L2848-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	86	rVB	164958	169705	12.21%	1.591%
2	1.560	139	146	157	rVB	126443	152018	10.94%	1.426%
3	2.116	310	319	332	rVB	251728	356118	25.63%	3.339%
4	2.489	433	435	436	rBV2	1356	668	0.05%	0.006%
5	2.560	454	457	459	rBV5	1320	872	0.06%	0.008%
6	2.978	585	587	591	rVB4	1666	1089	0.08%	0.010%
7	3.000	591	594	596	rBV3	1535	1079	0.08%	0.010%
8	3.093	621	623	626	rBV4	1373	931	0.07%	0.009%
9	3.138	633	637	638	rBV4	1285	682	0.05%	0.006%
10	3.187	649	652	653	rBV3	1190	692	0.05%	0.006%
11	3.264	670	676	680	rVB7	1517	1671	0.12%	0.016%
12	3.347	699	702	703	rBV3	1339	654	0.05%	0.006%
13	3.386	712	714	718	rBV3	1282	1045	0.08%	0.010%
14	3.540	759	762	763	rBV3	1447	632	0.05%	0.006%
15	3.643	791	794	797	rBV4	1059	769	0.06%	0.007%
16	3.772	830	834	836	rBV4	1235	887	0.06%	0.008%
17	3.843	853	856	859	rBV4	1139	693	0.05%	0.006%
18	3.897	862	873	904	rBV	120113	334468	24.07%	3.136%
19	4.196	964	966	970	rBV4	1133	670	0.05%	0.006%
20	4.373	1007	1021	1041	rVB	221305	532840	38.34%	4.997%
21	4.659	1108	1110	1114	rVB3	1735	940	0.07%	0.009%
22	4.785	1147	1149	1152	rVB4	1565	719	0.05%	0.007%
23	4.807	1152	1156	1158	rBV5	1600	1455	0.10%	0.014%
24	5.071	1217	1238	1264	rBV2	543602	1389687	100.00%	13.032%
25	5.585	1395	1398	1402	rBV6	1518	1426	0.10%	0.013%
26	5.640	1402	1415	1438	rBV	437922	874882	62.96%	8.204%
27	5.810	1464	1468	1469	rBV4	1634	997	0.07%	0.009%
28	5.926	1495	1504	1514	rBV4	7331	15913	1.15%	0.149%
29	6.093	1544	1556	1580	rVB	319727	640405	46.08%	6.005%
30	6.418	1656	1657	1662	rBV4	941	672	0.05%	0.006%
31	6.588	1708	1710	1713	rBV3	1426	930	0.07%	0.009%
32	6.839	1784	1788	1790	rBV6	1356	1180	0.08%	0.011%
33	6.958	1823	1825	1828	rBV3	913	604	0.04%	0.006%
34	7.006	1829	1840	1856	rVV	156922	278942	20.07%	2.616%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016532.D
 Acq On : 05 Jun 2020 13:44
 Operator : SY/MD
 Sample : L2848-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	7.338	1930	1943	1963	rBV	636475	1094581	78.76%	10.264%
36	7.531	2000	2003	2007	rBV5	1759	1535	0.11%	0.014%
37	7.643	2022	2038	2059	rBV	111782	199140	14.33%	1.867%
38	7.814	2087	2091	2092	rBV4	1190	778	0.06%	0.007%
39	7.897	2112	2117	2120	rBV6	1639	1605	0.12%	0.015%
40	8.071	2166	2171	2172	rBV4	1434	1082	0.08%	0.010%
41	8.106	2172	2182	2209	rBV	419953	701874	50.51%	6.582%
42	8.434	2279	2284	2286	rBV5	4690	4144	0.30%	0.039%
43	8.550	2317	2320	2321	rBV2	1711	859	0.06%	0.008%
44	8.627	2342	2344	2349	rBV4	778	602	0.04%	0.006%
45	8.646	2349	2350	2356	rVV4	935	695	0.05%	0.007%
46	8.714	2369	2371	2376	rVB4	2364	1694	0.12%	0.016%
47	8.736	2376	2378	2380	rBV3	1497	900	0.06%	0.008%
48	8.875	2409	2421	2440	rBV	661897	1061777	76.40%	9.957%
49	9.035	2468	2471	2473	rBV4	2399	1441	0.10%	0.014%
50	9.161	2506	2510	2511	rBV3	1863	1245	0.09%	0.012%
51	9.315	2553	2558	2564	rBV7	2339	2452	0.18%	0.023%
52	9.376	2574	2577	2579	rBV4	1302	930	0.07%	0.009%
53	9.502	2615	2616	2621	rBV4	1036	747	0.05%	0.007%
54	9.640	2656	2659	2661	rBV3	1376	970	0.07%	0.009%
55	9.682	2667	2672	2675	rBV6	1398	1482	0.11%	0.014%
56	9.717	2681	2683	2684	rBV2	1273	651	0.05%	0.006%
57	9.797	2706	2708	2711	rVB4	1189	662	0.05%	0.006%
58	9.833	2716	2719	2725	rBV7	1671	1765	0.13%	0.017%
59	9.993	2764	2769	2770	rBV4	1194	1041	0.07%	0.010%
60	10.090	2796	2799	2801	rBV3	1700	913	0.07%	0.009%
61	10.238	2833	2845	2859	rVV	441971	690765	49.71%	6.478%
62	10.360	2880	2883	2887	rVB4	1650	1220	0.09%	0.011%
63	10.524	2932	2934	2936	rVV3	1403	697	0.05%	0.007%
64	10.566	2945	2947	2950	rVB4	1635	798	0.06%	0.007%
65	10.637	2966	2969	2970	rBV3	1333	795	0.06%	0.007%
66	10.936	3060	3062	3064	rBV3	1114	700	0.05%	0.007%
67	11.048	3094	3097	3100	rVV4	916	675	0.05%	0.006%
68	11.164	3129	3133	3138	rBV7	1071	1248	0.09%	0.012%
69	11.202	3141	3145	3147	rBV4	1292	1285	0.09%	0.012%
70	11.270	3155	3166	3184	rBV	669247	1020721	73.45%	9.572%
71	11.444	3218	3220	3223	rBV5	1187	674	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016532.D
 Acq On : 05 Jun 2020 13:44
 Operator : SY/MD
 Sample : L2848-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.534	3246	3248	3250	rBV3	1125	612	0.04%	0.006%
73	11.582	3258	3263	3264	rBV5	1580	1329	0.10%	0.012%
74	11.646	3271	3283	3303	rBV	678746	1059900	76.27%	9.939%
75	11.823	3335	3338	3341	rBV4	1537	1217	0.09%	0.011%
76	11.929	3368	3371	3374	rVB3	2089	1299	0.09%	0.012%
77	12.196	3453	3454	3460	rVB5	972	672	0.05%	0.006%
78	12.225	3460	3463	3465	rBV3	1202	671	0.05%	0.006%
79	12.244	3467	3469	3474	rVB4	1311	749	0.05%	0.007%
80	12.321	3489	3493	3495	rBV4	1380	1031	0.07%	0.010%
81	12.354	3500	3503	3505	rBV3	1264	830	0.06%	0.008%
82	12.447	3529	3532	3535	rBV4	1634	1128	0.08%	0.011%
83	12.492	3541	3546	3547	rBV6	1128	940	0.07%	0.009%
84	12.540	3558	3561	3566	rBV5	977	930	0.07%	0.009%
85	12.620	3581	3586	3591	rBV9	1559	1489	0.11%	0.014%
86	12.643	3591	3593	3596	rBV3	1296	782	0.06%	0.007%
87	13.164	3750	3755	3762	rVB10	2220	3124	0.22%	0.029%
88	13.202	3762	3767	3771	rBV7	1987	1797	0.13%	0.017%
89	13.402	3827	3829	3833	rVB3	1617	961	0.07%	0.009%
90	13.424	3833	3836	3838	rBV4	931	726	0.05%	0.007%
91	13.582	3883	3885	3889	rVB3	1194	727	0.05%	0.007%
92	13.685	3914	3917	3919	rBV3	1358	730	0.05%	0.007%
93	13.762	3935	3941	3942	rBV5	2398	2422	0.17%	0.023%
94	13.849	3965	3968	3974	rBV6	1691	1424	0.10%	0.013%
95	14.263	4094	4097	4098	rBV3	1262	693	0.05%	0.006%
96	14.556	4183	4188	4191	rBV6	1828	1565	0.11%	0.015%
97	14.659	4217	4220	4221	rBV2	1762	961	0.07%	0.009%
98	14.800	4260	4264	4267	rBV5	1220	1187	0.09%	0.011%
99	15.006	4326	4328	4329	rBV2	1413	695	0.05%	0.007%
100	15.186	4382	4384	4389	rVB5	1775	1250	0.09%	0.012%


Sum of corrected areas: 10663919

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016532.D
Acq On : 05 Jun 2020 13:44
Operator : SY/MD
Sample : L2848-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

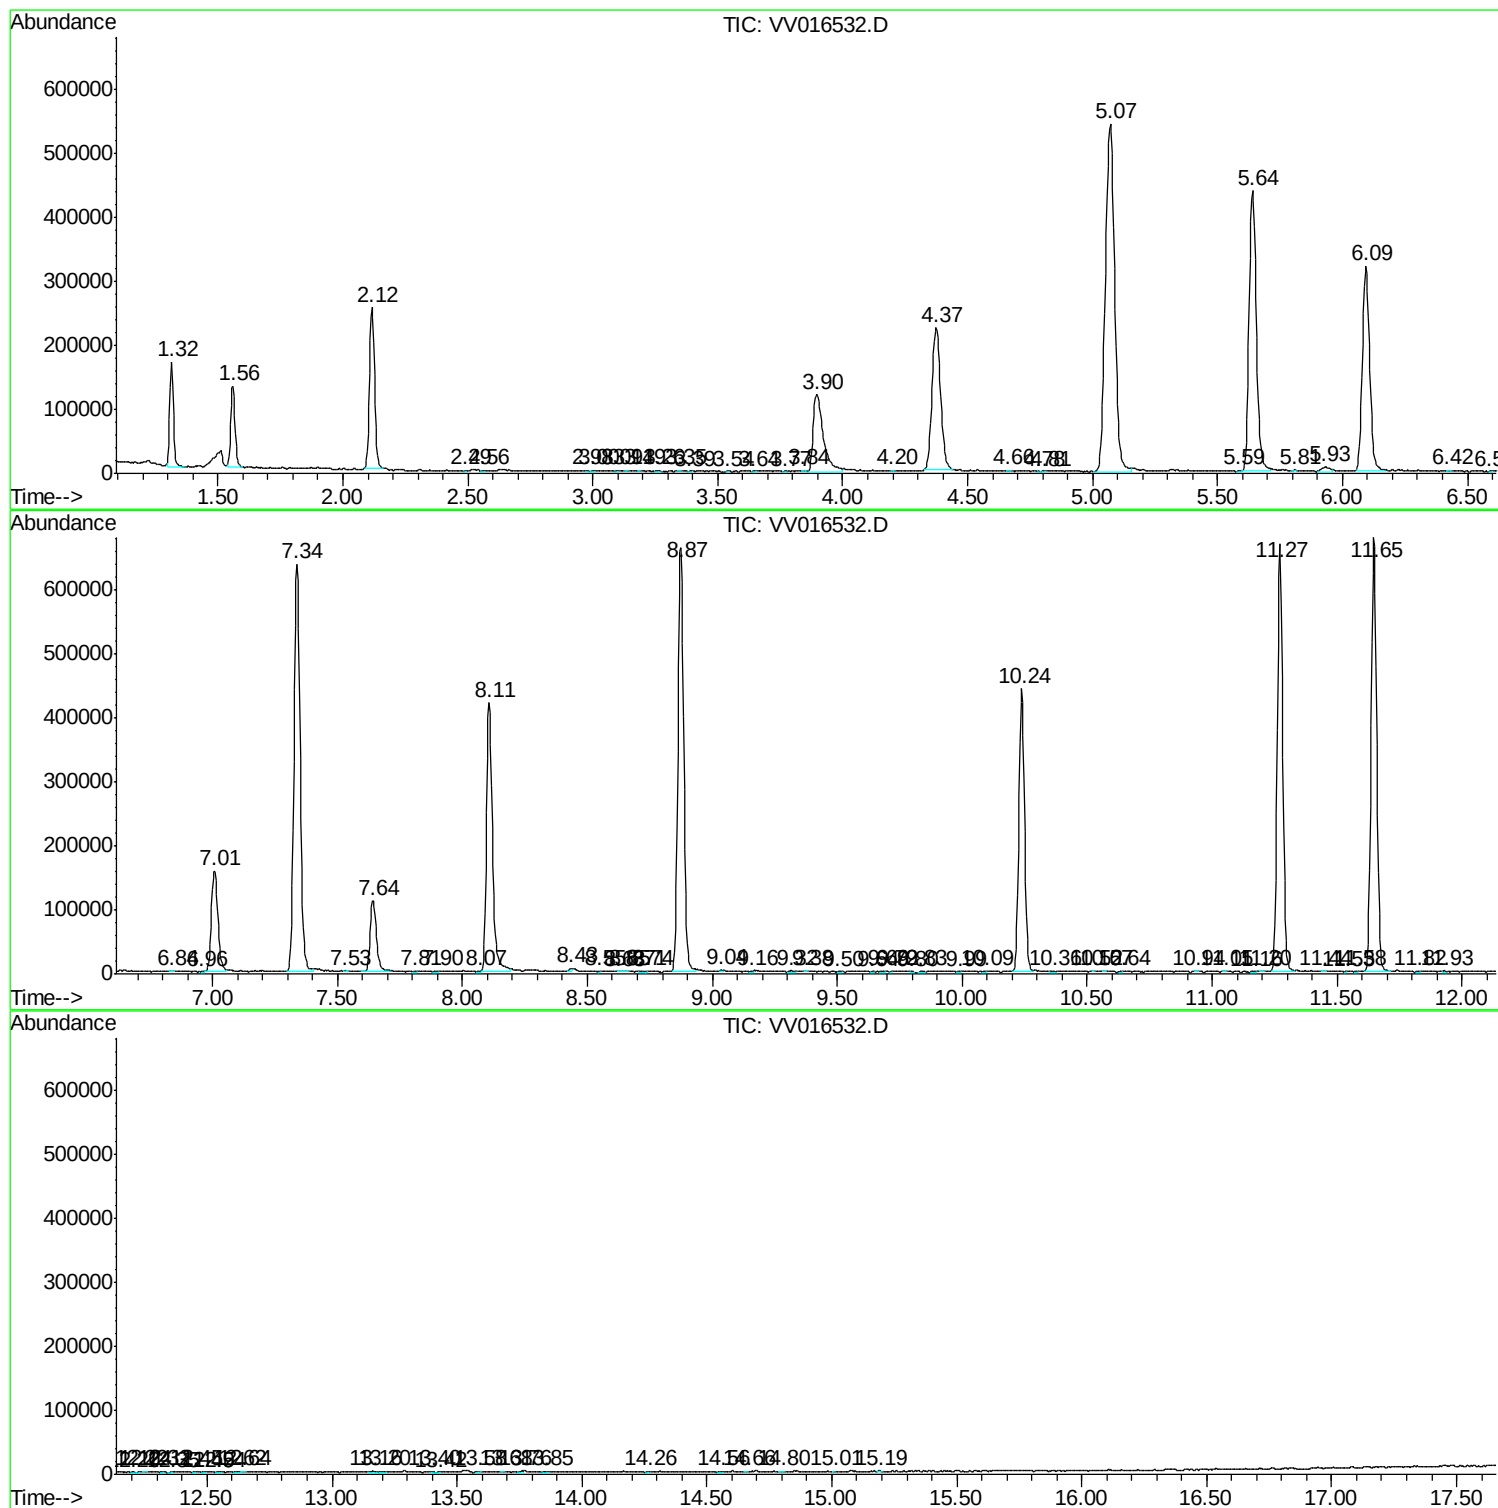

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016532.D
Acq On : 05 Jun 2020 13:44
Operator : SY/MD
Sample : L2848-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016532.D
Acq On : 05 Jun 2020 13:44
Operator : SY/MD
Sample : L2848-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc