

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016533.D
 Acq On : 05 Jun 2020 14:08
 Operator : SY/MD
 Sample : L2861-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	186836	187000	13.61%	1.807%
2	1.563	141	147	160	rVB	125505	153431	11.17%	1.483%
3	2.116	310	319	334	rBV	278049	410092	29.85%	3.963%
4	2.569	458	460	462	rBV2	1510	811	0.06%	0.008%
5	2.698	494	500	504	rBV7	1533	1690	0.12%	0.016%
6	2.817	534	537	539	rBV2	977	791	0.06%	0.008%
7	2.955	576	580	582	rBV4	1386	882	0.06%	0.009%
8	2.968	582	584	587	rVB4	1568	793	0.06%	0.008%
9	2.997	587	593	595	rBV7	836	835	0.06%	0.008%
10	3.248	666	671	673	rBV5	1186	1045	0.08%	0.010%
11	3.380	708	712	718	rBV7	1695	1879	0.14%	0.018%
12	3.434	727	729	734	rVB4	1389	1018	0.07%	0.010%
13	3.454	734	735	740	rBV5	1086	808	0.06%	0.008%
14	3.486	740	745	747	rVB6	1472	1244	0.09%	0.012%
15	3.544	760	763	766	rBV3	962	781	0.06%	0.008%
16	3.585	773	776	778	rBV4	1300	1024	0.07%	0.010%
17	3.827	846	851	856	rBV7	1335	1435	0.10%	0.014%
18	3.897	862	873	901	rBV	103466	274477	19.98%	2.652%
19	4.110	936	939	941	rBV5	1789	995	0.07%	0.010%
20	4.309	998	1001	1002	rBV2	1348	745	0.05%	0.007%
21	4.373	1007	1021	1041	rVV2	219132	528056	38.44%	5.103%
22	4.618	1092	1097	1099	rBV5	1474	1385	0.10%	0.013%
23	4.759	1136	1141	1146	rVB7	2576	2291	0.17%	0.022%
24	4.791	1146	1151	1153	rBV5	1221	1045	0.08%	0.010%
25	4.920	1189	1191	1193	rBV3	1623	831	0.06%	0.008%
26	4.946	1198	1199	1207	rVB7	1183	1259	0.09%	0.012%
27	5.071	1219	1238	1261	rBV2	537432	1373641	100.00%	13.274%
28	5.335	1317	1320	1322	rBV5	1879	1130	0.08%	0.011%
29	5.454	1354	1357	1361	rVB4	2333	1531	0.11%	0.015%
30	5.579	1392	1396	1400	rBV6	1873	1732	0.13%	0.017%
31	5.640	1401	1415	1436	rVV	422780	840474	61.19%	8.122%
32	5.872	1483	1487	1490	rBV5	1426	1231	0.09%	0.012%
33	6.019	1531	1533	1539	rBV7	1315	1063	0.08%	0.010%
34	6.093	1542	1556	1580	rBV	303402	620965	45.21%	6.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016533.D
 Acq On : 05 Jun 2020 14:08
 Operator : SY/MD
 Sample : L2861-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.463	1664	1671	1674	rBV5	1328	1889	0.14%	0.018%
36	6.547	1693	1697	1699	rBV5	949	810	0.06%	0.008%
37	6.627	1719	1722	1724	rBV4	1493	942	0.07%	0.009%
38	6.945	1817	1821	1824	rBV6	1329	1134	0.08%	0.011%
39	7.007	1827	1840	1858	rBV	157466	286308	20.84%	2.767%
40	7.219	1904	1906	1909	rBV3	1352	1072	0.08%	0.010%
41	7.338	1930	1943	1961	rBV	629404	1077378	78.43%	10.411%
42	7.643	2025	2038	2056	rBV	114663	197601	14.39%	1.909%
43	7.910	2114	2121	2122	rBV7	1796	1684	0.12%	0.016%
44	7.933	2126	2128	2130	rBV3	1525	849	0.06%	0.008%
45	8.106	2169	2182	2209	rBV	384198	655280	47.70%	6.332%
46	8.640	2344	2348	2351	rBV5	1998	1649	0.12%	0.016%
47	8.823	2403	2405	2407	rBV3	1424	846	0.06%	0.008%
48	8.875	2408	2421	2439	rVV	641844	1024764	74.60%	9.902%
49	9.196	2517	2521	2526	rVB8	1091	1095	0.08%	0.011%
50	9.283	2544	2548	2551	rVB5	1400	946	0.07%	0.009%
51	9.540	2620	2628	2632	rBV9	1938	2744	0.20%	0.027%
52	9.852	2722	2725	2729	rVB5	1454	836	0.06%	0.008%
53	9.878	2729	2733	2735	rBV4	1113	773	0.06%	0.007%
54	10.090	2797	2799	2803	rBV3	1387	791	0.06%	0.008%
55	10.135	2810	2813	2816	rBV5	1310	994	0.07%	0.010%
56	10.180	2825	2827	2830	rVB4	1675	838	0.06%	0.008%
57	10.238	2830	2845	2860	rBV	398610	636072	46.31%	6.146%
58	10.502	2925	2927	2930	rVB4	1468	866	0.06%	0.008%
59	10.556	2937	2944	2946	rBV6	1190	1125	0.08%	0.011%
60	10.675	2980	2981	2986	rVB4	1321	911	0.07%	0.009%
61	10.865	3034	3040	3041	rBV4	1998	1990	0.14%	0.019%
62	10.939	3061	3063	3066	rBV3	1396	852	0.06%	0.008%
63	10.971	3070	3073	3079	rVB7	1975	1934	0.14%	0.019%
64	10.994	3079	3080	3084	rBV4	1165	859	0.06%	0.008%
65	11.032	3088	3092	3094	rBV4	1594	1235	0.09%	0.012%
66	11.080	3105	3107	3110	rBV2	1174	822	0.06%	0.008%
67	11.135	3122	3124	3127	rBV3	997	828	0.06%	0.008%
68	11.270	3155	3166	3182	rBV	643367	972756	70.82%	9.400%
69	11.502	3233	3238	3240	rBV4	1478	1210	0.09%	0.012%
70	11.527	3244	3246	3249	rVB4	1204	803	0.06%	0.008%
71	11.550	3249	3253	3255	rBV4	1692	1254	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016533.D
 Acq On : 05 Jun 2020 14:08
 Operator : SY/MD
 Sample : L2861-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9D77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.646	3270	3283	3301	rBV	649256	1010173	73.54%	9.761%
73	11.801	3329	3331	3334	rBV3	1494	1239	0.09%	0.012%
74	11.945	3374	3376	3381	rVB4	1094	1033	0.08%	0.010%
75	12.061	3410	3412	3414	rBV3	1766	820	0.06%	0.008%
76	12.116	3427	3429	3432	rVB3	1498	755	0.05%	0.007%
77	12.141	3433	3437	3439	rBV3	1110	787	0.06%	0.008%
78	12.193	3449	3453	3455	rBV4	1389	1128	0.08%	0.011%
79	12.228	3461	3464	3468	rVB5	1322	1072	0.08%	0.010%
80	12.283	3476	3481	3484	rBV6	1480	1517	0.11%	0.015%
81	12.318	3489	3492	3495	rBV5	1678	928	0.07%	0.009%
82	12.399	3515	3517	3520	rBV3	1465	969	0.07%	0.009%
83	12.469	3535	3539	3540	rBV4	1104	909	0.07%	0.009%
84	12.585	3571	3575	3578	rVB5	1560	1012	0.07%	0.010%
85	12.608	3578	3582	3583	rBV3	1589	1084	0.08%	0.010%
86	12.694	3607	3609	3613	rBV4	1151	797	0.06%	0.008%
87	13.132	3741	3745	3749	rBV5	1476	1206	0.09%	0.012%
88	13.161	3749	3754	3762	rBV10	2012	3252	0.24%	0.031%
89	13.264	3782	3786	3790	rBV6	1835	2000	0.15%	0.019%
90	13.325	3802	3805	3809	rBV4	1756	1686	0.12%	0.016%
91	13.530	3862	3869	3871	rBV8	2728	2974	0.22%	0.029%
92	13.710	3922	3925	3928	rBV4	889	801	0.06%	0.008%
93	13.849	3965	3968	3973	rBV7	1334	1442	0.10%	0.014%
94	13.894	3978	3982	3985	rBV5	1861	1818	0.13%	0.018%
95	13.955	3998	4001	4004	rBV4	1230	934	0.07%	0.009%
96	14.241	4088	4090	4094	rVB5	1493	803	0.06%	0.008%
97	14.627	4205	4210	4211	rBV4	1772	1492	0.11%	0.014%
98	14.836	4273	4275	4280	rBV5	1304	1102	0.08%	0.011%
99	15.096	4353	4356	4357	rBV3	1543	812	0.06%	0.008%
100	15.193	4384	4386	4390	rBV5	1071	875	0.06%	0.008%


Sum of corrected areas: 10348570

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016533.D
Acq On : 05 Jun 2020 14:08
Operator : SY/MD
Sample : L2861-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D77

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

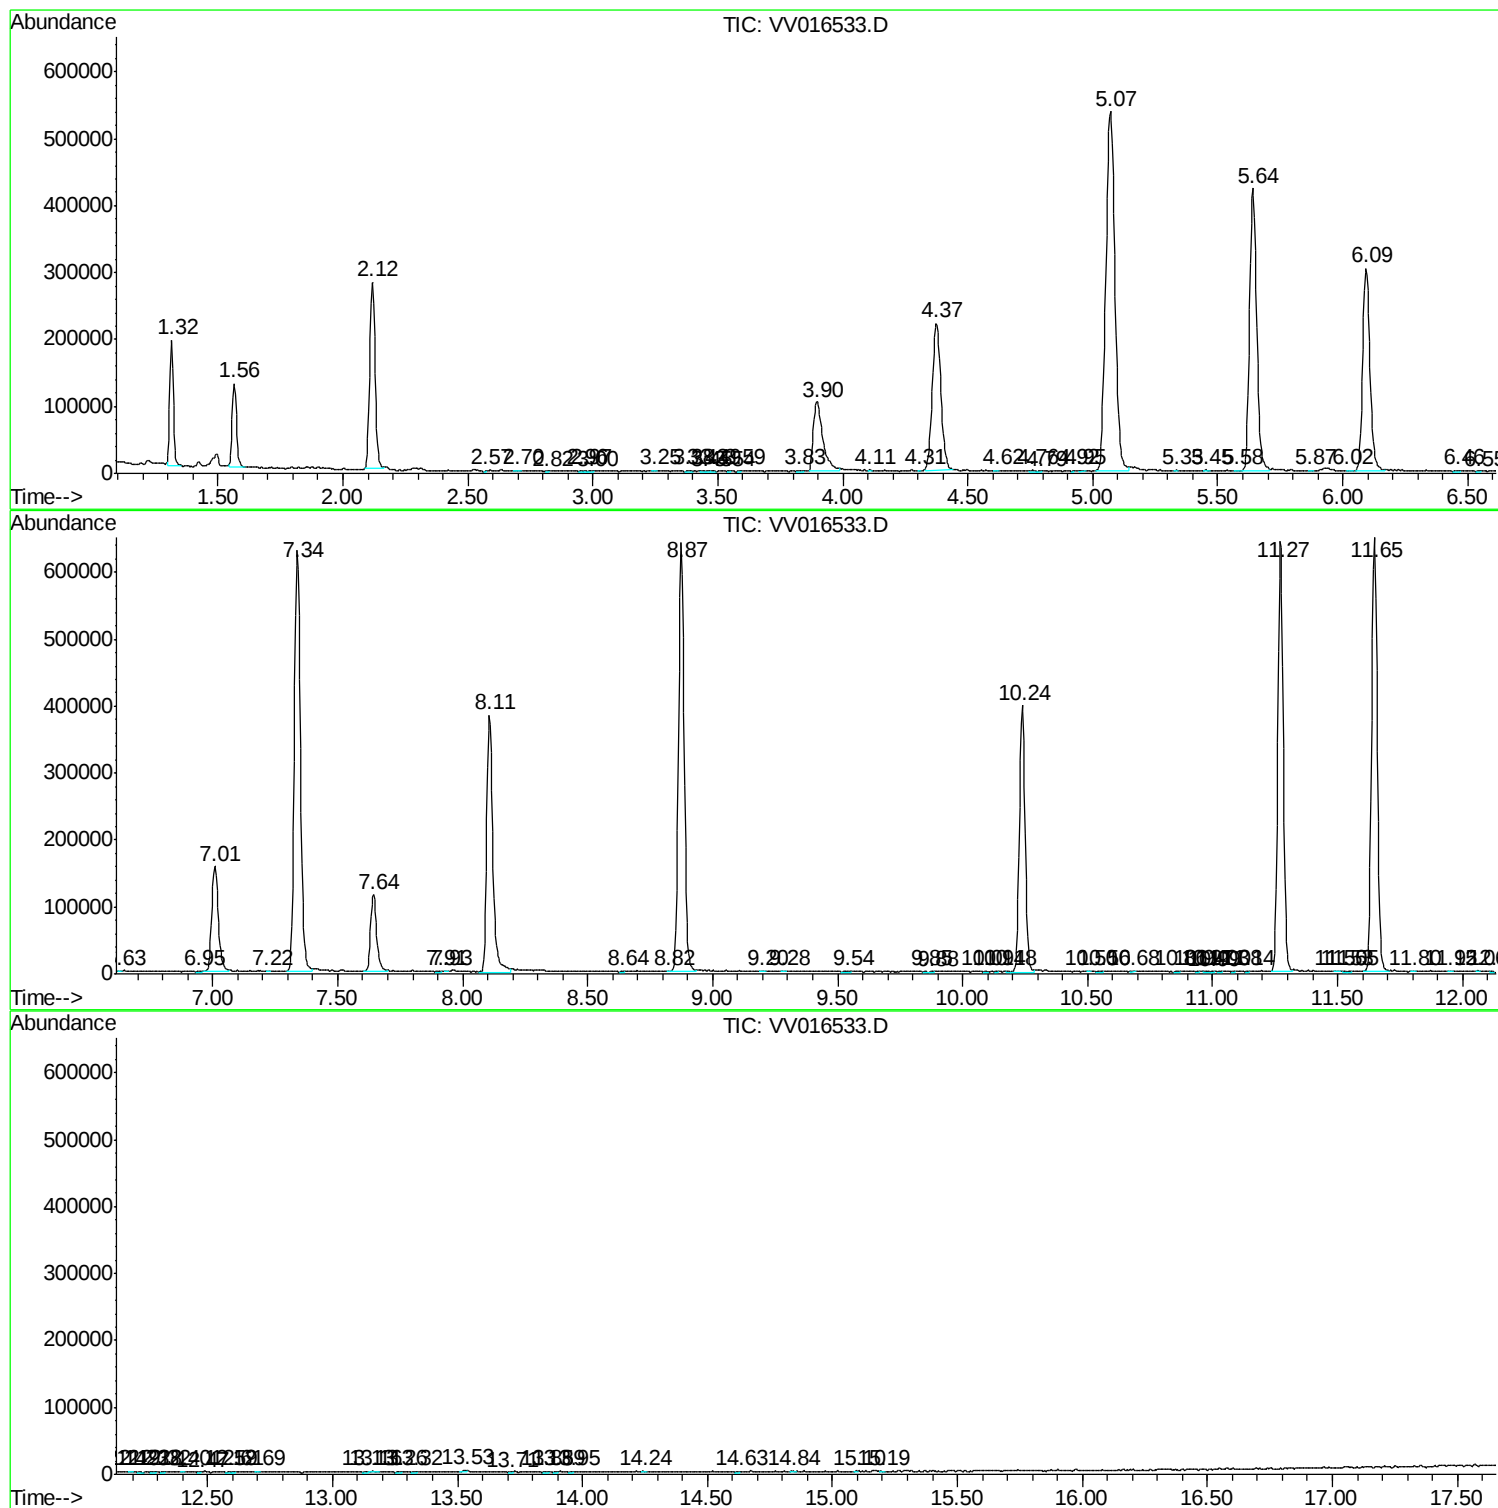

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016533.D
Acq On : 05 Jun 2020 14:08
Operator : SY/MD
Sample : L2861-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D77

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016533.D
Acq On : 05 Jun 2020 14:08
Operator : SY/MD
Sample : L2861-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9D77

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc