

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016548.D
 Acq On : 05 Jun 2020 20:03
 Operator : SY/MD
 Sample : L2861-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	80	rVB	187424	188793	13.63%	1.614%
2	1.556	138	145	158	rVB	124909	151192	10.92%	1.292%
3	2.116	309	319	332	rBV	281356	415283	29.99%	3.549%
4	2.296	373	375	380	rVB5	1835	1269	0.09%	0.011%
5	2.482	431	433	435	rBV2	2106	1214	0.09%	0.010%
6	2.592	459	467	469	rBV7	2809	3014	0.22%	0.026%
7	2.630	477	479	483	rBV5	1183	877	0.06%	0.007%
8	2.672	488	492	497	rBV6	1610	1564	0.11%	0.013%
9	3.048	605	609	610	rBV3	1407	845	0.06%	0.007%
10	3.058	610	612	615	rVV3	1290	1022	0.07%	0.009%
11	3.090	619	622	626	rVV4	1063	822	0.06%	0.007%
12	3.158	641	643	646	rVV4	1580	1232	0.09%	0.011%
13	3.171	646	647	651	rVB2	1815	914	0.07%	0.008%
14	3.199	651	656	660	rBV6	1736	1486	0.11%	0.013%
15	3.228	660	665	666	rBV5	1521	1139	0.08%	0.010%
16	3.376	709	711	714	rVB2	1456	831	0.06%	0.007%
17	3.396	714	717	721	rBV6	1055	955	0.07%	0.008%
18	3.447	728	733	736	rBV7	1763	1675	0.12%	0.014%
19	3.531	754	759	761	rBV5	1103	879	0.06%	0.008%
20	3.563	767	769	773	rBV4	1368	983	0.07%	0.008%
21	3.894	862	872	895	rVV2	108951	281488	20.33%	2.406%
22	4.080	928	930	934	rVB5	1454	882	0.06%	0.008%
23	4.145	948	950	954	rVB2	1965	1261	0.09%	0.011%
24	4.174	954	959	960	rBV5	1330	1085	0.08%	0.009%
25	4.373	1001	1021	1046	rBV	231366	582488	42.06%	4.978%
26	4.550	1074	1076	1080	rVB3	1681	1047	0.08%	0.009%
27	4.678	1113	1116	1118	rBV5	1216	827	0.06%	0.007%
28	4.817	1155	1159	1162	rVB6	1212	1097	0.08%	0.009%
29	5.068	1215	1237	1247	rBV2	548183	1384911	100.00%	11.837%
30	5.328	1314	1318	1320	rBV4	1379	985	0.07%	0.008%
31	5.418	1342	1346	1348	rVB4	1306	831	0.06%	0.007%
32	5.559	1388	1390	1394	rBV5	1109	852	0.06%	0.007%
33	5.640	1402	1415	1437	rBV	503443	994130	71.78%	8.497%
34	5.929	1494	1505	1514	rVV9	8185	16086	1.16%	0.137%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016548.D
 Acq On : 05 Jun 2020 20:03
 Operator : SY/MD
 Sample : L2861-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.093	1542	1556	1579	rVV	317083	631914	45.63%	5.401%
36	6.386	1644	1647	1650	rBV4	1342	842	0.06%	0.007%
37	6.402	1650	1652	1657	rVB5	1380	1069	0.08%	0.009%
38	6.434	1657	1662	1665	rBV6	1225	960	0.07%	0.008%
39	6.492	1678	1680	1684	rVB4	1358	920	0.07%	0.008%
40	6.630	1720	1723	1726	rVV4	1485	1180	0.09%	0.010%
41	6.646	1726	1728	1734	rVB6	2226	1779	0.13%	0.015%
42	6.682	1734	1739	1741	rBV4	1556	1355	0.10%	0.012%
43	6.948	1817	1822	1823	rBV4	1449	940	0.07%	0.008%
44	7.006	1827	1840	1863	rBV2	169103	303606	21.92%	2.595%
45	7.090	1863	1866	1869	rBV3	1090	918	0.07%	0.008%
46	7.180	1890	1894	1898	rBV6	2290	2113	0.15%	0.018%
47	7.338	1929	1943	1958	rBV	655714	1118346	80.75%	9.558%
48	7.411	1958	1966	1979	rVB	50722	93176	6.73%	0.796%
49	7.547	2002	2008	2010	rBV7	2689	2523	0.18%	0.022%
50	7.643	2027	2038	2054	rBV	115305	198709	14.35%	1.698%
51	7.913	2119	2122	2125	rVB3	1200	852	0.06%	0.007%
52	7.932	2125	2128	2132	rVB7	1374	1183	0.09%	0.010%
53	7.961	2135	2137	2144	rVB7	1818	1713	0.12%	0.015%
54	8.106	2169	2182	2211	rBV	413594	718915	51.91%	6.144%
55	8.363	2260	2262	2267	rVB4	1285	1012	0.07%	0.009%
56	8.392	2267	2271	2275	rVV	18831	11004	0.79%	0.094%
57	8.418	2275	2279	2282	rVB6	1285	1078	0.08%	0.009%
58	8.440	2282	2286	2292	rVB8	1844	2127	0.15%	0.018%
59	8.505	2303	2306	2309	rVB5	1380	963	0.07%	0.008%
60	8.874	2407	2421	2447	rVV	752587	1239166	89.48%	10.591%
61	9.035	2459	2471	2486	rBV	45506	80011	5.78%	0.684%
62	9.161	2502	2510	2519	rBV2	16411	27806	2.01%	0.238%
63	9.325	2559	2561	2565	rBV5	1113	882	0.06%	0.008%
64	9.408	2579	2587	2593	rBV10	5348	8198	0.59%	0.070%
65	9.463	2600	2604	2605	rBV3	1983	1315	0.09%	0.011%
66	9.527	2620	2624	2627	rVB5	1855	1260	0.09%	0.011%
67	9.569	2627	2637	2645	rBV2	17201	28674	2.07%	0.245%
68	9.688	2672	2674	2675	rBV2	1624	835	0.06%	0.007%
69	9.887	2729	2736	2744	rVB2	4608	6653	0.48%	0.057%
70	9.932	2747	2750	2752	rBV4	1564	1010	0.07%	0.009%
71	10.099	2794	2802	2805	rBV7	4158	5759	0.42%	0.049%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016548.D
Acq On : 05 Jun 2020 20:03
Operator : SY/MD
Sample : L2861-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E71

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Title : VOC Analysis

72	10.167	2820	2823	2825	rBV4	1169	824	0.06%	0.007%
73	10.238	2832	2845	2858	rBV	422670	656510	47.40%	5.611%
74	10.382	2884	2890	2900	rVB	5294	10166	0.73%	0.087%
75	10.427	2900	2904	2905	rBV3	2282	1553	0.11%	0.013%
76	10.534	2933	2937	2939	rBV4	2605	2425	0.18%	0.021%
77	10.710	2986	2992	2994	rBV6	2327	2090	0.15%	0.018%
78	10.759	3004	3007	3009	rBV3	3189	2246	0.16%	0.019%
79	10.942	3058	3064	3070	rBV6	4511	6348	0.46%	0.054%
80	11.054	3095	3099	3101	rBV3	1074	869	0.06%	0.007%
81	11.270	3154	3166	3183	rBV	804157	1230791	88.87%	10.519%
82	11.360	3187	3194	3203	rVB7	7938	12888	0.93%	0.110%
83	11.556	3249	3255	3264	rVB10	4116	6684	0.48%	0.057%
84	11.646	3270	3283	3299	rBV	703658	1091568	78.82%	9.329%
85	11.778	3315	3324	3327	rBV	6198	9212	0.67%	0.079%
86	11.939	3362	3374	3385	rBV	5711	14304	1.03%	0.122%
87	12.112	3423	3428	3435	rBV8	4011	6779	0.49%	0.058%
88	12.466	3535	3538	3542	rBV6	1495	1372	0.10%	0.012%
89	12.595	3576	3578	3581	rBV4	1862	1145	0.08%	0.010%
90	12.974	3692	3696	3697	rBV4	2857	2193	0.16%	0.019%
91	13.035	3713	3715	3721	rVB6	2374	2097	0.15%	0.018%
92	13.090	3725	3732	3740	rBV6	3592	6637	0.48%	0.057%
93	13.466	3843	3849	3860	rBV2	12187	20235	1.46%	0.173%
94	13.530	3862	3869	3885	rVB2	18165	32086	2.32%	0.274%
95	13.623	3890	3898	3903	rBV3	12614	21134	1.53%	0.181%
96	13.865	3970	3973	3974	rBV3	2034	1133	0.08%	0.010%
97	13.977	4005	4008	4010	rBV4	1457	1075	0.08%	0.009%
98	15.331	4420	4429	4435	rBV10	5184	8739	0.63%	0.075%
99	15.482	4472	4476	4477	rBV3	1814	1514	0.11%	0.013%
100	15.566	4500	4502	4505	rVB4	1966	872	0.06%	0.007%


Sum of corrected areas: 11700214

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016548.D
Acq On : 05 Jun 2020 20:03
Operator : SY/MD
Sample : L2861-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E71

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

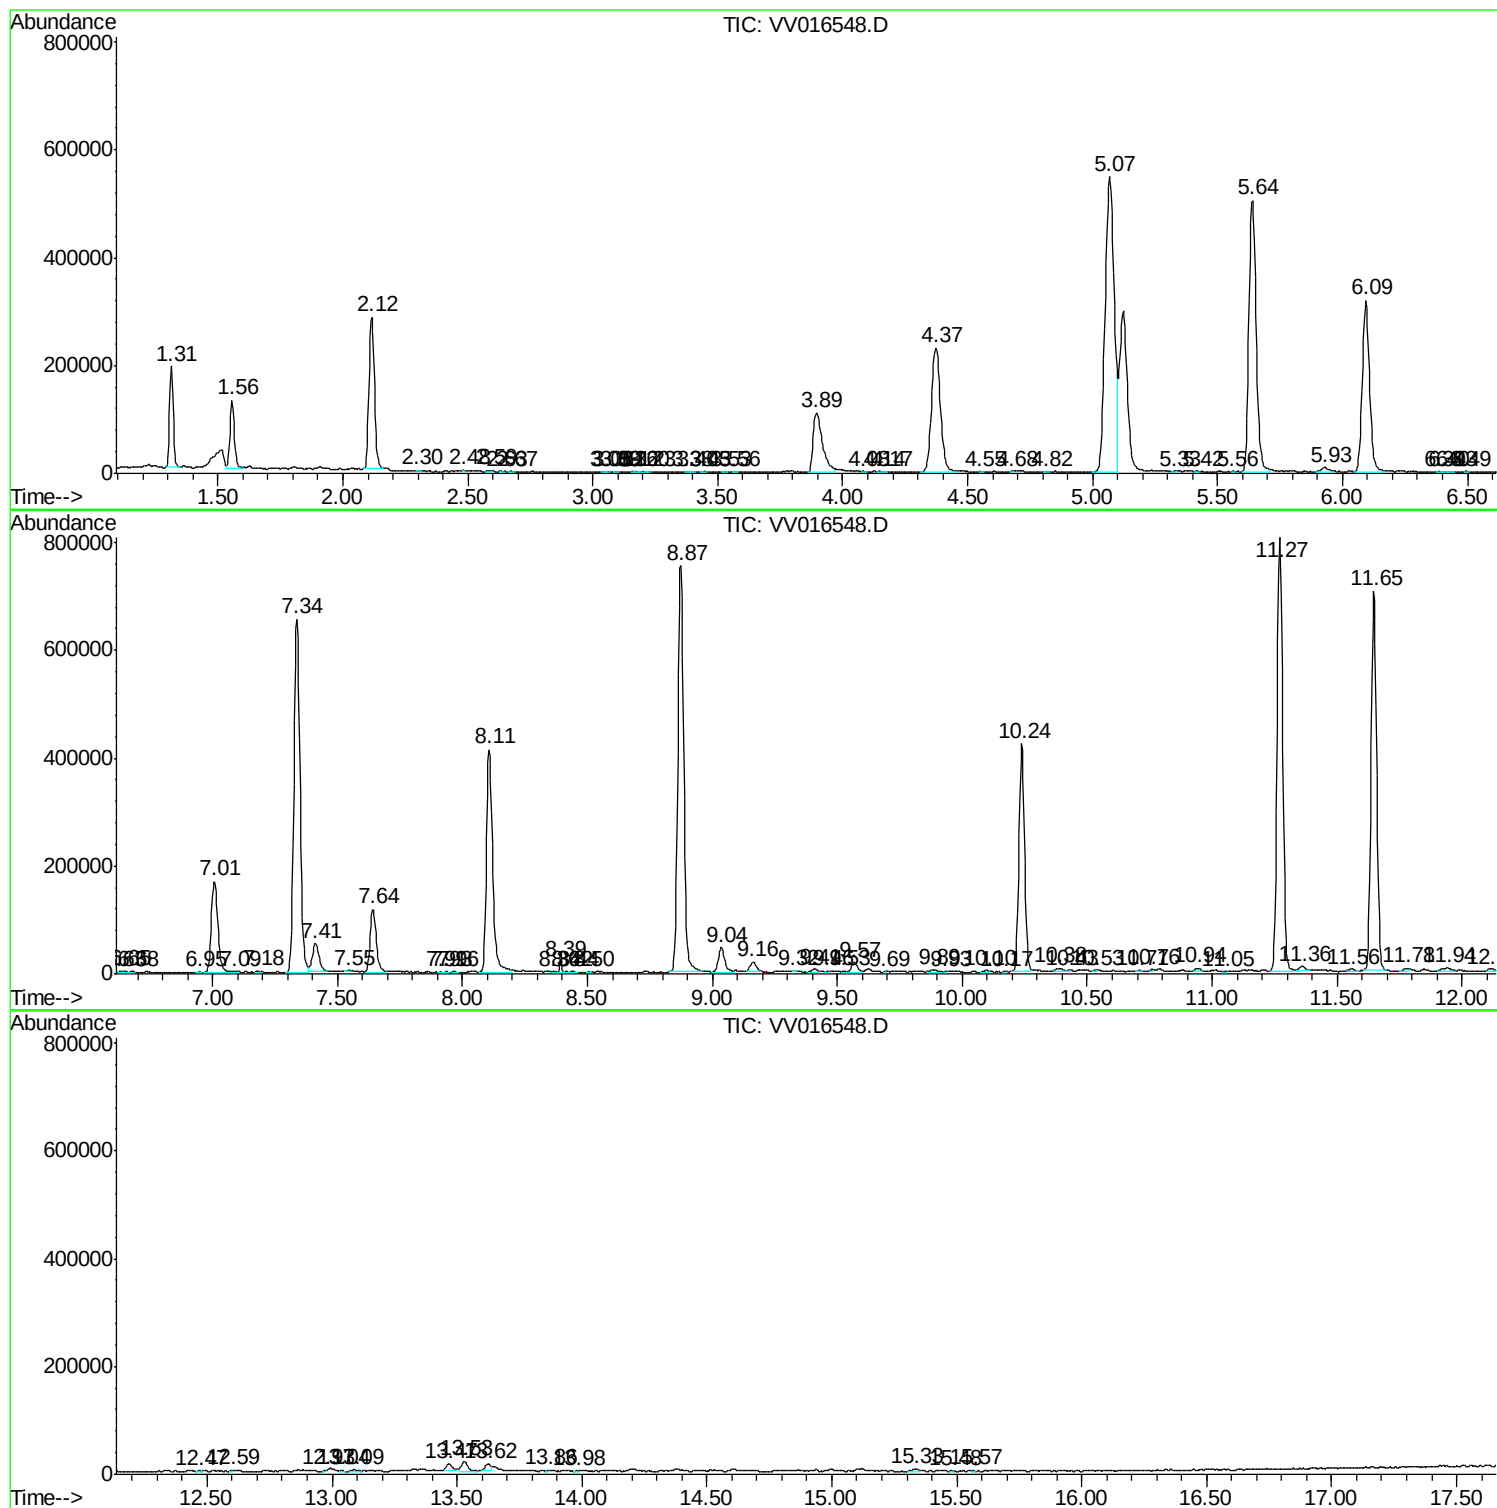

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016548.D
Acq On : 05 Jun 2020 20:03
Operator : SY/MD
Sample : L2861-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E71

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016548.D
Acq On : 05 Jun 2020 20:03
Operator : SY/MD
Sample : L2861-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E71

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc