

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016550.D
 Acq On : 05 Jun 2020 20:50
 Operator : SY/MD
 Sample : L2872-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEN5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	81	rVB	202795	205740	1.99%	0.922%
2	1.563	140	147	159	rVB	131975	159179	1.54%	0.713%
3	2.116	310	319	341	rVB	311238	464991	4.49%	2.083%
4	2.422	411	414	417	rVB5	1463	810	0.01%	0.004%
5	2.698	498	500	504	rBV3	1425	1152	0.01%	0.005%
6	2.730	506	510	512	rVB4	1202	713	0.01%	0.003%
7	2.865	549	552	553	rBV3	1140	648	0.01%	0.003%
8	2.926	568	571	575	rBV4	1583	1641	0.02%	0.007%
9	3.126	632	633	637	rVB4	1733	817	0.01%	0.004%
10	3.177	645	649	650	rBV3	1122	586	0.01%	0.003%
11	3.241	666	669	674	rBV7	1257	1332	0.01%	0.006%
12	3.264	674	676	679	rVB3	1437	660	0.01%	0.003%
13	3.287	681	683	686	rVB4	1050	608	0.01%	0.003%
14	3.306	686	689	692	rBV5	1066	727	0.01%	0.003%
15	3.434	724	729	733	rBV5	1060	1109	0.01%	0.005%
16	3.476	739	742	746	rBV5	1158	802	0.01%	0.004%
17	3.624	786	788	792	rVB3	1117	558	0.01%	0.002%
18	3.730	817	821	824	rBV4	1651	1523	0.01%	0.007%
19	3.897	861	873	914	rBV2	119803	439666	4.24%	1.969%
20	4.254	981	984	985	rBV3	1170	647	0.01%	0.003%
21	4.306	998	1000	1003	rBV4	931	692	0.01%	0.003%
22	4.373	1003	1021	1047	rVV	238012	589749	5.69%	2.642%
23	4.540	1070	1073	1076	rBV3	1245	1121	0.01%	0.005%
24	4.740	1133	1135	1141	rVB6	1207	1042	0.01%	0.005%
25	4.823	1159	1161	1166	rBV6	1974	1505	0.01%	0.007%
26	4.856	1167	1171	1175	rVV5	1275	1109	0.01%	0.005%
27	4.894	1180	1183	1186	rBV5	1454	1015	0.01%	0.005%
28	4.933	1193	1195	1198	rBV4	1312	1013	0.01%	0.005%
29	4.978	1207	1209	1214	rVB3	1401	984	0.01%	0.004%
30	5.000	1214	1216	1219	rBV3	1106	647	0.01%	0.003%
31	5.071	1219	1238	1273	rBV2	594384	1602136	15.46%	7.177%
32	5.331	1317	1319	1323	rBV3	1858	971	0.01%	0.004%
33	5.405	1339	1342	1344	rBV3	1730	1134	0.01%	0.005%
34	5.470	1361	1362	1364	rBV2	1242	580	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016550.D
 Acq On : 05 Jun 2020 20:50
 Operator : SY/MD
 Sample : L2872-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEN5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	5.563	1388	1391	1395	rVB5	1145	796	0.01%	0.004%
36	5.589	1395	1399	1400	rBV2	912	672	0.01%	0.003%
37	5.640	1403	1415	1438	rVV	509035	1004187	9.69%	4.498%
38	5.942	1496	1509	1524	rBV4	22891	52324	0.50%	0.234%
39	6.093	1544	1556	1578	rVB	332684	664055	6.41%	2.975%
40	6.463	1668	1671	1673	rBV3	1953	1261	0.01%	0.006%
41	6.492	1677	1680	1683	rVV5	1213	963	0.01%	0.004%
42	6.521	1686	1689	1694	rBV5	1856	1687	0.02%	0.008%
43	6.621	1716	1720	1723	rBV5	977	1064	0.01%	0.005%
44	6.772	1763	1767	1768	rBV3	818	571	0.01%	0.003%
45	6.849	1787	1791	1793	rVB5	1113	834	0.01%	0.004%
46	6.862	1793	1795	1798	rBV3	1096	862	0.01%	0.004%
47	6.878	1798	1800	1803	rVB3	1306	636	0.01%	0.003%
48	6.901	1803	1807	1812	rBV7	1276	1377	0.01%	0.006%
49	6.939	1815	1819	1824	rVB6	1597	1569	0.02%	0.007%
50	7.007	1828	1840	1857	rBV	172491	313853	3.03%	1.406%
51	7.338	1931	1943	1958	rBV	707070	1201351	11.59%	5.381%
52	7.640	2028	2037	2057	rBV	122012	206659	1.99%	0.926%
53	7.997	2133	2148	2171	rVV	6197636	10364496	100.00%	46.426%
54	8.106	2173	2182	2215	rVB	441712	750548	7.24%	3.362%
55	8.875	2409	2421	2437	rBV	742389	1203651	11.61%	5.392%
56	9.035	2463	2471	2484	rBV2	13652	22552	0.22%	0.101%
57	9.161	2505	2510	2511	rBV5	4185	3692	0.04%	0.017%
58	9.318	2556	2559	2562	rBV2	1622	970	0.01%	0.004%
59	9.437	2593	2596	2603	rBV8	1440	1667	0.02%	0.007%
60	9.563	2630	2635	2641	rBV7	3607	5118	0.05%	0.023%
61	9.627	2651	2655	2656	rBV4	901	712	0.01%	0.003%
62	9.717	2679	2683	2687	rBV5	1774	1482	0.01%	0.007%
63	9.746	2690	2692	2696	rBV4	917	752	0.01%	0.003%
64	9.839	2716	2721	2723	rBV5	1911	1376	0.01%	0.006%
65	9.888	2734	2736	2739	rBV3	978	652	0.01%	0.003%
66	10.093	2797	2800	2804	rBV4	1119	987	0.01%	0.004%
67	10.177	2823	2826	2829	rBV4	1595	1436	0.01%	0.006%
68	10.238	2833	2845	2864	rVV	444181	705361	6.81%	3.160%
69	10.431	2903	2905	2910	rVB5	2109	1272	0.01%	0.006%
70	10.569	2946	2948	2950	rBV2	1712	922	0.01%	0.004%
71	10.910	3050	3054	3056	rBV4	1163	1087	0.01%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016550.D
 Acq On : 05 Jun 2020 20:50
 Operator : SY/MD
 Sample : L2872-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEN5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.984	3075	3077	3079	rBV2	1456	728	0.01%	0.003%
73	11.058	3095	3100	3101	rBV4	1442	889	0.01%	0.004%
74	11.164	3128	3133	3134	rBV4	1265	979	0.01%	0.004%
75	11.270	3154	3166	3185	rBV	767597	1160639	11.20%	5.199%
76	11.547	3249	3252	3253	rBV3	1278	804	0.01%	0.004%
77	11.598	3266	3268	3270	rBV3	1169	660	0.01%	0.003%
78	11.646	3272	3283	3302	rVV	726058	1125692	10.86%	5.042%
79	11.842	3341	3344	3348	rBV5	1636	1333	0.01%	0.006%
80	11.878	3351	3355	3357	rVB4	1235	867	0.01%	0.004%
81	11.916	3364	3367	3370	rBV4	1740	1402	0.01%	0.006%
82	11.932	3370	3372	3374	rVB3	1568	624	0.01%	0.003%
83	12.135	3429	3435	3440	rVB8	1504	1795	0.02%	0.008%
84	12.273	3474	3478	3480	rBV5	1570	1099	0.01%	0.005%
85	12.437	3528	3529	3533	rBV4	1472	846	0.01%	0.004%
86	12.543	3560	3562	3567	rVB4	1773	1079	0.01%	0.005%
87	12.669	3598	3601	3602	rBV	1666	752	0.01%	0.003%
88	12.727	3615	3619	3620	rBV4	1035	755	0.01%	0.003%
89	12.833	3649	3652	3654	rBV3	936	557	0.01%	0.002%
90	13.058	3720	3722	3723	rBV2	1396	638	0.01%	0.003%
91	13.087	3728	3731	3733	rVV3	1004	784	0.01%	0.004%
92	13.154	3749	3752	3755	rBV4	965	673	0.01%	0.003%
93	13.222	3771	3773	3775	rBV3	1502	737	0.01%	0.003%
94	13.238	3775	3778	3780	rBV3	1076	699	0.01%	0.003%
95	13.283	3789	3792	3797	rVB5	1819	1665	0.02%	0.007%
96	13.315	3797	3802	3806	rBV8	1561	1949	0.02%	0.009%
97	13.405	3828	3830	3832	rBV3	1266	792	0.01%	0.004%
98	13.688	3914	3918	3922	rBV5	1315	1584	0.02%	0.007%
99	13.990	4010	4012	4014	rBV3	1077	618	0.01%	0.003%
100	14.296	4101	4107	4109	rBV6	1760	1884	0.02%	0.008%


Sum of corrected areas: 22324584

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016550.D
Acq On : 05 Jun 2020 20:50
Operator : SY/MD
Sample : L2872-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEN5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

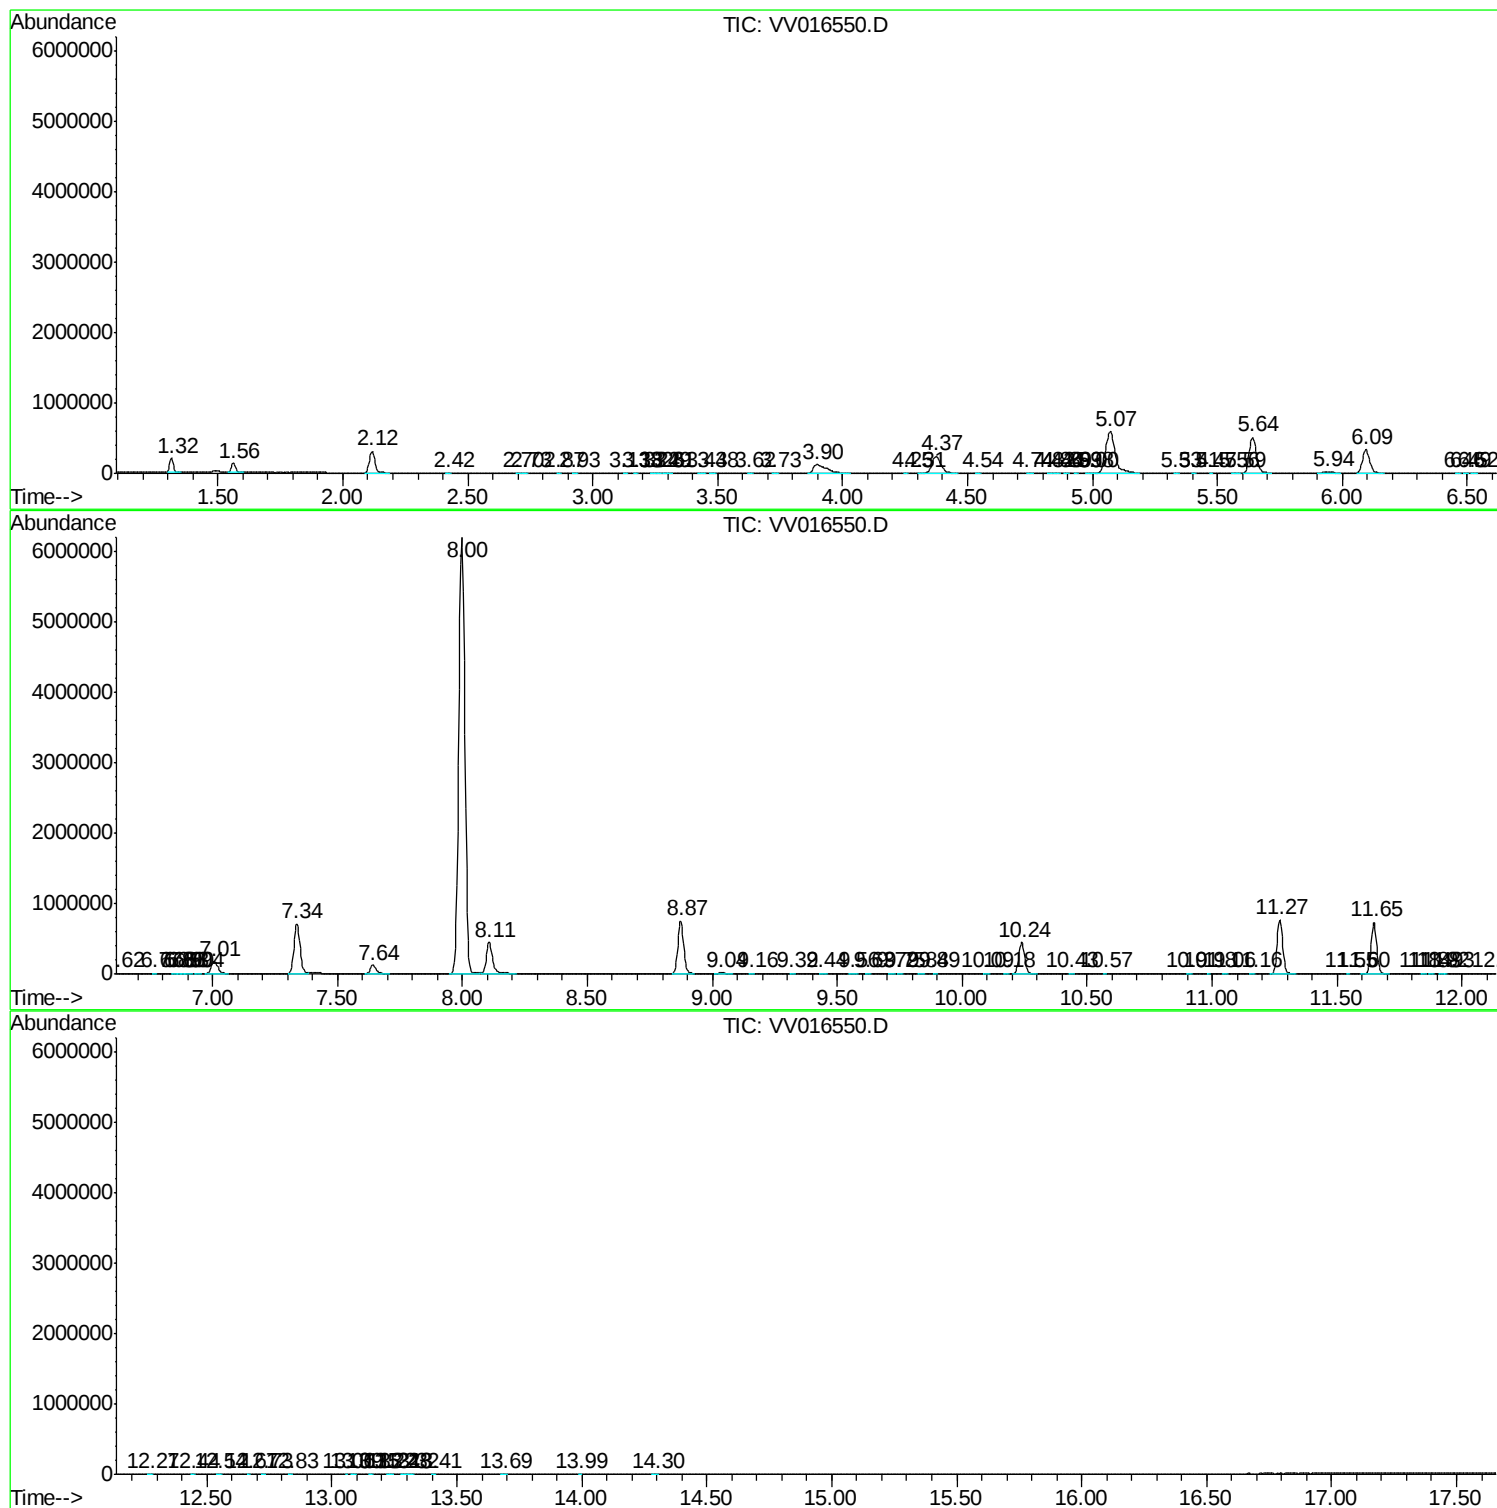

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016550.D
Acq On : 05 Jun 2020 20:50
Operator : SY/MD
Sample : L2872-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEN5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016550.D
Acq On : 05 Jun 2020 20:50
Operator : SY/MD
Sample : L2872-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEN5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc