

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016552.D
 Acq On : 05 Jun 2020 22:30
 Operator : SY/MD
 Sample : VV0605WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK69

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	218627	220653	13.44%	1.798%
2	1.557	139	145	158	rVB	136209	168984	10.29%	1.377%
3	2.116	310	319	342	rVB	325729	493977	30.09%	4.024%
4	2.338	386	388	390	rBV3	1423	617	0.04%	0.005%
5	2.724	506	508	511	rVB3	1172	601	0.04%	0.005%
6	2.785	518	527	530	rBV9	2464	2872	0.17%	0.023%
7	2.859	547	550	554	rBV6	1066	994	0.06%	0.008%
8	2.913	564	567	571	rBV4	1312	1161	0.07%	0.009%
9	3.000	590	594	596	rBV5	931	851	0.05%	0.007%
10	3.055	608	611	614	rVB4	1506	976	0.06%	0.008%
11	3.126	630	633	637	rBV4	1228	1089	0.07%	0.009%
12	3.158	641	643	646	rBV4	918	664	0.04%	0.005%
13	3.212	658	660	663	rBV3	1331	732	0.04%	0.006%
14	3.344	699	701	706	rVB4	1312	950	0.06%	0.008%
15	3.454	730	735	736	rBV4	1704	1122	0.07%	0.009%
16	3.534	757	760	761	rBV3	1203	811	0.05%	0.007%
17	3.605	779	782	786	rBV4	1076	701	0.04%	0.006%
18	3.624	786	788	792	rVV5	960	886	0.05%	0.007%
19	3.653	795	797	802	rBV3	1115	665	0.04%	0.005%
20	3.753	823	828	830	rBV4	1587	1587	0.10%	0.013%
21	3.830	850	852	856	rBV5	969	656	0.04%	0.005%
22	3.894	862	872	899	rBV2	125031	345856	21.07%	2.818%
23	4.254	978	984	987	rBV7	1872	2328	0.14%	0.019%
24	4.373	1004	1021	1045	rBV	253756	622146	37.90%	5.069%
25	4.881	1177	1179	1180	rBV	1140	608	0.04%	0.005%
26	5.068	1219	1237	1269	rBV2	622908	1641698	100.00%	13.375%
27	5.640	1401	1415	1437	rBV	498946	999093	60.86%	8.140%
28	5.846	1475	1479	1482	rVB3	1244	987	0.06%	0.008%
29	5.933	1495	1506	1518	rVB3	6634	14357	0.87%	0.117%
30	5.997	1522	1526	1529	rVB3	1243	887	0.05%	0.007%
31	6.093	1542	1556	1574	rBV	358946	725020	44.16%	5.907%
32	6.341	1629	1633	1635	rBV4	1398	1089	0.07%	0.009%
33	6.434	1659	1662	1665	rBV4	1629	875	0.05%	0.007%
34	6.527	1689	1691	1695	rVV5	1187	773	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016552.D
 Acq On : 05 Jun 2020 22:30
 Operator : SY/MD
 Sample : VV0605WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK69

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.569	1701	1704	1705	rBV3	1382	706	0.04%	0.006%
36	6.621	1717	1720	1723	rBV5	1329	1126	0.07%	0.009%
37	6.714	1747	1749	1752	rVB3	1397	725	0.04%	0.006%
38	6.756	1760	1762	1766	rVB4	1340	739	0.05%	0.006%
39	6.823	1781	1783	1787	rVB5	1996	1359	0.08%	0.011%
40	6.871	1795	1798	1806	rVB8	1396	1949	0.12%	0.016%
41	6.907	1806	1809	1813	rBV4	1965	1643	0.10%	0.013%
42	7.007	1829	1840	1865	rBV2	200218	357642	21.78%	2.914%
43	7.241	1910	1913	1918	rBV7	1976	1590	0.10%	0.013%
44	7.338	1931	1943	1960	rBV	748450	1267341	77.20%	10.325%
45	7.640	2027	2037	2058	rBV2	142964	241702	14.72%	1.969%
46	7.762	2073	2075	2076	rBV2	1297	627	0.04%	0.005%
47	7.974	2137	2141	2143	rBV4	1318	1009	0.06%	0.008%
48	8.039	2159	2161	2164	rVB3	1388	610	0.04%	0.005%
49	8.068	2167	2170	2171	rBV2	1989	1138	0.07%	0.009%
50	8.106	2172	2182	2211	rVV	465299	803551	48.95%	6.547%
51	8.595	2332	2334	2340	rBV6	1115	978	0.06%	0.008%
52	8.678	2358	2360	2364	rVB4	1347	923	0.06%	0.008%
53	8.875	2409	2421	2443	rBV	741840	1187125	72.31%	9.672%
54	9.039	2465	2472	2473	rBV4	7159	7405	0.45%	0.060%
55	9.231	2529	2532	2536	rBV7	1324	1217	0.07%	0.010%
56	9.299	2548	2553	2558	rBV7	1564	1674	0.10%	0.014%
57	9.347	2565	2568	2569	rBV3	911	609	0.04%	0.005%
58	9.685	2671	2673	2677	rVB3	1188	837	0.05%	0.007%
59	9.714	2677	2682	2685	rBV4	1154	999	0.06%	0.008%
60	9.881	2731	2734	2736	rBV4	1327	824	0.05%	0.007%
61	10.074	2792	2794	2797	rVB3	1298	718	0.04%	0.006%
62	10.093	2797	2800	2802	rBV4	1075	649	0.04%	0.005%
63	10.141	2812	2815	2817	rBV4	1020	762	0.05%	0.006%
64	10.238	2833	2845	2862	rBV	474759	746101	45.45%	6.079%
65	10.347	2876	2879	2880	rBV	1317	857	0.05%	0.007%
66	10.395	2891	2894	2901	rVB7	1601	1478	0.09%	0.012%
67	10.450	2906	2911	2914	rBV6	1749	1687	0.10%	0.014%
68	10.485	2921	2922	2926	rBV3	913	622	0.04%	0.005%
69	10.543	2937	2940	2942	rBV4	1410	903	0.06%	0.007%
70	10.559	2942	2945	2947	rBV4	1909	1281	0.08%	0.010%
71	10.759	3003	3007	3012	rVB8	1713	1533	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016552.D
 Acq On : 05 Jun 2020 22:30
 Operator : SY/MD
 Sample : VV0605WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK69

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.784	3012	3015	3017	rBV3	1247	1006	0.06%	0.008%
73	11.032	3090	3092	3096	rBV4	1275	872	0.05%	0.007%
74	11.270	3155	3166	3185	rBV	737449	1135582	69.17%	9.252%
75	11.453	3221	3223	3228	rVB5	1139	990	0.06%	0.008%
76	11.495	3233	3236	3240	rBV5	882	804	0.05%	0.007%
77	11.524	3243	3245	3248	rVB4	1301	734	0.04%	0.006%
78	11.543	3248	3251	3252	rBV3	1254	622	0.04%	0.005%
79	11.646	3272	3283	3302	rBV	764226	1195445	72.82%	9.739%
80	11.894	3358	3360	3362	rBV3	1296	692	0.04%	0.006%
81	11.932	3370	3372	3376	rVB5	1122	796	0.05%	0.006%
82	12.096	3420	3423	3425	rBV3	1277	990	0.06%	0.008%
83	12.148	3436	3439	3441	rBV4	1097	714	0.04%	0.006%
84	12.183	3443	3450	3455	rBV8	2063	2717	0.17%	0.022%
85	12.495	3544	3547	3550	rVB4	1594	965	0.06%	0.008%
86	12.521	3553	3555	3559	rVV3	1185	732	0.04%	0.006%
87	12.633	3587	3590	3593	rBV4	1168	993	0.06%	0.008%
88	12.813	3642	3646	3649	rBV5	1313	1075	0.07%	0.009%
89	12.839	3649	3654	3658	rBV6	1254	1503	0.09%	0.012%
90	12.945	3684	3687	3688	rBV2	1304	636	0.04%	0.005%
91	13.235	3775	3777	3782	rBV3	873	727	0.04%	0.006%
92	13.440	3835	3841	3845	rBV7	1762	2366	0.14%	0.019%
93	13.530	3864	3869	3880	rVB4	5932	8554	0.52%	0.070%
94	13.768	3937	3943	3951	rVB9	5129	8045	0.49%	0.066%
95	14.103	4045	4047	4050	rVB3	1483	715	0.04%	0.006%
96	14.141	4057	4059	4061	rBV2	1164	628	0.04%	0.005%
97	14.170	4066	4068	4070	rBV3	1704	1099	0.07%	0.009%
98	14.196	4073	4076	4077	rBV2	1885	979	0.06%	0.008%
99	14.231	4085	4087	4092	rVB5	2024	1536	0.09%	0.013%
100	14.553	4183	4187	4192	rBV7	1561	1828	0.11%	0.015%


Sum of corrected areas: 12274250

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016552.D
Acq On : 05 Jun 2020 22:30
Operator : SY/MD
Sample : VV0605WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK69

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

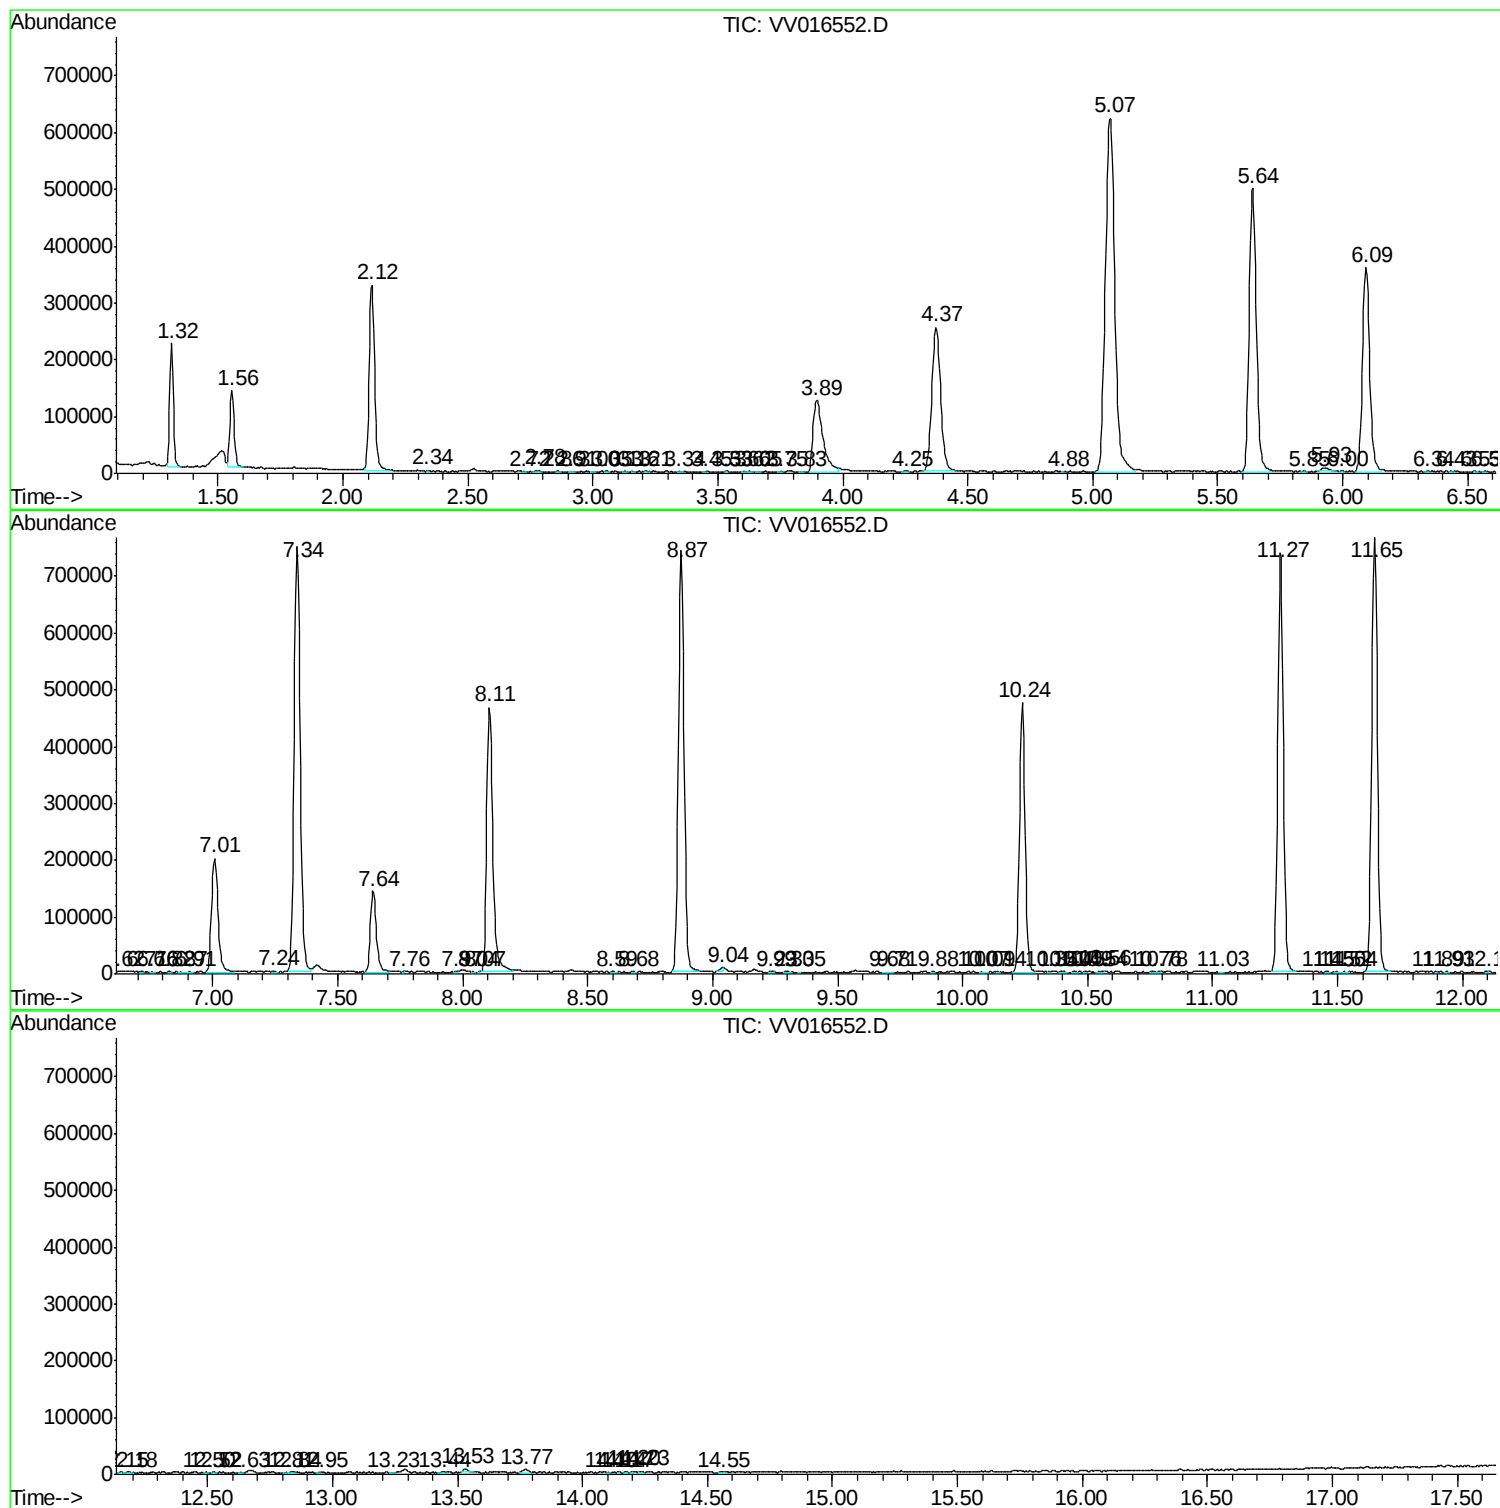

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016552.D
Acq On : 05 Jun 2020 22:30
Operator : SY/MD
Sample : VV0605WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK69

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016552.D
Acq On : 05 Jun 2020 22:30
Operator : SY/MD
Sample : VV0605WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK69

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc