

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016553.D
 Acq On : 05 Jun 2020 22:54
 Operator : SY/MD
 Sample : L2872-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEN7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	81	rVB	197575	199240	13.46%	1.712%
2	1.557	139	145	156	rVB	130512	154595	10.44%	1.329%
3	2.116	310	319	333	rVB	295297	427183	28.86%	3.671%
4	2.634	470	480	496	rVB2	6523	14397	0.97%	0.124%
5	2.765	518	521	524	rBV4	1961	1353	0.09%	0.012%
6	2.933	570	573	576	rBV4	1135	837	0.06%	0.007%
7	3.132	632	635	639	rBV5	1267	976	0.07%	0.008%
8	3.254	670	673	676	rVB5	1678	1059	0.07%	0.009%
9	3.273	676	679	681	rBV4	992	786	0.05%	0.007%
10	3.347	700	702	705	rBV3	1775	1020	0.07%	0.009%
11	3.425	724	726	730	rBV4	1362	1006	0.07%	0.009%
12	3.492	744	747	751	rBV4	1290	1105	0.07%	0.009%
13	3.515	751	754	756	rBV3	1379	782	0.05%	0.007%
14	3.675	801	804	807	rBV3	921	708	0.05%	0.006%
15	3.897	863	873	912	rBV2	117895	362610	24.50%	3.116%
16	4.248	980	982	987	rBV5	873	600	0.04%	0.005%
17	4.373	1005	1021	1043	rBV	231493	562928	38.03%	4.837%
18	4.534	1068	1071	1074	rBV3	1336	821	0.06%	0.007%
19	4.601	1090	1092	1096	rVB2	1077	650	0.04%	0.006%
20	4.624	1096	1099	1101	rVB4	1149	620	0.04%	0.005%
21	4.643	1103	1105	1107	rBV3	1452	792	0.05%	0.007%
22	4.685	1114	1118	1120	rBV3	2939	1966	0.13%	0.017%
23	4.955	1197	1202	1203	rBV5	1705	1382	0.09%	0.012%
24	5.068	1216	1237	1268	rBV2	570370	1480196	100.00%	12.720%
25	5.338	1318	1321	1322	rBV2	1243	616	0.04%	0.005%
26	5.479	1362	1365	1367	rVB4	1547	939	0.06%	0.008%
27	5.508	1367	1374	1376	rBV4	1440	1543	0.10%	0.013%
28	5.521	1376	1378	1385	rVB7	1744	1859	0.13%	0.016%
29	5.553	1385	1388	1390	rBV4	1325	947	0.06%	0.008%
30	5.640	1401	1415	1437	rBV	503263	998870	67.48%	8.584%
31	5.933	1498	1506	1507	rBV8	4712	5760	0.39%	0.049%
32	6.093	1544	1556	1575	rBV	323919	643511	43.47%	5.530%
33	6.457	1667	1669	1673	rBV3	1013	798	0.05%	0.007%
34	6.537	1691	1694	1699	rBV6	1763	1451	0.10%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016553.D
 Acq On : 05 Jun 2020 22:54
 Operator : SY/MD
 Sample : L2872-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFEN7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.598	1709	1713	1716	rBV5	1497	1596	0.11%	0.014%
36	6.640	1723	1726	1729	rBV3	1592	1133	0.08%	0.010%
37	6.781	1767	1770	1772	rBV4	820	627	0.04%	0.005%
38	7.006	1828	1840	1861	rBV2	168585	302091	20.41%	2.596%
39	7.215	1901	1905	1909	rBV6	1125	1110	0.07%	0.010%
40	7.338	1929	1943	1960	rBV	677125	1163492	78.60%	9.998%
41	7.643	2028	2038	2054	rBV	117748	200370	13.54%	1.722%
42	7.997	2138	2148	2165	rVB	142616	239077	16.15%	2.054%
43	8.106	2172	2182	2203	rBV	412385	704005	47.56%	6.050%
44	8.447	2284	2288	2291	rBV6	1543	1194	0.08%	0.010%
45	8.531	2312	2314	2318	rBV5	1330	983	0.07%	0.008%
46	8.579	2325	2329	2330	rBV3	1270	858	0.06%	0.007%
47	8.817	2401	2403	2406	rVB4	1647	786	0.05%	0.007%
48	8.875	2406	2421	2440	rBV	734858	1202223	81.22%	10.331%
49	9.122	2496	2498	2502	rBV4	960	626	0.04%	0.005%
50	9.302	2551	2554	2558	rBV6	1155	806	0.05%	0.007%
51	9.341	2562	2566	2572	rVB7	699	702	0.05%	0.006%
52	9.469	2603	2606	2608	rBV3	1330	892	0.06%	0.008%
53	9.527	2622	2624	2630	rBV6	968	769	0.05%	0.007%
54	9.559	2630	2634	2636	rBV5	2149	1621	0.11%	0.014%
55	9.694	2673	2676	2679	rBV4	842	657	0.04%	0.006%
56	9.804	2707	2710	2711	rBV3	1180	604	0.04%	0.005%
57	9.884	2732	2735	2739	rBV5	1251	1186	0.08%	0.010%
58	9.923	2744	2747	2749	rBV4	971	606	0.04%	0.005%
59	10.010	2767	2774	2778	rBV8	1527	2127	0.14%	0.018%
60	10.071	2788	2793	2795	rBV4	1323	911	0.06%	0.008%
61	10.238	2834	2845	2865	rVB	435842	677117	45.75%	5.819%
62	10.447	2908	2910	2912	rBV3	1249	787	0.05%	0.007%
63	10.556	2938	2944	2946	rBV5	1952	2124	0.14%	0.018%
64	10.665	2972	2978	2981	rBV7	1914	1892	0.13%	0.016%
65	10.714	2990	2993	2995	rBV3	1168	786	0.05%	0.007%
66	10.756	3003	3006	3009	rBV4	1675	1404	0.09%	0.012%
67	10.849	3031	3035	3037	rBV3	1309	994	0.07%	0.009%
68	10.881	3040	3045	3048	rBV6	1777	1690	0.11%	0.015%
69	11.125	3117	3121	3124	rBV4	1718	1397	0.09%	0.012%
70	11.270	3156	3166	3183	rBV	741391	1137462	76.85%	9.775%
71	11.418	3210	3212	3214	rBV3	1815	852	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016553.D
Acq On : 05 Jun 2020 22:54
Operator : SY/MD
Sample : L2872-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEN7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Title : VOC Analysis

72	11.646	3272	3283	3302	rBV	683164	1070246	72.30%	9.197%
73	12.032	3400	3403	3405	rBV3	1205	761	0.05%	0.007%
74	12.045	3405	3407	3410	rBV4	1152	769	0.05%	0.007%
75	12.093	3418	3422	3425	rBV5	1365	1133	0.08%	0.010%
76	12.263	3472	3475	3479	rBV5	1264	1324	0.09%	0.011%
77	12.376	3504	3510	3513	rBV6	1531	1696	0.11%	0.015%
78	12.540	3557	3561	3563	rBV5	931	722	0.05%	0.006%
79	12.614	3581	3584	3586	rBV4	1274	705	0.05%	0.006%
80	12.736	3619	3622	3623	rBV3	1319	833	0.06%	0.007%
81	12.781	3631	3636	3643	rBV8	1290	1471	0.10%	0.013%
82	12.829	3647	3651	3652	rBV3	1200	804	0.05%	0.007%
83	13.074	3723	3727	3729	rBV4	1646	992	0.07%	0.009%
84	13.180	3757	3760	3762	rBV4	1410	647	0.04%	0.006%
85	13.241	3775	3779	3782	rBV3	1248	999	0.07%	0.009%
86	13.379	3819	3822	3824	rBV3	1609	941	0.06%	0.008%
87	13.460	3842	3847	3850	rBV6	1558	1054	0.07%	0.009%
88	13.530	3863	3869	3877	rVB6	5911	8328	0.56%	0.072%
89	13.652	3904	3907	3909	rBV3	1361	913	0.06%	0.008%
90	13.730	3928	3931	3933	rBV4	1400	866	0.06%	0.007%
91	13.743	3933	3935	3938	rBV2	980	623	0.04%	0.005%
92	13.881	3975	3978	3981	rBV3	912	705	0.05%	0.006%
93	13.968	4002	4005	4008	rBV5	965	859	0.06%	0.007%
94	14.019	4018	4021	4027	rBV6	1341	1273	0.09%	0.011%
95	14.077	4030	4039	4040	rBV8	1665	2001	0.14%	0.017%
96	14.119	4048	4052	4055	rBV5	1848	1667	0.11%	0.014%
97	14.199	4075	4077	4080	rBV4	1433	894	0.06%	0.008%
98	14.257	4093	4095	4100	rBV5	1106	687	0.05%	0.006%
99	14.292	4103	4106	4107	rBV2	1261	718	0.05%	0.006%
100	14.344	4120	4122	4124	rBV2	1219	665	0.04%	0.006%


Sum of corrected areas: 11636759

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016553.D
Acq On : 05 Jun 2020 22:54
Operator : SY/MD
Sample : L2872-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEN7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

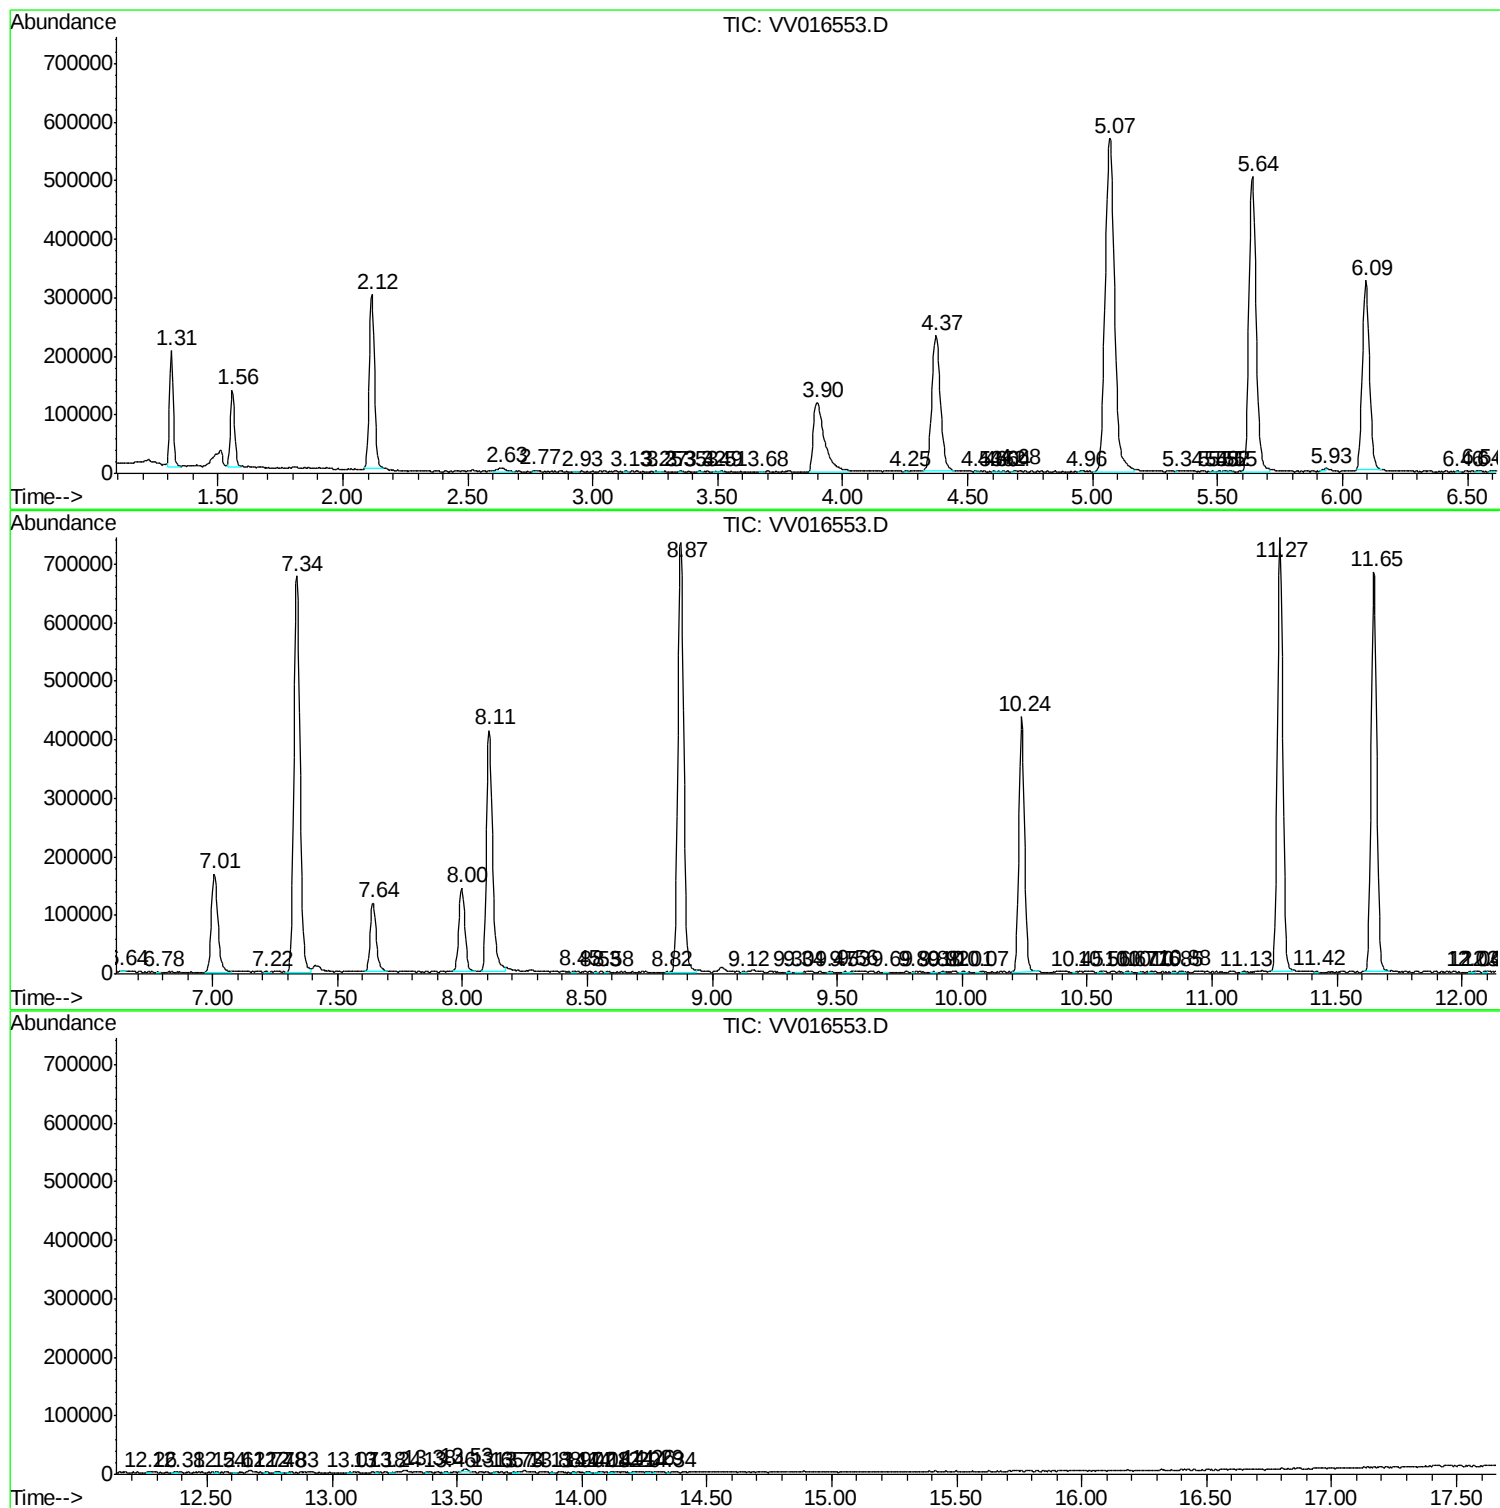

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016553.D
Acq On : 05 Jun 2020 22:54
Operator : SY/MD
Sample : L2872-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEN7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
Data File : VV016553.D
Acq On : 05 Jun 2020 22:54
Operator : SY/MD
Sample : L2872-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFEN7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc