


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060520\
 Data File : VV016523.D
 Acq On : 05 Jun 2020 09:59
 Operator : SY/MD
 Sample : BFB81
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB81

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis
 Last Update : Sun Jun 07 07:46:43 2020

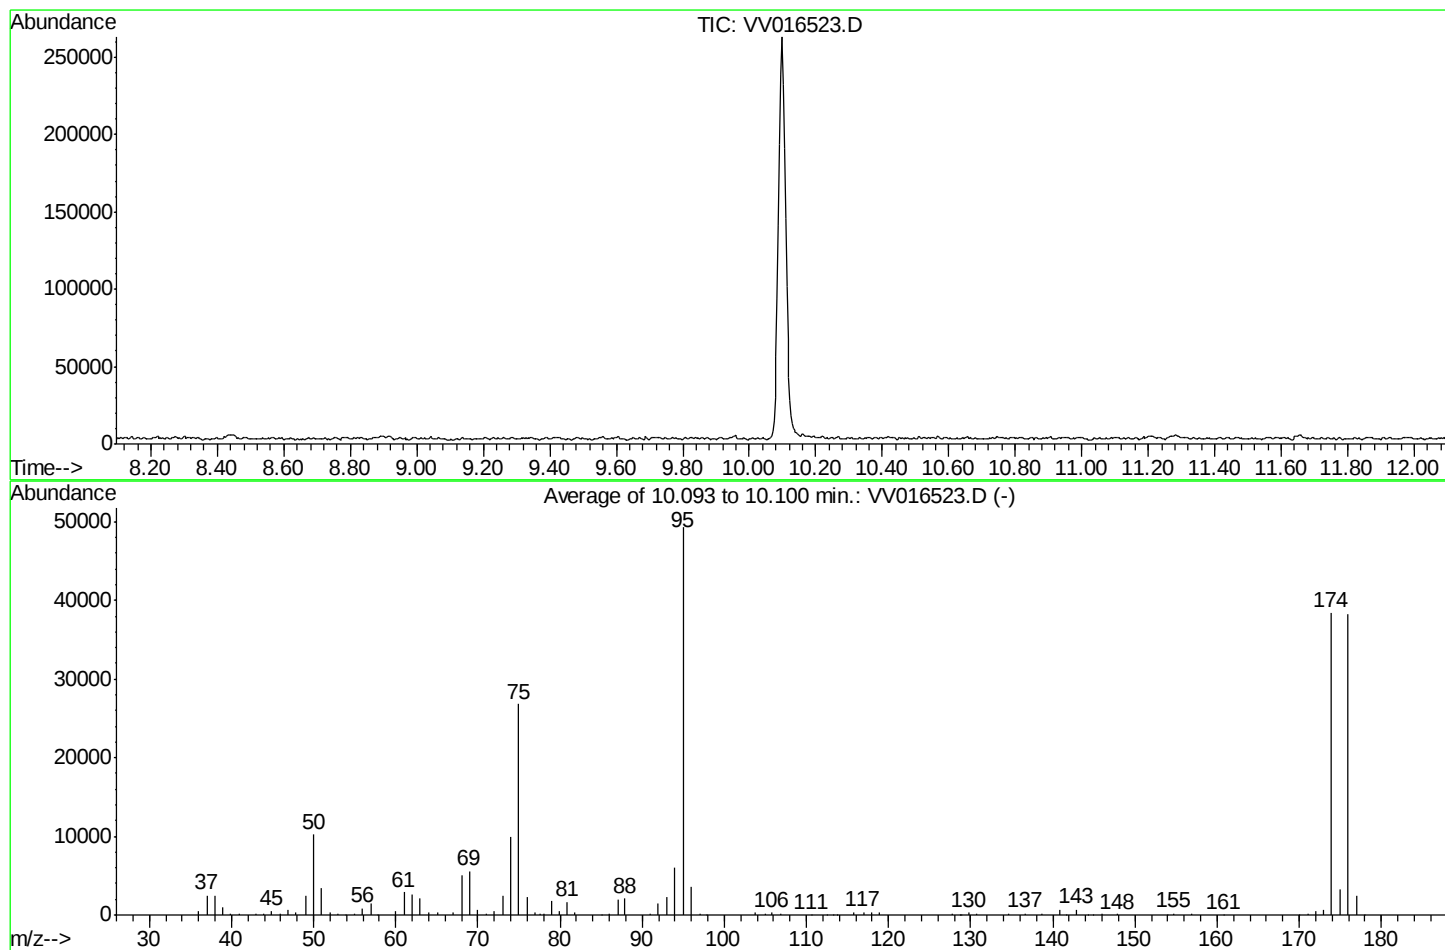

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	10250	PASS
75	95	30	80	54.3	26792	PASS
95	95	100	100	100.0	49301	PASS
96	95	5	9	7.2	3569	PASS
173	174	0.00	2	1.6	624	PASS
174	95	50	120	77.9	38424	PASS
175	174	5	9	8.5	3270	PASS
176	174	95	101	99.7	38306	PASS
177	176	5	9	6.2	2372	PASS

m/z	Abundance
35.20	166.0
35.70	143.0
36.30	110.0
37.00	156.0
38.00	188.0
38.90	137.0
39.90	312.0
42.10	159.0
43.90	529.0
44.80	153.0
47.80	107.0
48.70	151.0
53.20	123.0
55.30	105.0
57.70	112.0
58.90	109.0
60.00	113.0
63.80	106.0
73.60	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
36.00	513.0
37.00	2668.0
38.00	2466.0
39.00	1214.0
39.90	412.0
40.90	115.0
42.90	105.0
43.90	719.0
45.00	533.0
46.10	202.0
46.90	643.0
47.90	475.0
49.00	2265.0
50.00	9842.0
51.00	3176.0
52.00	275.0
52.90	119.0
55.00	236.0
56.00	873.0
57.00	1427.0
57.80	121.0
58.90	128.0
59.90	533.0
61.00	2809.0
62.00	2443.0
63.00	1978.0
64.00	348.0
65.10	376.0
67.00	234.0
68.00	4882.0
69.00	5287.0
70.00	619.0
70.90	156.0
72.00	442.0
73.00	2389.0
74.00	9277.0
75.00	25344.0
76.00	2217.0
76.90	277.0
77.60	231.0
78.10	255.0
78.90	1586.0
80.00	541.0
80.90	1661.0
81.80	398.0
85.10	110.0
86.00	123.0
87.00	1935.0
87.90	2014.0
91.00	201.0
91.90	1353.0
93.00	2180.0
94.00	5725.0
95.00	46960.0
96.00	3386.0
97.00	157.0
97.90	125.0
103.80	242.0
105.00	154.0
105.80	273.0
106.90	129.0
113.70	107.0
115.80	231.0
117.00	323.0
117.90	203.0
118.90	299.0
127.80	168.0
128.70	115.0
129.80	242.0
130.80	144.0
134.70	127.0
136.70	186.0
138.60	109.0
140.80	472.0
142.90	665.0
148.00	147.0
154.00	112.0
154.80	165.0
156.90	149.0
169.90	106.0
171.00	113.0
172.00	332.0
173.00	646.0
173.90	35096.0
175.00	2974.0
175.90	35456.0
176.90	2236.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
36.00	549.0
37.00	2756.0
38.00	2695.0
39.00	1245.0
39.90	485.0
40.90	107.0
43.00	105.0
44.00	760.0
45.00	677.0
46.00	142.0
47.00	714.0
47.90	507.0
49.00	2482.0
50.00	10660.0
51.00	3516.0
52.00	268.0
52.90	139.0
53.90	111.0
54.90	220.0
56.00	918.0
57.00	1440.0
57.90	121.0
58.90	118.0
59.90	556.0
61.00	2976.0
62.00	2801.0
63.00	2101.0
64.00	382.0
65.10	377.0
67.00	271.0
68.00	5197.0
69.00	5828.0
70.00	646.0
71.00	129.0
72.00	445.0
73.00	2553.0
74.00	10490.0
75.00	27728.0
76.00	2382.0
76.90	327.0
78.00	223.0
78.90	1857.0
79.90	603.0
80.90	1700.0
81.80	406.0
86.00	178.0
87.00	2117.0
87.90	2102.0
90.90	171.0
92.00	1494.0
93.00	2404.0
94.00	6122.0
95.00	51104.0
96.00	3768.0
97.00	186.0
103.80	277.0
105.00	144.0
105.80	296.0
107.00	131.0
110.60	103.0
113.20	104.0
115.80	299.0
116.90	388.0
118.00	303.0
118.90	327.0
127.80	176.0
128.70	115.0
129.80	278.0
130.70	143.0
134.60	147.0
136.70	199.0
138.60	109.0
140.80	601.0
141.60	101.0
142.90	767.0
144.20	105.0
146.00	136.0
147.90	137.0
154.00	106.0
154.80	188.0
156.90	181.0
171.00	143.0
171.90	473.0
173.00	657.0
173.90	39840.0
175.00	3437.0
175.90	39832.0
177.00	2446.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81

m/z	Abundance
36.00	556.0
37.00	2559.0
38.00	2599.0
39.00	1134.0
39.90	491.0
41.00	105.0
43.10	144.0
44.00	705.0
44.90	728.0
45.90	142.0
47.00	688.0
47.80	513.0
49.00	2484.0
50.00	10248.0
51.00	3365.0
51.90	243.0
53.00	163.0
53.90	137.0
54.90	197.0
55.90	824.0
57.00	1421.0
58.00	134.0
59.90	520.0
61.00	2807.0
62.00	2809.0
63.00	2085.0
64.00	372.0
65.10	375.0
66.90	295.0
68.00	5102.0
69.00	5653.0
70.00	609.0
71.10	152.0
72.00	399.0
73.00	2428.0
74.00	10227.0
75.00	27304.0
76.00	2306.0
76.90	371.0
77.70	187.0
78.90	1962.0
79.80	575.0
80.90	1601.0
81.80	383.0
86.10	200.0
87.00	2002.0
87.90	2108.0
90.80	228.0
92.00	1582.0
93.00	2426.0
94.00	6049.0
95.00	49840.0
96.00	3554.0
97.00	200.0
103.80	268.0
105.00	145.0
105.80	274.0
106.80	128.0
110.70	109.0
112.50	111.0
115.80	298.0
116.90	444.0
118.00	393.0
118.90	338.0
127.80	214.0
128.90	142.0
129.80	242.0
130.70	118.0
134.60	152.0
136.70	175.0
138.70	101.0
140.80	658.0
141.70	107.0
142.90	776.0
144.20	126.0
144.90	140.0
146.00	137.0
147.80	142.0
154.70	180.0
156.90	152.0
160.80	104.0
171.00	180.0
171.90	603.0
172.90	570.0
173.90	40336.0
174.90	3400.0
175.90	39632.0
177.00	2436.0
177.90	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB81