




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031338.D
 Acq On : 05 Jun 2023 11:06
 Operator : SY/MD
 Sample : VV0605WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK346

Manual IntegrationsAPPROVED

Quant Time: Jun 06 02:06:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 06 02:05:53 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/06/2023
 Supervised By :Mahesh Dadoda 06/08/2023

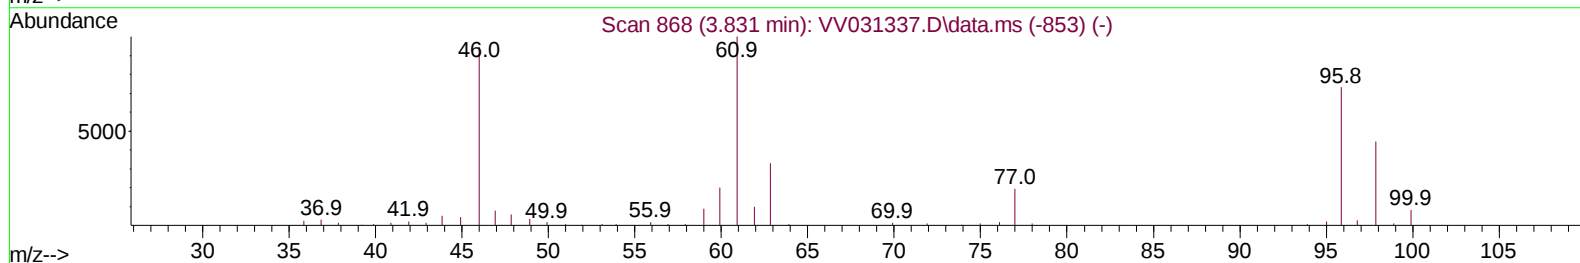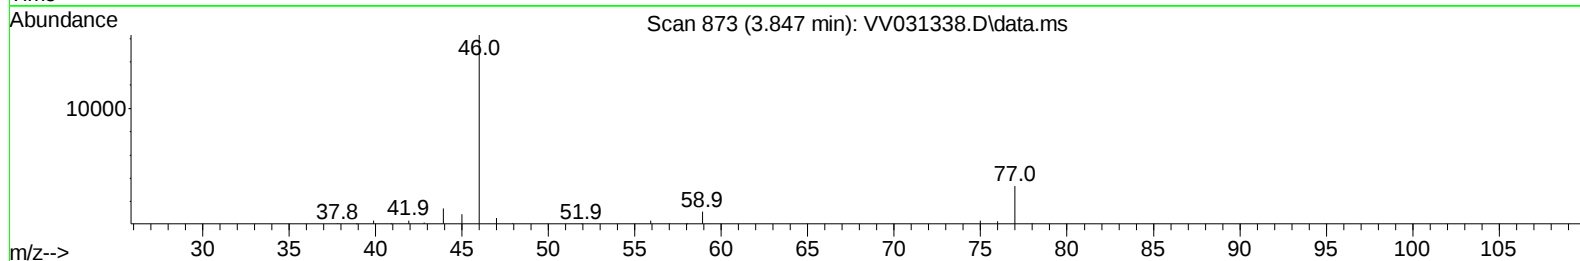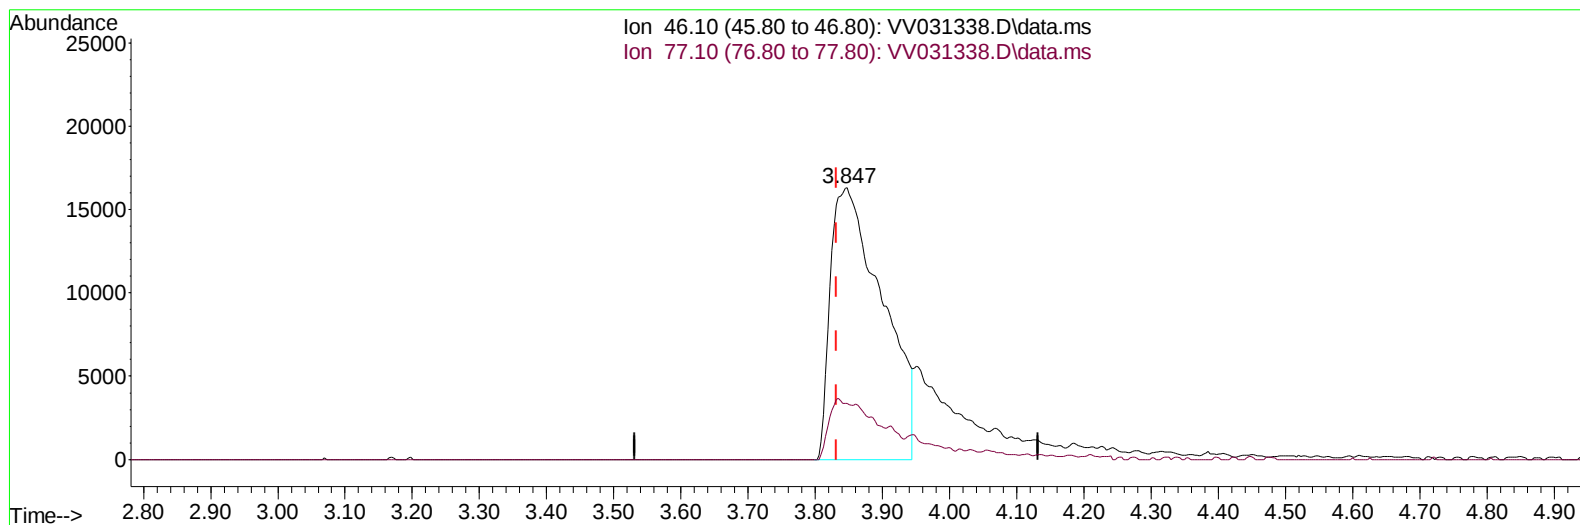

TIC: VV031338.D\data.ms

(20) 2-Butanone-d5 (S)

3.847min (+ 0.016) 31.28 ug/L

response 87532

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	15.40	9.68#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031338.D
 Acq On : 05 Jun 2023 11:06
 Operator : SY/MD
 Sample : VV0605WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK346

Manual IntegrationsAPPROVED

Quant Time: Jun 06 02:06:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 06 02:05:53 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/06/2023
 Supervised By :Mahesh Dadoda 06/08/2023

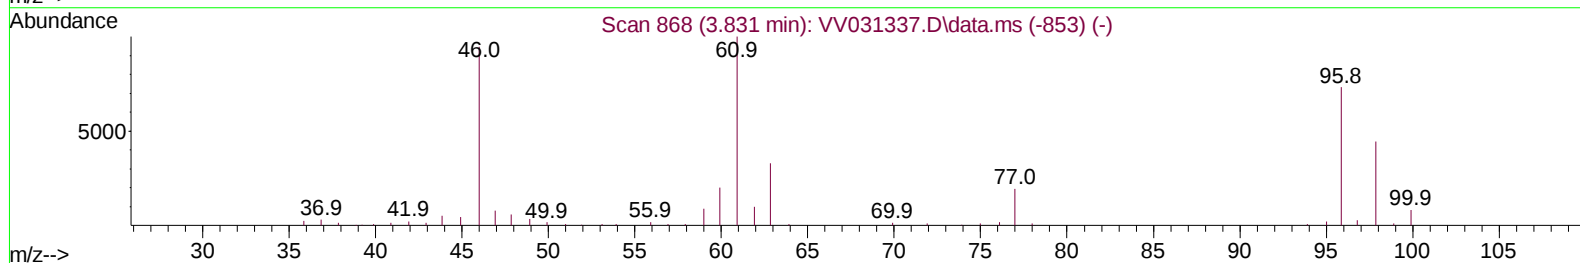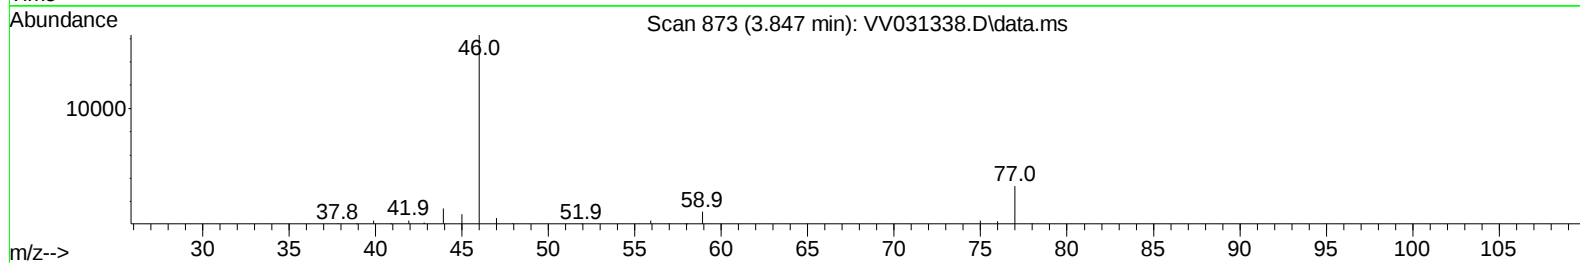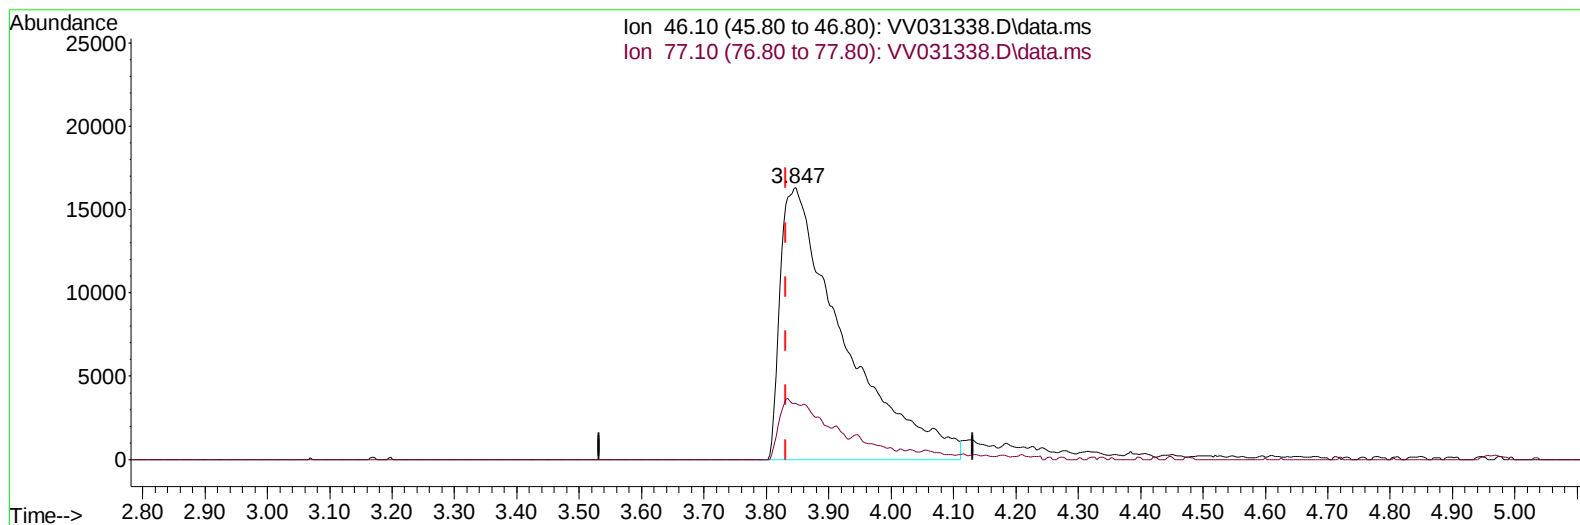

TIC: VV031338.D\data.ms

(20) 2-Butanone-d5 (S)

3.847min (+ 0.016) 40.95 ug/L m

response 114578

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	15.40	7.39#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031338.D
 Acq On : 05 Jun 2023 11:06
 Operator : SY/MD
 Sample : VV0605WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK346

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/06/2023
 Supervised By :Mahesh Dadoda 06/08/2023

Quant Time: Jun 06 02:06:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 06 02:05:53 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.542	114		118846	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117		123489	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152		55901	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.275	65		48680	4.027	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.600%	
7) Chloroethane-d5	1.532	69		44969	4.404	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.000%	
11) 1,1-Dichloroethene-d2	2.060	65		25709	4.380	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.600%	
20) 2-Butanone-d5	3.847	46		114578m	40.948	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	81.900%	
24) Chloroform-d	4.256	84		105859	5.208	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.200%	
26) 1,2-Dichloroethane-d4	4.950	65		55130	5.057	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.200%	
32) Benzene-d6	4.966	84		175935	4.686	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.800%	
36) 1,2-Dichloropropane-d6	5.995	67		61146	4.822	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.400%	
41) Toluene-d8	7.249	98		147933	4.196	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.000%	
43) trans-1,3-Dichloroprop...	7.561	79		19634	4.253	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.000%	
46) 2-Hexanone-d5	8.037	63		73465	39.615	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.220%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		42231	4.381	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.600%	
66) 1,2-Dichlorobenzene-d4	11.567	152		52344	4.965	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.200%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031338.D
Acq On : 05 Jun 2023 11:06
Operator : SY/MD
Sample : VV0605WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK346

Manual IntegrationsAPPROVED

Quant Time: Jun 06 02:06:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 06 02:05:53 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/06/2023
Supervised By :Mahesh Dadoda 06/08/2023

