




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031348.D
 Acq On : 05 Jun 2023 15:41
 Operator : SY/MD
 Sample : 02990-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C00

Manual IntegrationsAPPROVED

Quant Time: Jun 06 02:09:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 06 02:05:53 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/06/2023
 Supervised By :Mahesh Dadoda 06/08/2023

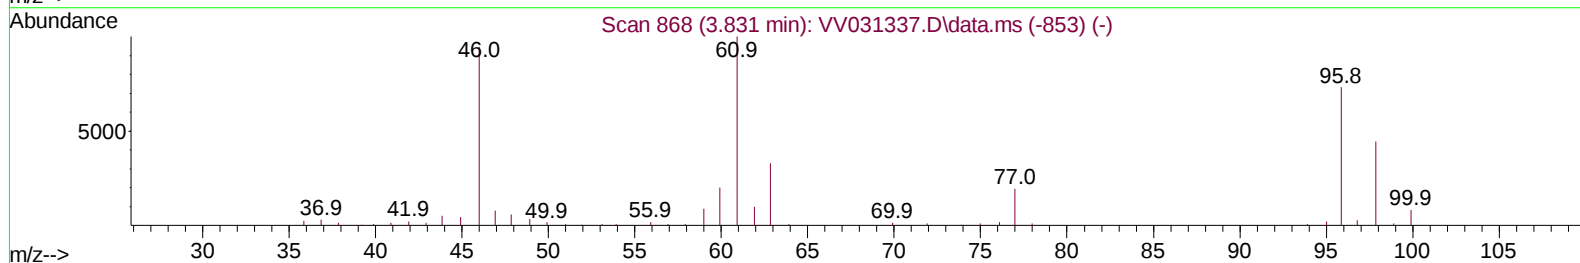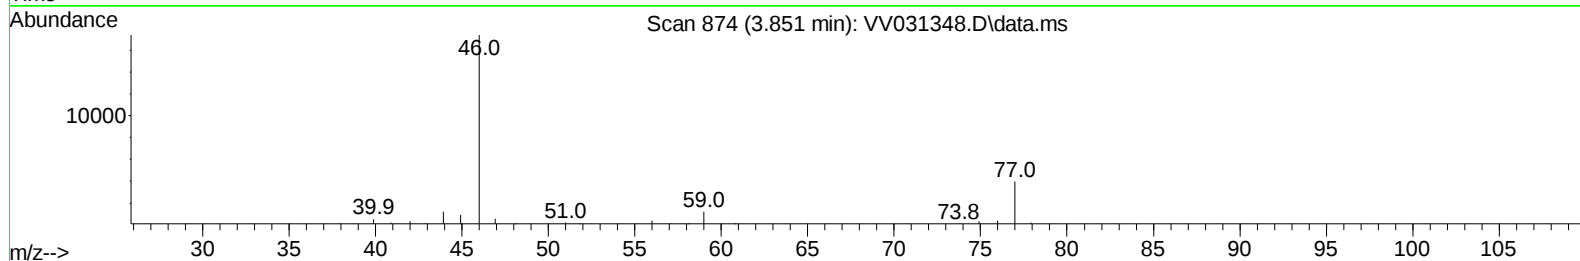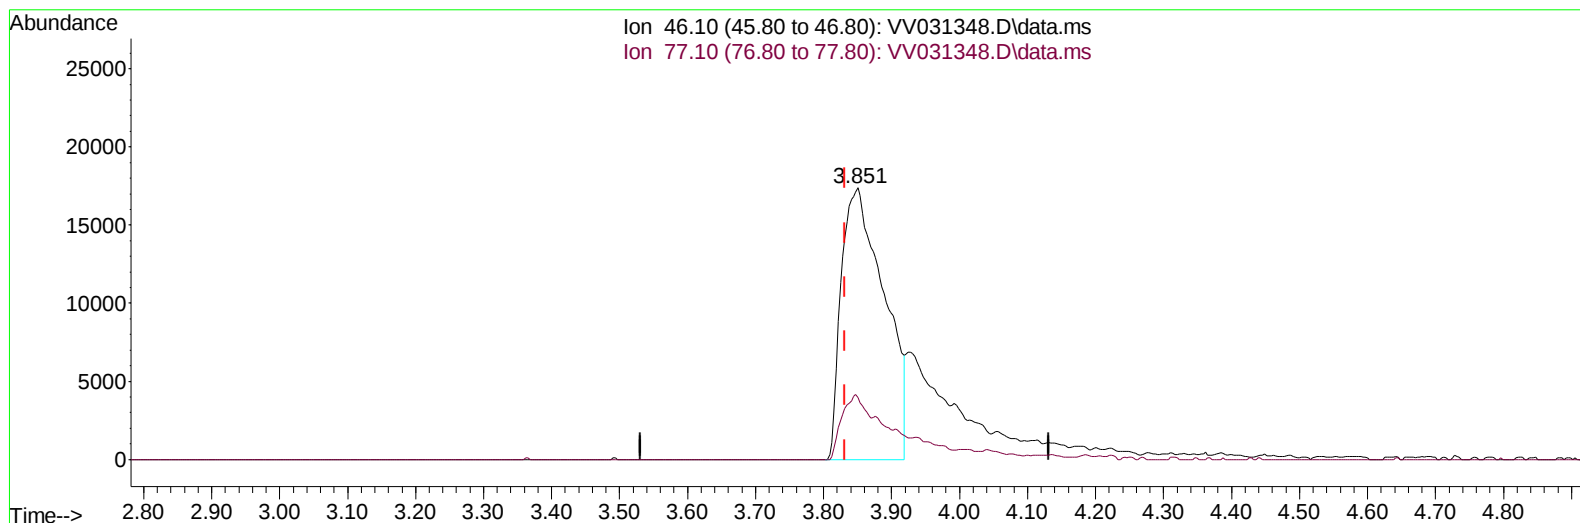

TIC: VV031348.D\data.ms

(20) 2-Butanone-d5 (S)

3.851min (+ 0.019) 27.98 ug/L

response 76011

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	15.40	19.69
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031348.D
Acq On : 05 Jun 2023 15:41
Operator : SY/MD
Sample : 02990-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C00

Manual IntegrationsAPPROVED

Quant Time: Jun 06 02:09:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123wMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 06 02:05:53 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/06/2023
Supervised By :Mahesh Dadoda 06/08/2023

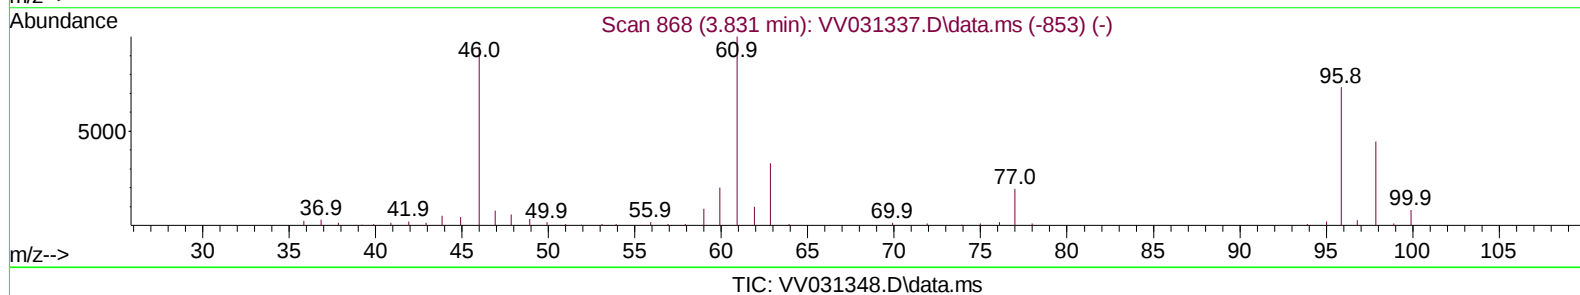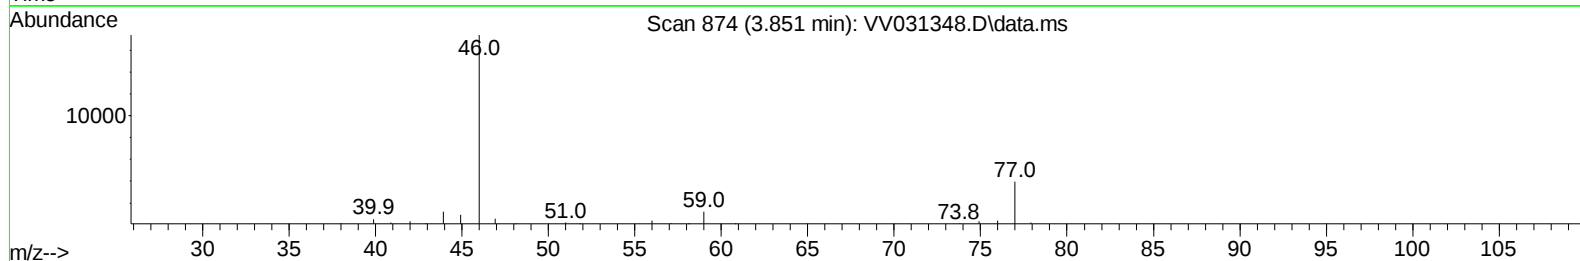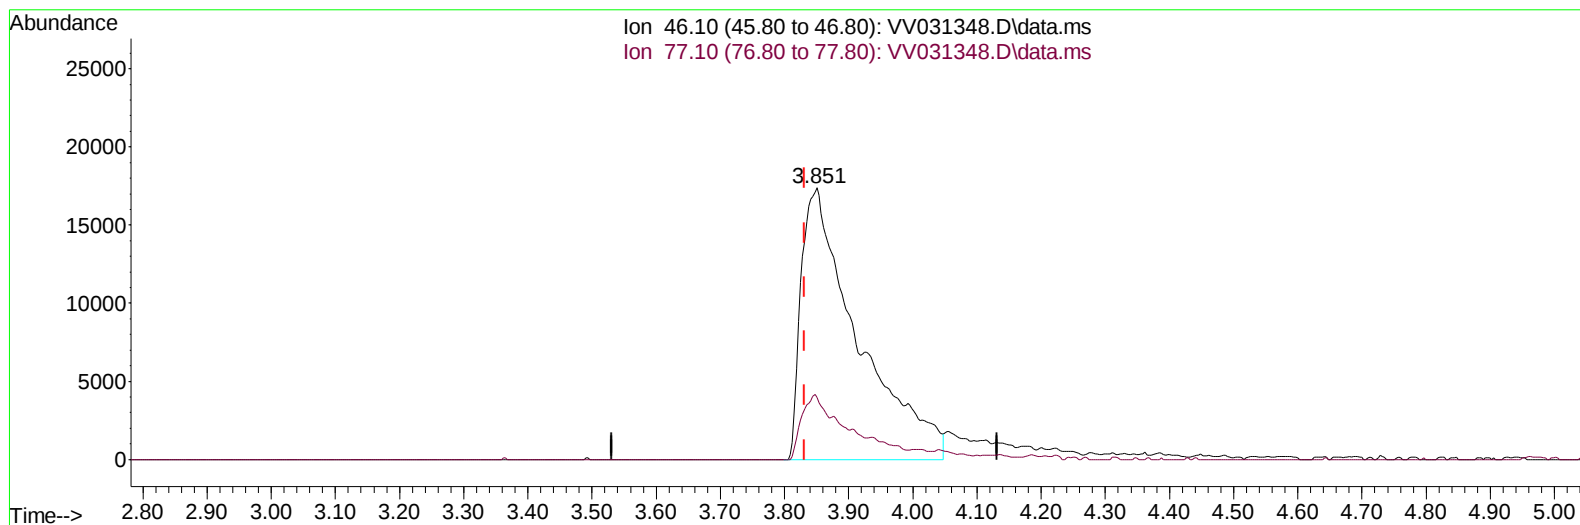

(20) 2-Butanone-d5 (S)

3.851min (+ 0.019) 39.05 ug/L m

response 106094

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	15.40	14.11
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031348.D
 Acq On : 05 Jun 2023 15:41
 Operator : SY/MD
 Sample : 02990-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C00

Manual IntegrationsAPPROVED

Quant Time: Jun 06 02:09:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 06 02:05:53 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/06/2023
 Supervised By :Mahesh Dadoda 06/08/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.542	114		115386	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117		120627	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152		54463	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.275	65		46536	3.965	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	79.200%	
7) Chloroethane-d5	1.532	69		42398	4.276	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	85.600%	
11) 1,1-Dichloroethene-d2	2.060	65		25082	4.401	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	88.000%	
20) 2-Butanone-d5	3.851	46		106094m	39.053	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130		Recovery	=	78.100%	
24) Chloroform-d	4.256	84		99985	5.067	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	101.400%	
26) 1,2-Dichloroethane-d4	4.953	65		51943	4.908	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	98.200%	
32) Benzene-d6	4.966	84		169661	4.627	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	92.600%	
36) 1,2-Dichloropropane-d6	5.995	67		59132	4.774	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	95.400%	
41) Toluene-d8	7.249	98		142297	4.132	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	82.600%	
43) trans-1,3-Dichloroprop...	7.564	79		19225	4.263	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	85.200%	
46) 2-Hexanone-d5	8.040	63		66246	36.569	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	73.140%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		37247	3.956	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	79.200%	
66) 1,2-Dichlorobenzene-d4	11.567	152		50452	4.912	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	98.200%	
Target Compounds							
47) Tetrachloroethene	7.921	164		1202	0.133	ug/L #	Qvalue 75

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031348.D
Acq On : 05 Jun 2023 15:41
Operator : SY/MD
Sample : 02990-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C00

Manual IntegrationsAPPROVED

Quant Time: Jun 06 02:09:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 06 02:05:53 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/06/2023
Supervised By :Mahesh Dadoda 06/08/2023

