




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031352.D
Acq On : 05 Jun 2023 17:14
Operator : SY/MD
Sample : 02990-07 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C32

Manual IntegrationsAPPROVED

Quant Time: Jun 06 02:09:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123wMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 06 02:05:53 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/06/2023
Supervised By :Mahesh Dadoda 06/08/2023

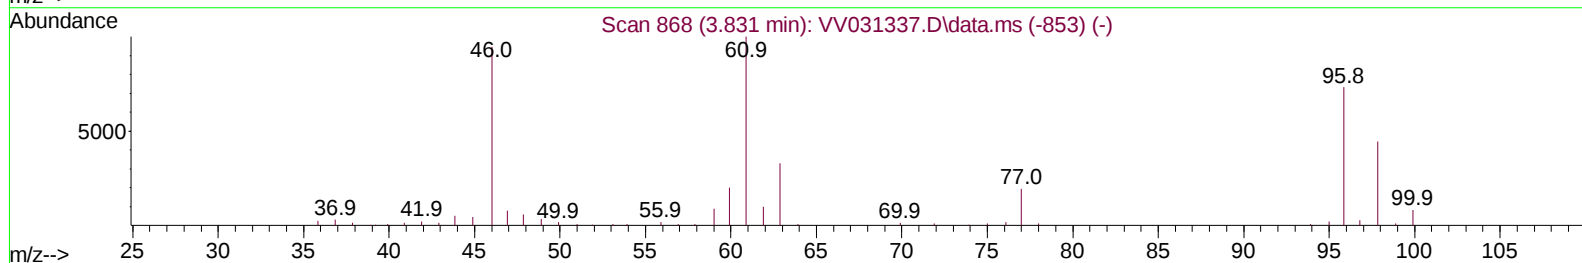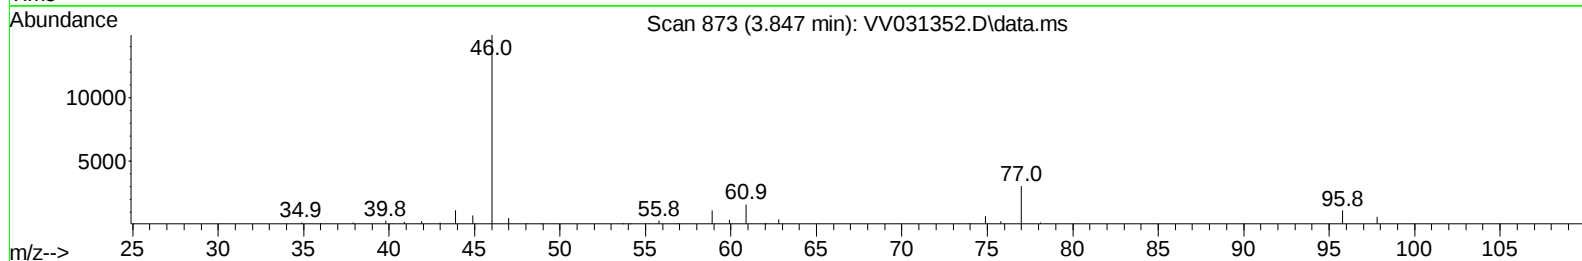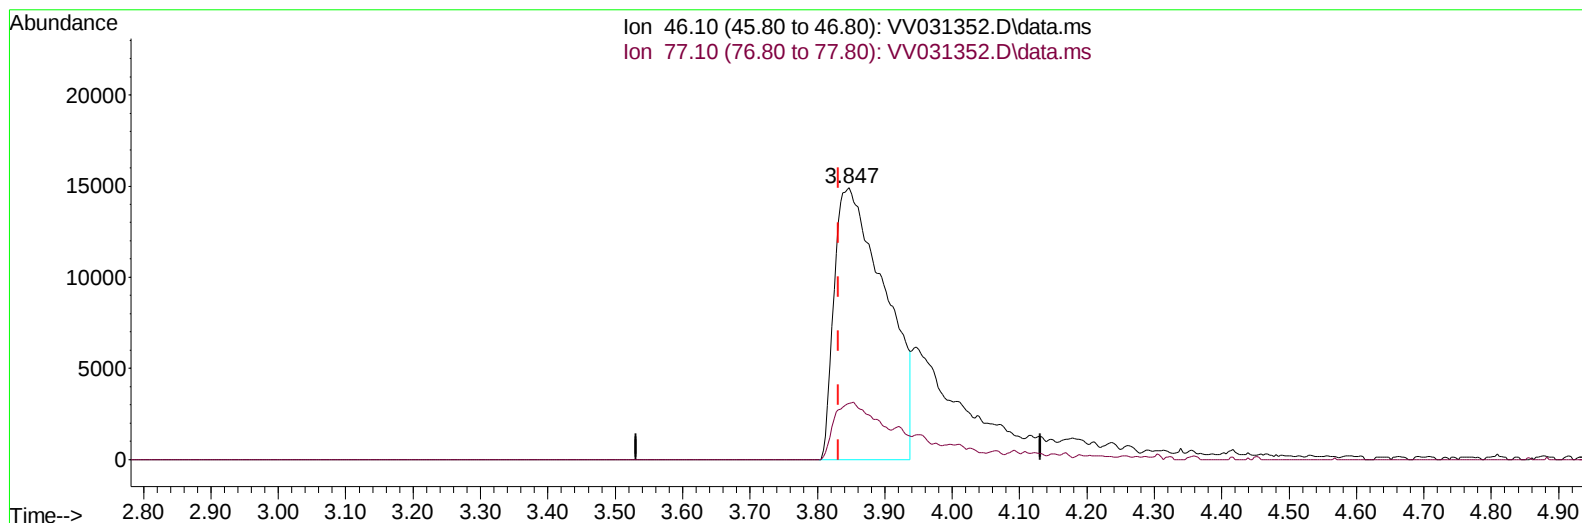

TIC: VV031352.D\data.ms

(20) 2-Butanone-d5 (S)

3.847min (+ 0.016) 25.28 ug/L

response 78102

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	15.40	17.68
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031352.D
 Acq On : 05 Jun 2023 17:14
 Operator : SY/MD
 Sample : 02990-07 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C32

Manual IntegrationsAPPROVED

Quant Time: Jun 06 02:09:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 06 02:05:53 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/06/2023
 Supervised By :Mahesh Dadoda 06/08/2023

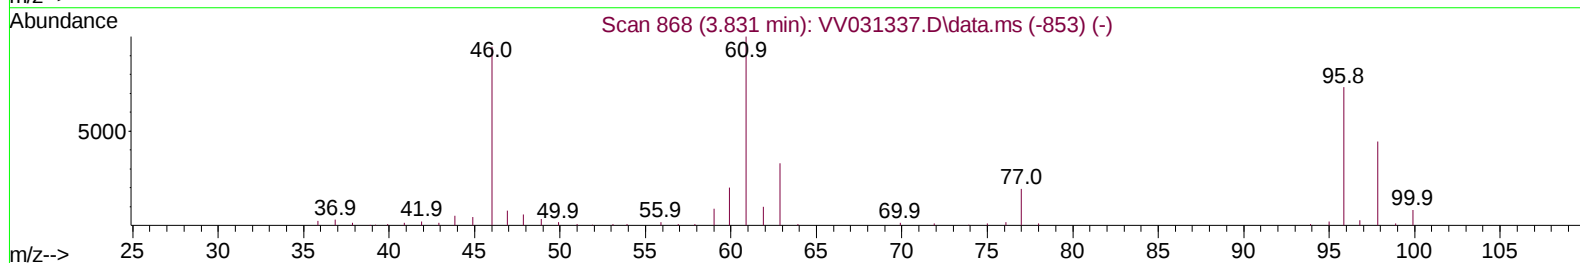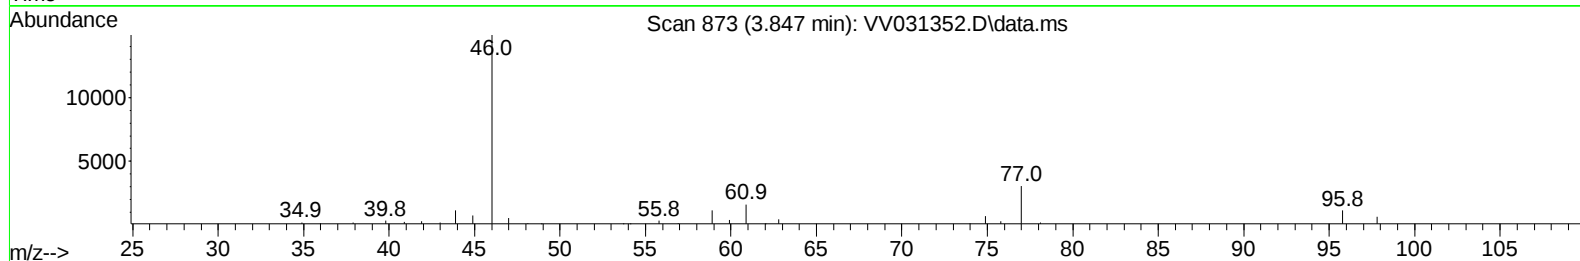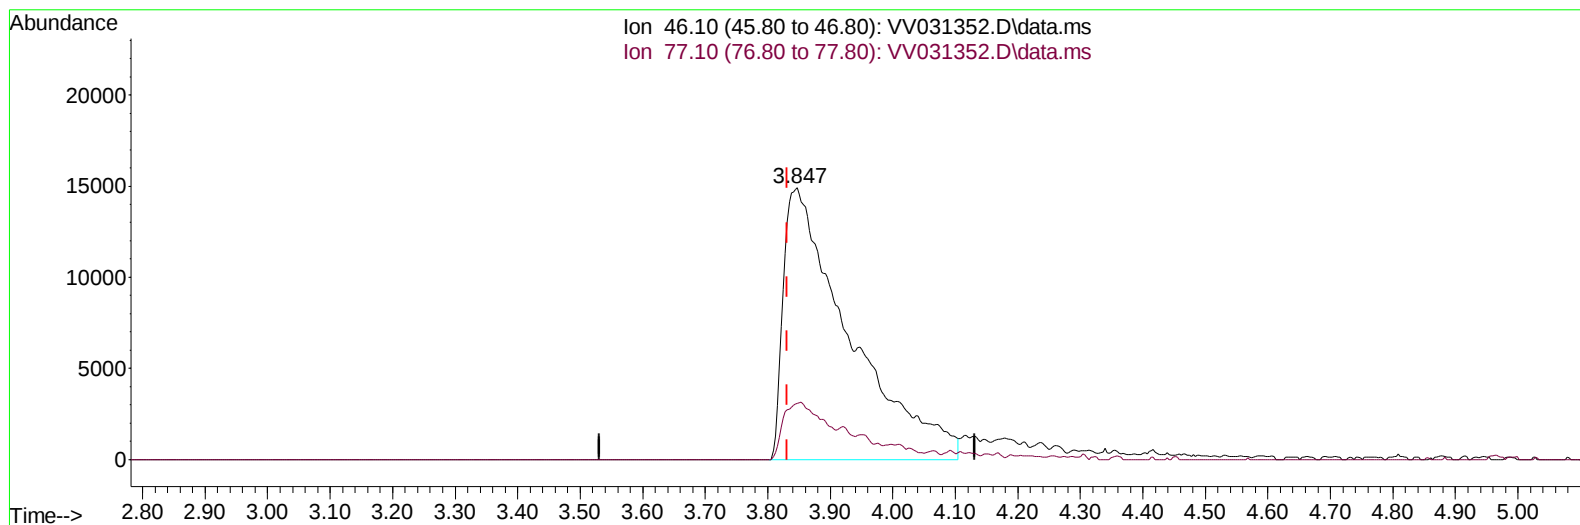

TIC: VV031352.D\data.ms

(20) 2-Butanone-d5 (S)

3.847min (+ 0.016) 35.27 ug/L m

response 108975

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	15.40	12.67
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031352.D
 Acq On : 05 Jun 2023 17:14
 Operator : SY/MD
 Sample : 02990-07 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C32

Manual IntegrationsAPPROVED

Quant Time: Jun 06 02:09:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jun 06 02:05:53 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/06/2023
 Supervised By :Mahesh Dadoda 06/08/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	131230	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	133915	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	59762	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	45801	3.431	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	68.600%		
7) Chloroethane-d5	1.532	69	41714	3.699	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	74.000%		
11) 1,1-Dichloroethene-d2	2.060	65	25175	3.884	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	77.600%		
20) 2-Butanone-d5	3.847	46	108975m	35.270	ug/L	0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	70.540%		
24) Chloroform-d	4.256	84	100166	4.463	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	89.200%		
26) 1,2-Dichloroethane-d4	4.950	65	51765	4.300	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	86.000%		
32) Benzene-d6	4.966	84	170229	4.181	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	83.600%		
36) 1,2-Dichloropropane-d6	5.995	67	61852	4.498	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	90.000%		
41) Toluene-d8	7.249	98	140169	3.666	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	73.400%		
43) trans-1,3-Dichloroprop...	7.564	79	18986	3.792	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	75.800%		
46) 2-Hexanone-d5	8.037	63	71100	35.354	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	70.700%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	39624	3.791	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	75.800%		
66) 1,2-Dichlorobenzene-d4	11.567	152	49587	4.399	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	88.000%		
Target Compounds						
16) Methylene chloride	2.452	84	3399	0.228	ug/L	98
22) cis-1,2-Dichloroethene	3.822	96	5385	0.457	ug/L	92
34) Trichloroethene	5.844	95	18366	1.427	ug/L	91
47) Tetrachloroethene	7.911	164	75293	7.507	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031352.D
Acq On : 05 Jun 2023 17:14
Operator : SY/MD
Sample : 02990-07 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C32

Manual IntegrationsAPPROVED

Quant Time: Jun 06 02:09:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jun 06 02:05:53 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/06/2023
Supervised By :Mahesh Dadoda 06/08/2023

