

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031343.D
 Acq On : 05 Jun 2023 13:39
 Operator : SY/MD
 Sample : VIBLK300
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK300

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031343.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	85	rVB	73465	79516	15.73%	2.050%
2	1.532	145	153	167	rVB	71414	84281	16.67%	2.173%
3	2.060	307	317	330	rBV	145033	211964	41.93%	5.466%
4	2.449	425	438	454	rBV	16798	29773	5.89%	0.768%
5	2.973	590	601	614	rVB5	4426	9272	1.83%	0.239%
6	3.835	858	869	883	rBV2	24596	85762	16.96%	2.211%
7	4.256	982	1000	1024	rBV	91037	237756	47.03%	6.131%
8	4.963	1203	1220	1247	rBV2	197285	505570	100.00%	13.036%
9	5.539	1388	1399	1425	rBV	133431	284500	56.27%	7.336%
10	5.834	1479	1491	1505	rBV	4193	10270	2.03%	0.265%
11	5.995	1527	1541	1580	rBV	118325	261623	51.75%	6.746%
12	6.921	1816	1829	1857	rBV2	43911	93926	18.58%	2.422%
13	7.249	1919	1931	1960	rBV	203642	376585	74.49%	9.710%
14	7.561	2017	2028	2054	rBV2	28621	58091	11.49%	1.498%
15	7.912	2128	2137	2153	rBV2	10694	19845	3.93%	0.512%
16	8.037	2164	2176	2215	rBV	168928	431598	85.37%	11.129%
17	8.793	2399	2411	2432	rBV	209646	358151	70.84%	9.235%
18	10.159	2825	2836	2859	rVB	83668	137164	27.13%	3.537%
19	11.191	3147	3157	3179	rBV	188713	297074	58.76%	7.660%
20	11.567	3260	3274	3291	rBV	190601	305411	60.41%	7.875%




Sum of corrected areas: 3878132

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031343.D
Acq On : 05 Jun 2023 13:39
Operator : SY/MD
Sample : VIBLK300
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK300

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

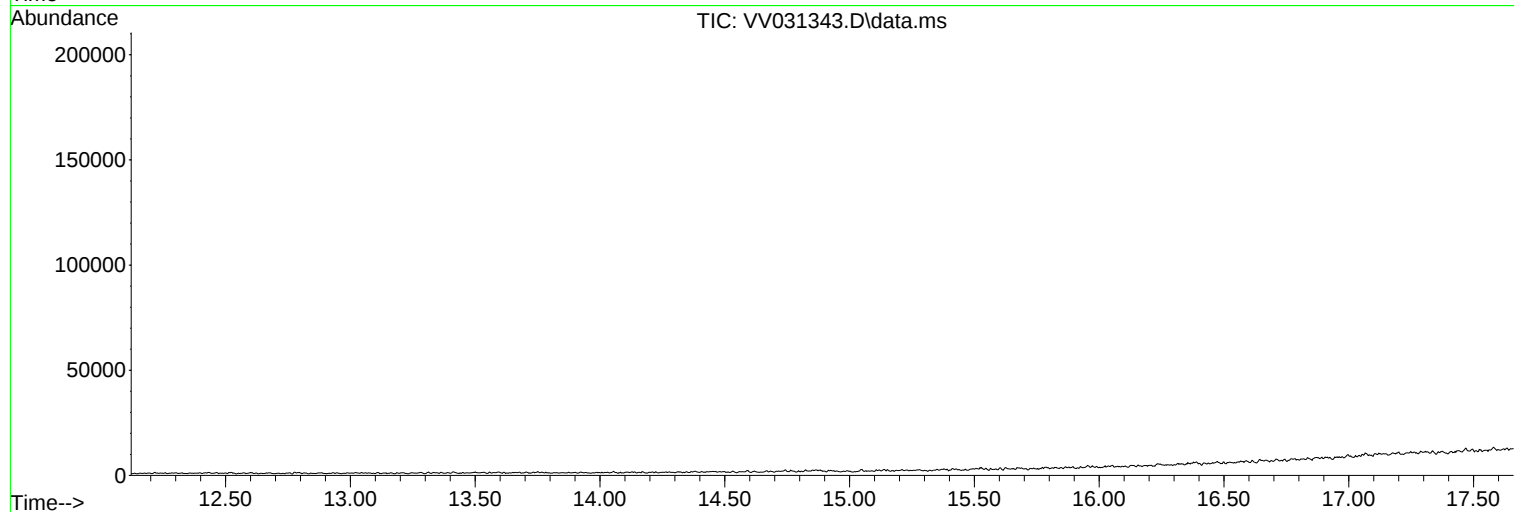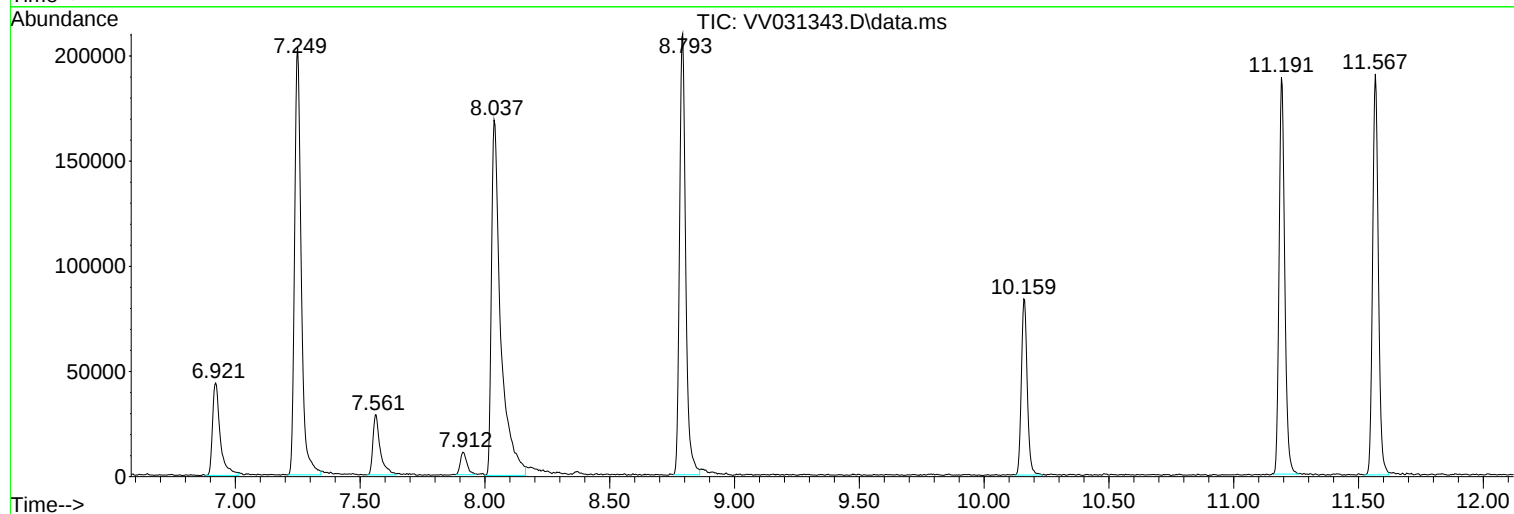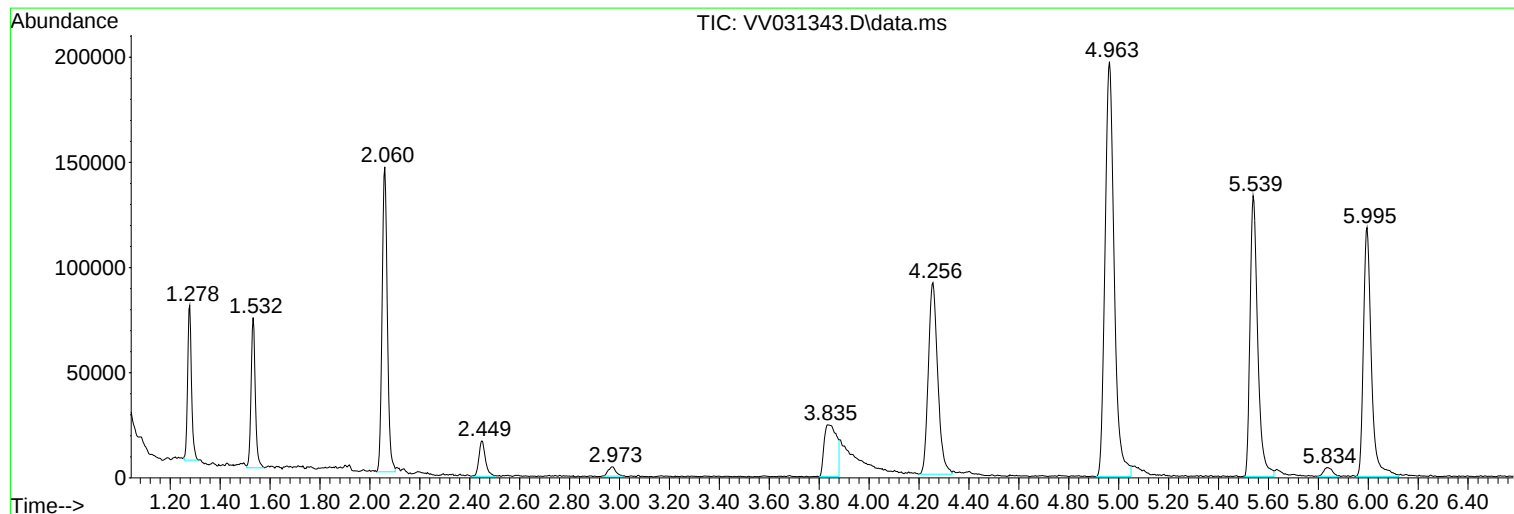

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031343.D
Acq On : 05 Jun 2023 13:39
Operator : SY/MD
Sample : VIBLK300
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK300

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031343.D
Acq On : 05 Jun 2023 13:39
Operator : SY/MD
Sample : VIBLK300
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK300

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------