

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031345.D
 Acq On : 05 Jun 2023 14:30
 Operator : SY/MD
 Sample : 03000-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C41

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	84	rVB	63793	67289	13.49%	1.771%
2	1.532	146	153	163	rVB	59063	69482	13.93%	1.829%
3	2.060	306	317	330	rBV	121329	178905	35.86%	4.709%
4	2.449	428	438	452	rBV5	3670	6870	1.38%	0.181%
5	3.825	854	866	908	rBV2	44904	204569	41.01%	5.385%
6	4.256	978	1000	1024	rBV	83736	220667	44.23%	5.809%
7	4.963	1204	1220	1249	rBV2	186821	487258	97.68%	12.827%
8	5.542	1387	1400	1427	rBV	114046	246749	49.46%	6.495%
9	5.831	1480	1490	1491	rBV5	8288	8312	1.67%	0.219%
10	5.995	1527	1541	1570	rBV	112456	250772	50.27%	6.601%
11	6.172	1588	1596	1611	rVB5	6815	13840	2.77%	0.364%
12	6.921	1819	1829	1846	rBV2	45774	91363	18.31%	2.405%
13	7.249	1920	1931	1956	rBV	183575	341228	68.40%	8.982%
14	7.564	2019	2029	2050	rBV2	28803	56532	11.33%	1.488%
15	7.915	2128	2138	2156	rVB2	23064	41396	8.30%	1.090%
16	8.037	2165	2176	2211	rBV	214334	498853	100.00%	13.132%
17	8.792	2399	2411	2430	rBV	183471	311534	62.45%	8.201%
18	10.159	2826	2836	2850	rBV	86004	138620	27.79%	3.649%
19	11.191	3145	3157	3180	rBV	166573	268409	53.81%	7.066%
20	11.567	3262	3274	3289	rBV	183974	296171	59.37%	7.796%




Sum of corrected areas: 3798819

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031345.D
Acq On : 05 Jun 2023 14:30
Operator : SY/MD
Sample : 03000-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

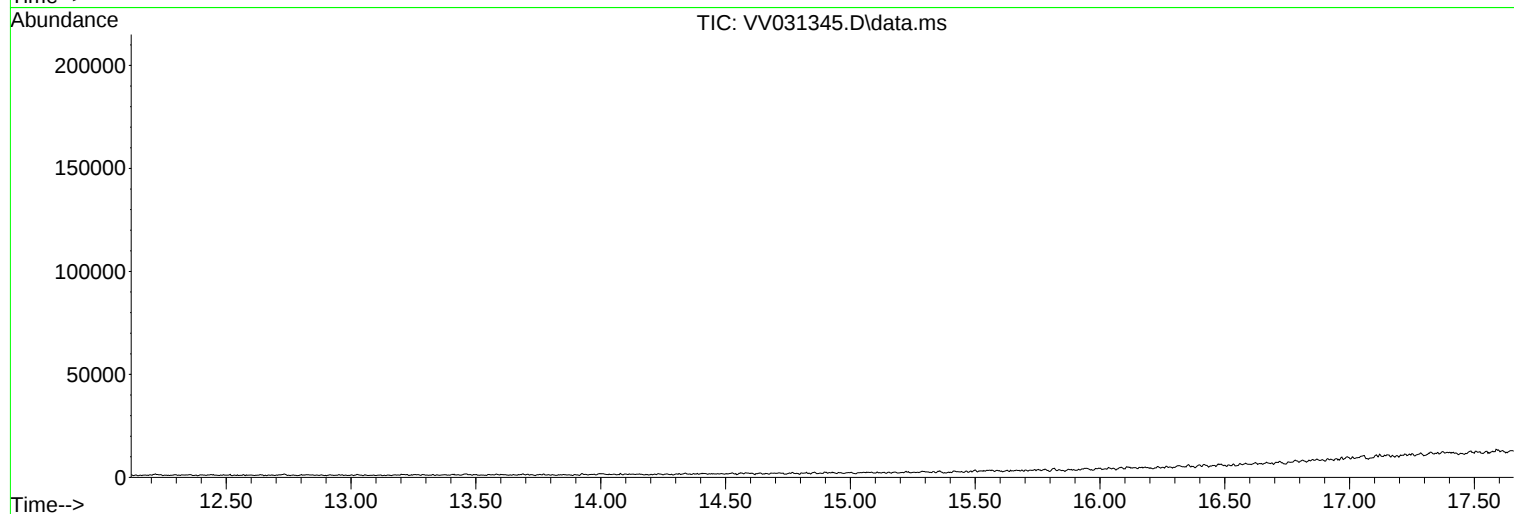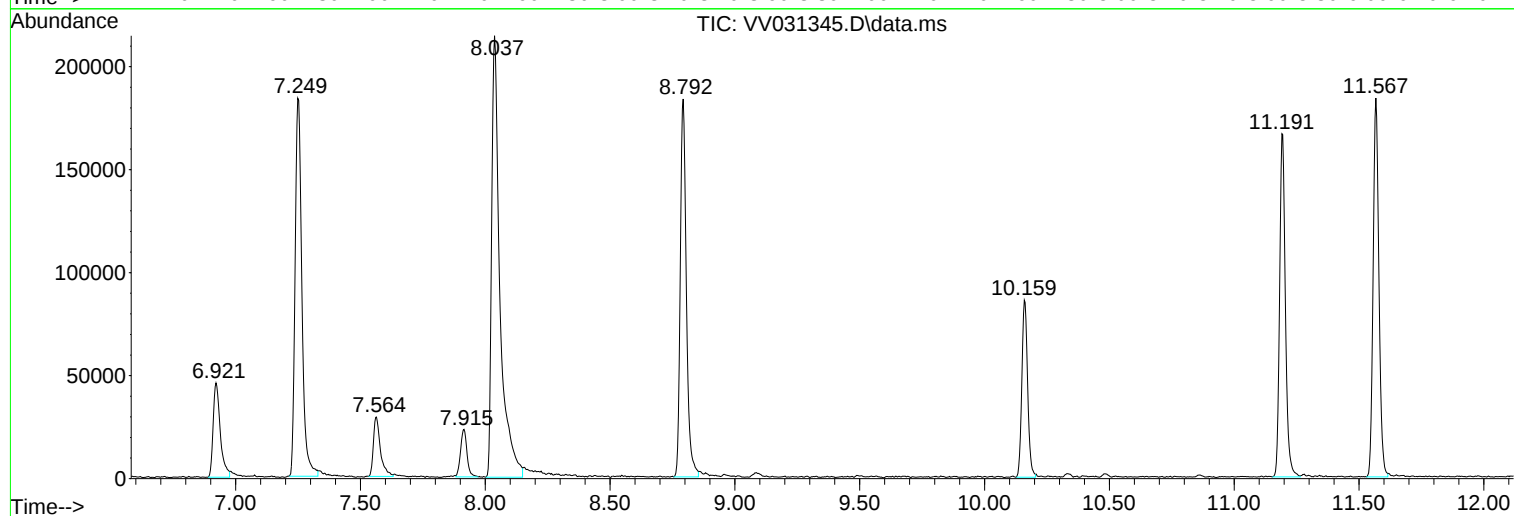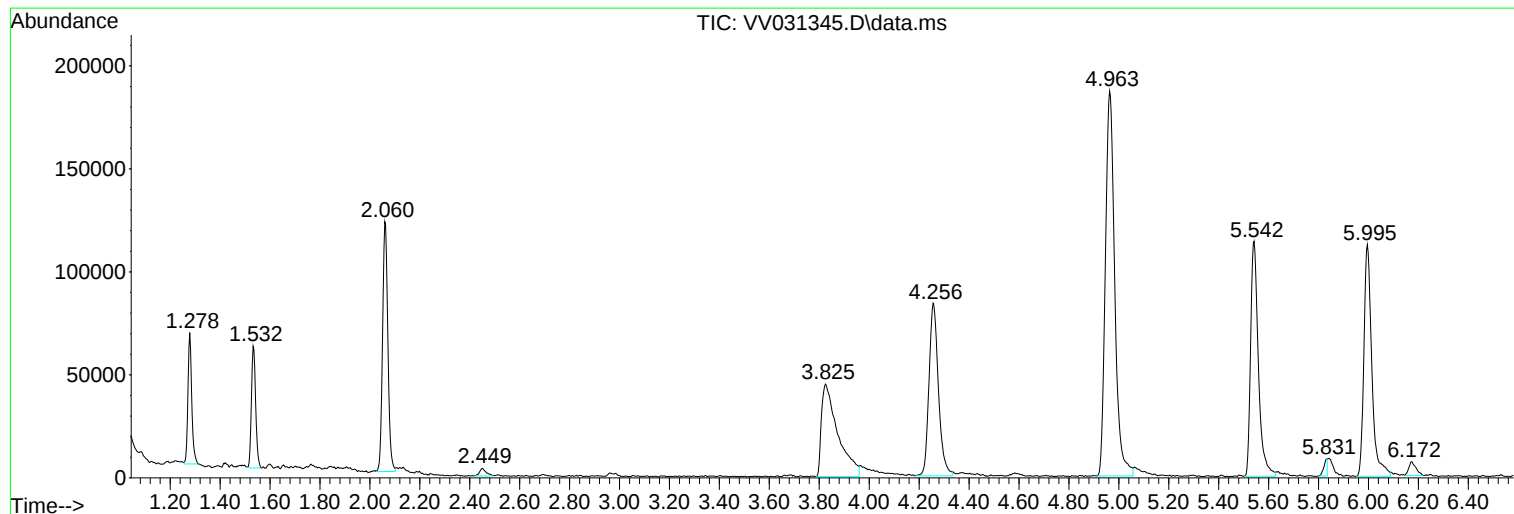

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031345.D
Acq On : 05 Jun 2023 14:30
Operator : SY/MD
Sample : 03000-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031345.D
Acq On : 05 Jun 2023 14:30
Operator : SY/MD
Sample : 03000-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc