

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031346.D
 Acq On : 05 Jun 2023 14:55
 Operator : SY/MD
 Sample : 03000-08 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C34

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031346.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	92	rVB	76935	89221	13.88%	1.700%
2	1.532	145	153	164	rVB	71782	84672	13.17%	1.614%
3	2.059	306	317	340	rVB	146422	220721	34.34%	4.207%
4	2.448	430	438	450	rVB2	4876	8367	1.30%	0.159%
5	3.838	852	870	891	rBV4	34397	145020	22.56%	2.764%
6	4.256	983	1000	1023	rBV2	93397	245065	38.12%	4.671%
7	4.963	1205	1220	1245	rBV3	204976	529968	82.44%	10.100%
8	5.542	1387	1400	1425	rBV	160457	343989	53.51%	6.556%
9	5.837	1477	1492	1510	rBV	207616	423632	65.90%	8.074%
10	5.995	1529	1541	1574	rVB2	123879	266800	41.50%	5.085%
11	6.921	1816	1829	1844	rBV	47406	93594	14.56%	1.784%
12	7.249	1916	1931	1954	rBV	216045	397930	61.90%	7.584%
13	7.564	2019	2029	2055	rBV3	29465	60240	9.37%	1.148%
14	7.911	2120	2137	2162	rBV	368538	642818	100.00%	12.251%
15	8.040	2167	2177	2210	rBV	180629	441154	68.63%	8.408%
16	8.792	2399	2411	2436	rBV	242771	422926	65.79%	8.060%
17	10.162	2825	2837	2858	rBV	82070	142798	22.21%	2.722%
18	11.191	3147	3157	3177	rBV	217315	358626	55.79%	6.835%
19	11.567	3262	3274	3297	rBV	202289	329473	51.25%	6.279%




Sum of corrected areas: 5247014

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031346.D
Acq On : 05 Jun 2023 14:55
Operator : SY/MD
Sample : 03000-08 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

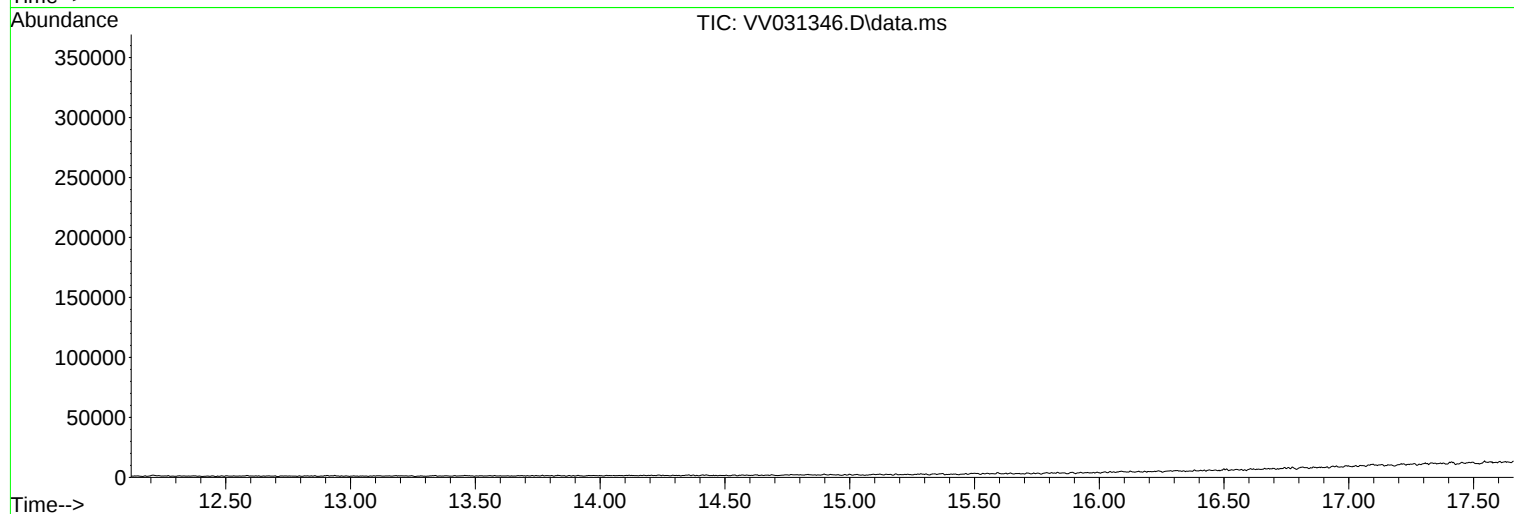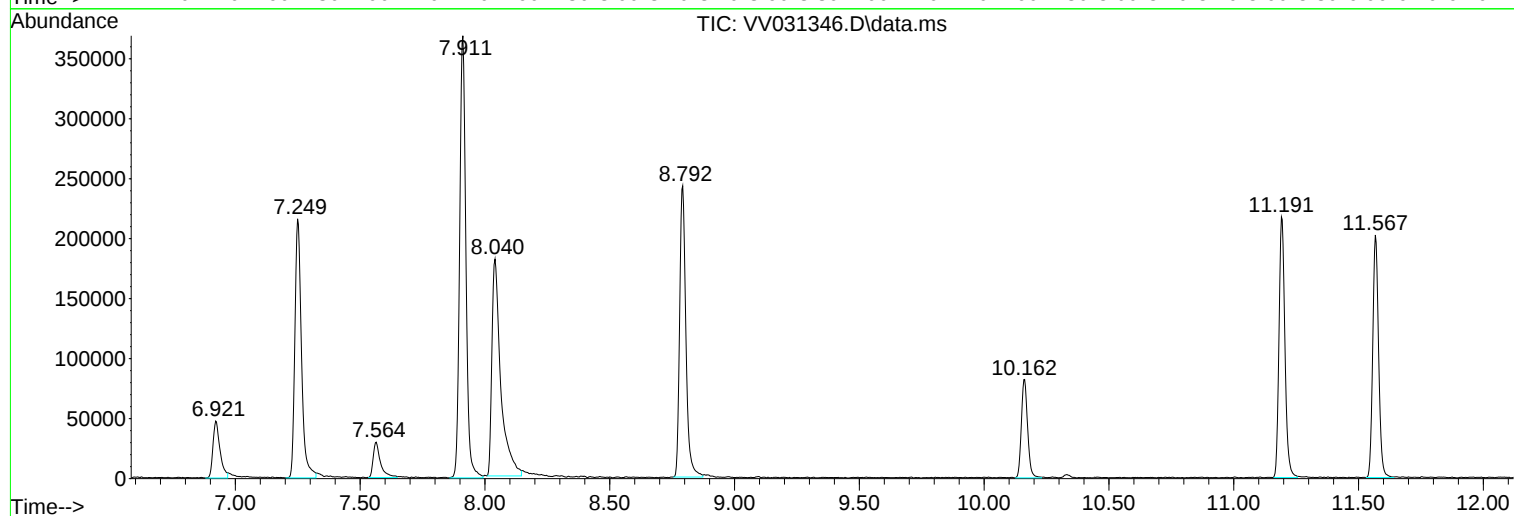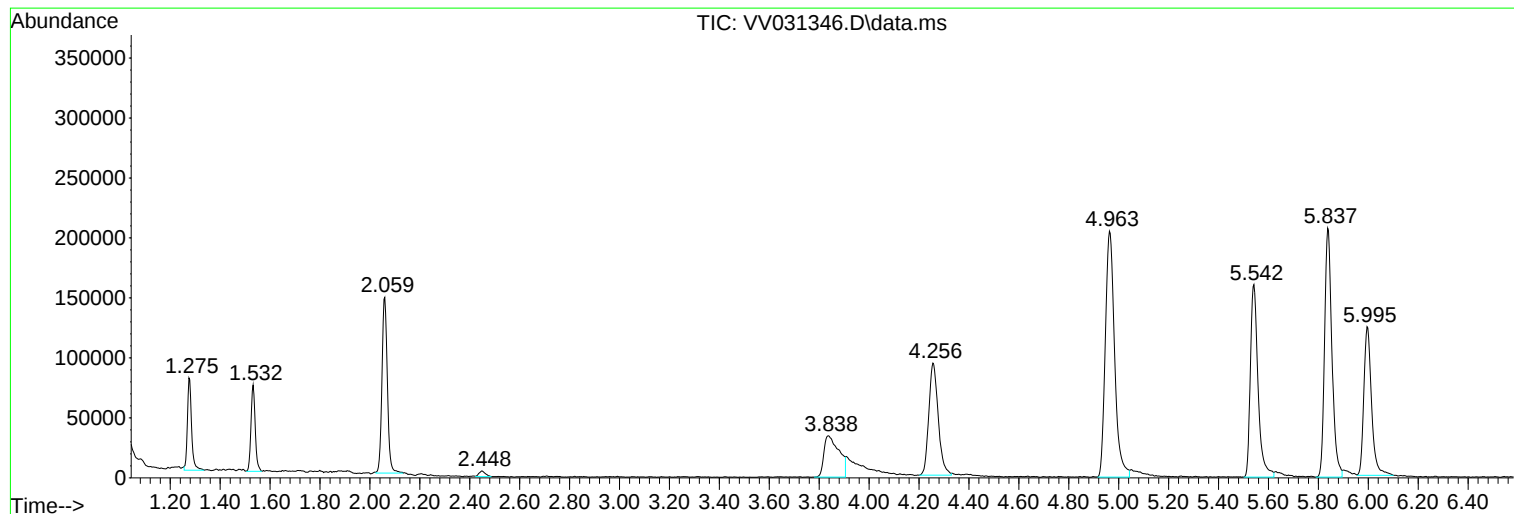

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031346.D
Acq On : 05 Jun 2023 14:55
Operator : SY/MD
Sample : 03000-08 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031346.D
Acq On : 05 Jun 2023 14:55
Operator : SY/MD
Sample : 03000-08 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc