

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031347.D
 Acq On : 05 Jun 2023 15:18
 Operator : SY/MD
 Sample : 03000-09 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C40

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rVB	76619	82253	15.53%	1.968%
2	1.532	146	153	164	rBV	70380	80205	15.15%	1.919%
3	2.060	307	317	330	rBV	148353	215432	40.68%	5.155%
4	2.452	429	439	453	rVB4	5556	10714	2.02%	0.256%
5	3.851	859	874	908	rBV2	29918	169452	32.00%	4.055%
6	4.259	985	1001	1024	rBV	90645	239395	45.21%	5.729%
7	4.963	1201	1220	1247	rBV2	208130	529530	100.00%	12.672%
8	5.542	1388	1400	1419	rBV	153502	324764	61.33%	7.772%
9	5.835	1482	1491	1504	rVB	3954	9665	1.83%	0.231%
10	5.995	1528	1541	1561	rBV	124108	266251	50.28%	6.372%
11	6.921	1815	1829	1844	rBV	48372	94592	17.86%	2.264%
12	7.249	1919	1931	1948	rBV	212767	386765	73.04%	9.256%
13	7.564	2016	2029	2051	rBV2	29993	60134	11.36%	1.439%
14	7.908	2125	2136	2149	rVB8	5707	11165	2.11%	0.267%
15	8.040	2166	2177	2221	rBV	184946	456563	86.22%	10.926%
16	8.793	2397	2411	2437	rBV	243390	417040	78.76%	9.980%
17	10.162	2824	2837	2853	rBV	86171	141591	26.74%	3.388%
18	11.191	3147	3157	3180	rBV	218824	357100	67.44%	8.546%
19	11.567	3261	3274	3289	rBV	203787	326080	61.58%	7.803%




Sum of corrected areas: 4178691

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031347.D
Acq On : 05 Jun 2023 15:18
Operator : SY/MD
Sample : 03000-09 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

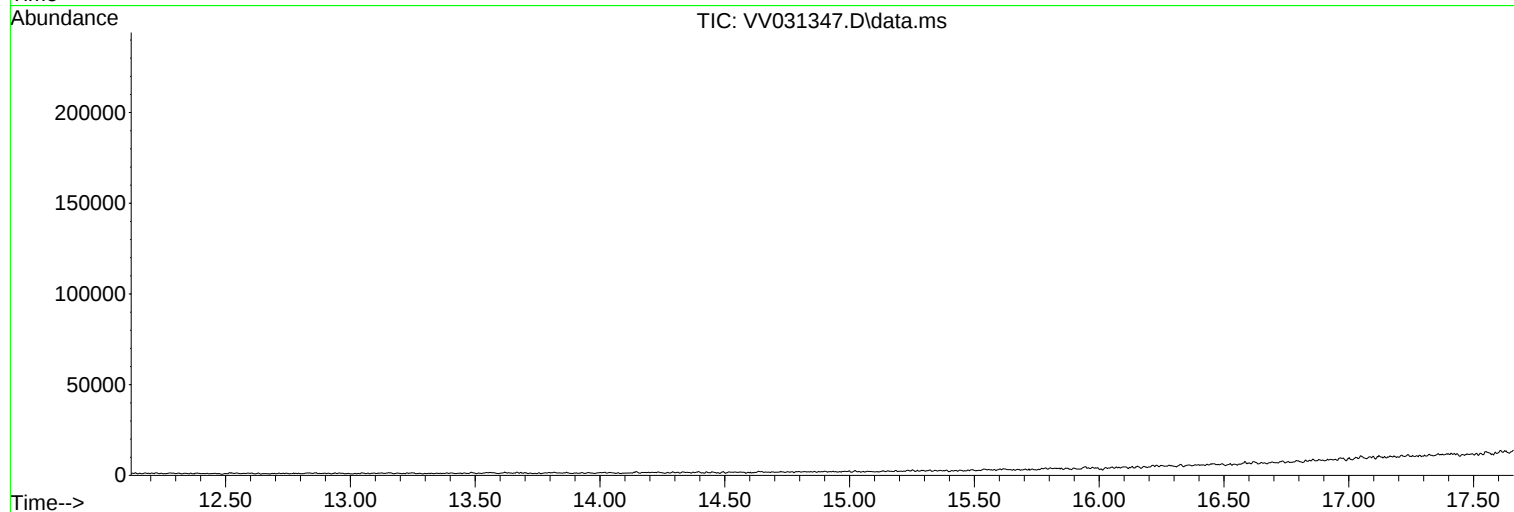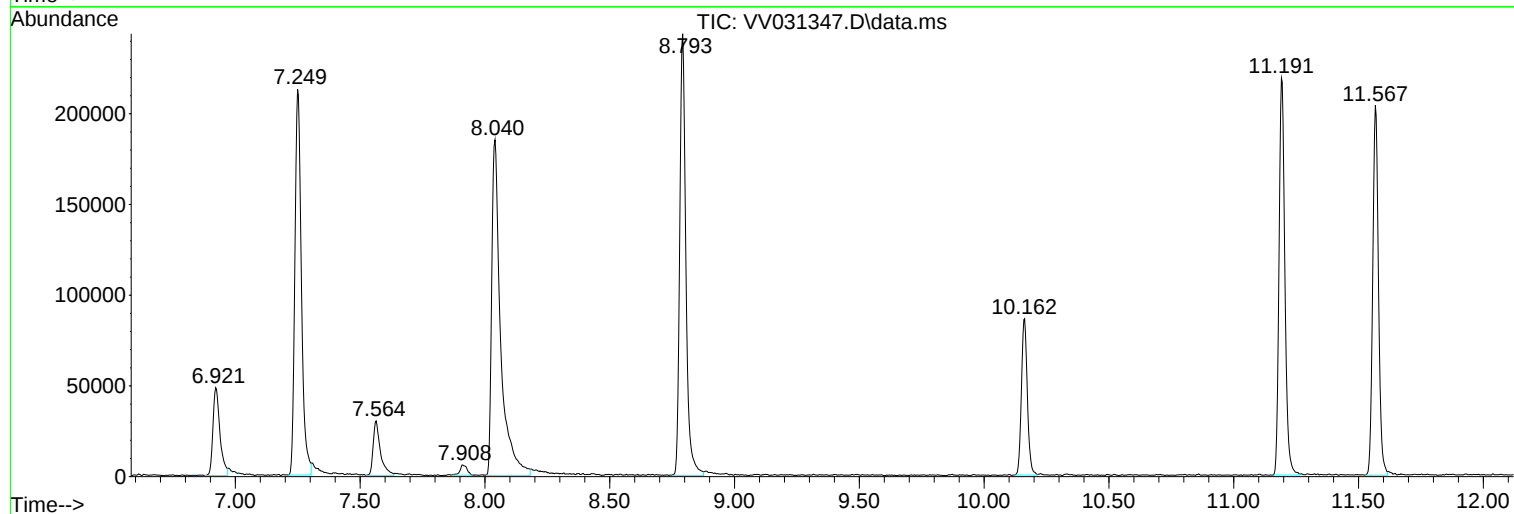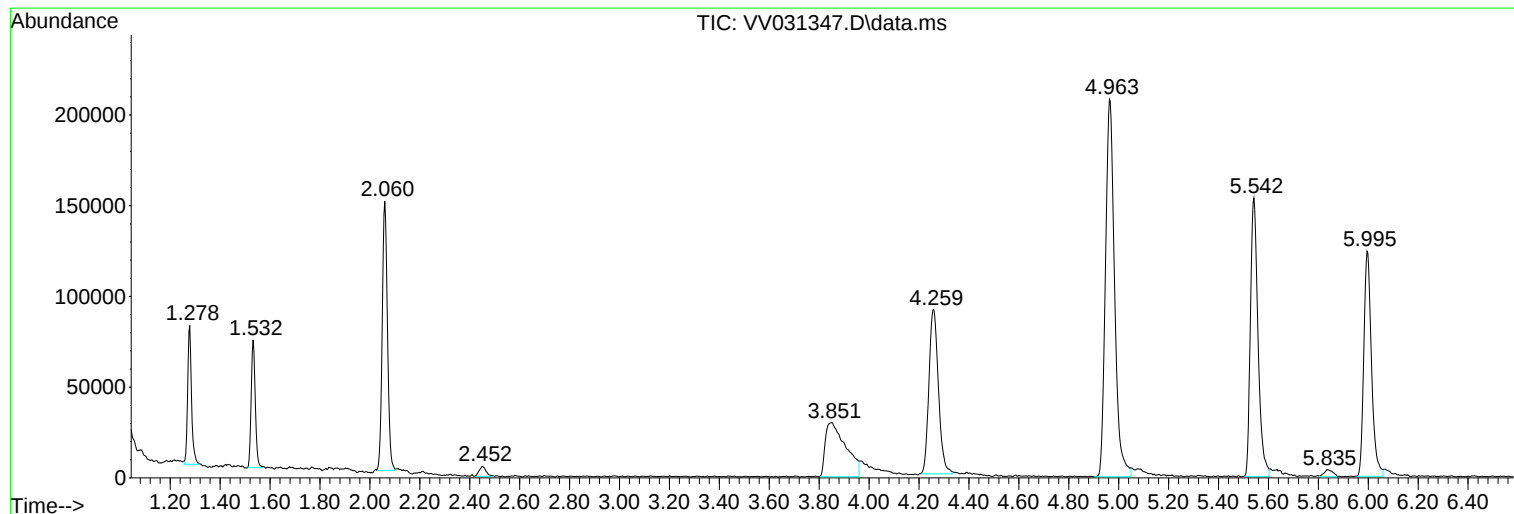

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031347.D
Acq On : 05 Jun 2023 15:18
Operator : SY/MD
Sample : 03000-09 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031347.D
Acq On : 05 Jun 2023 15:18
Operator : SY/MD
Sample : 03000-09 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------