

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031348.D
 Acq On : 05 Jun 2023 15:41
 Operator : SY/MD
 Sample : 02990-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C00

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031348.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	94	rVB	72384	83668	16.43%	2.116%
2	1.417	113	117	125	rVB7	5408	5998	1.18%	0.152%
3	1.532	145	153	168	rVB	70102	80191	15.75%	2.028%
4	2.060	306	317	329	rBV	140365	203192	39.90%	5.138%
5	2.452	431	439	447	rBV3	3839	5901	1.16%	0.149%
6	3.847	860	873	895	rBV2	28697	127733	25.08%	3.230%
7	4.259	984	1001	1027	rBV	88410	235373	46.22%	5.952%
8	4.966	1204	1221	1247	rBV3	196970	509249	100.00%	12.877%
9	5.542	1388	1400	1420	rBV	140108	294606	57.85%	7.450%
10	5.838	1481	1492	1506	rVB	6134	12523	2.46%	0.317%
11	5.995	1528	1541	1565	rBV	119542	259491	50.96%	6.562%
12	6.172	1586	1596	1615	rVB7	6984	15204	2.99%	0.384%
13	6.921	1819	1829	1844	rBV2	45366	89227	17.52%	2.256%
14	7.249	1920	1931	1953	rBV	203780	374586	73.56%	9.472%
15	7.561	2019	2028	2049	rBV	30234	59020	11.59%	1.492%
16	7.918	2131	2139	2148	rVB7	4468	7876	1.55%	0.199%
17	8.040	2167	2177	2221	rBV2	177235	439862	86.37%	11.123%
18	8.793	2397	2411	2430	rBV	217938	375935	73.82%	9.506%
19	10.162	2821	2837	2852	rBV	77807	127819	25.10%	3.232%
20	11.191	3146	3157	3177	rBV	199758	327167	64.24%	8.273%
21	11.567	3262	3274	3298	rBV	195939	320036	62.84%	8.093%




Sum of corrected areas: 3954657

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031348.D
Acq On : 05 Jun 2023 15:41
Operator : SY/MD
Sample : 02990-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

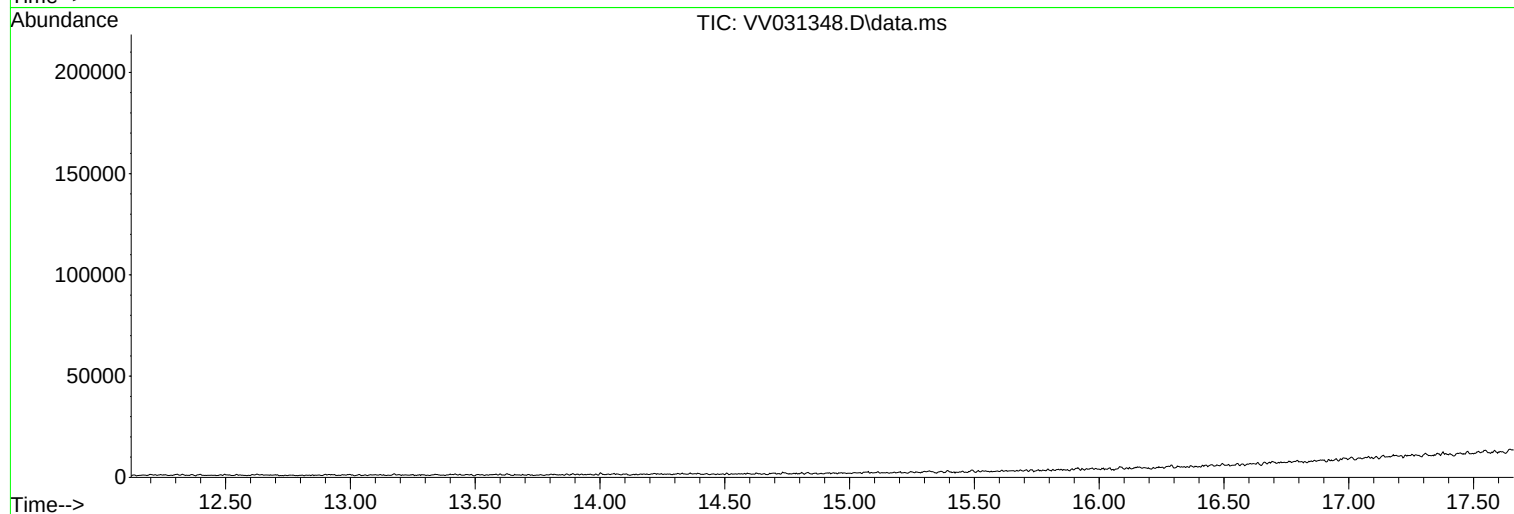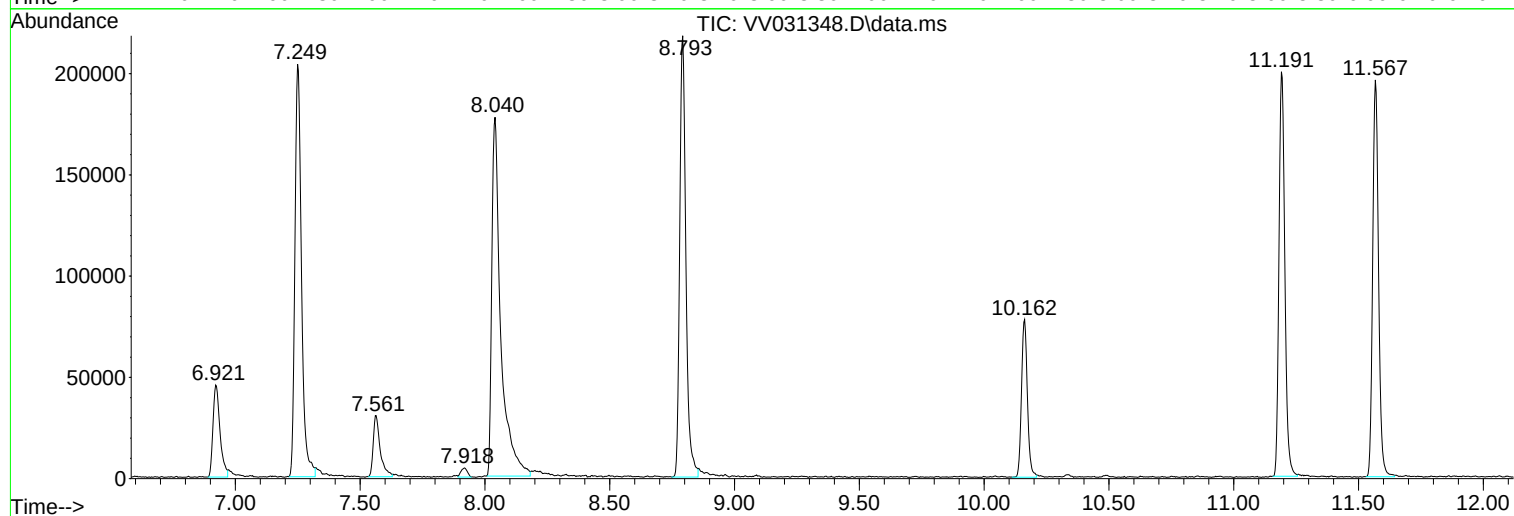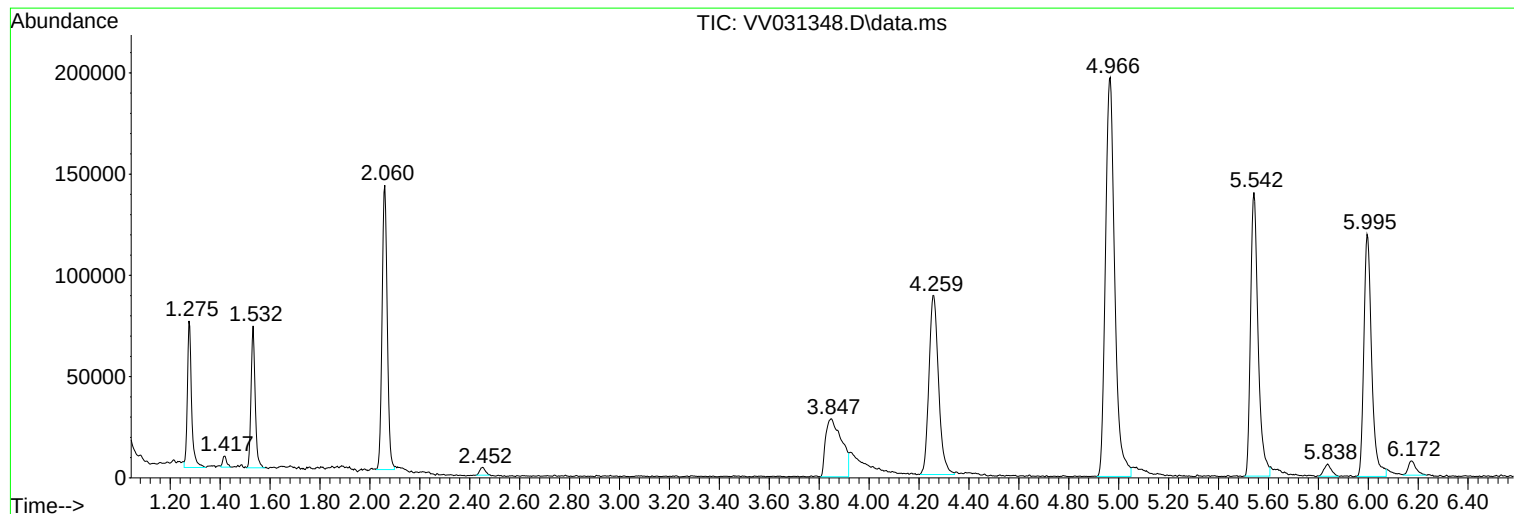

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031348.D
Acq On : 05 Jun 2023 15:41
Operator : SY/MD
Sample : 02990-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031348.D
Acq On : 05 Jun 2023 15:41
Operator : SY/MD
Sample : 02990-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc