

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031350.D
 Acq On : 05 Jun 2023 16:25
 Operator : SY/MD
 Sample : 02990-02 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C27

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	85	rVB	78783	87887	14.96%	1.784%
2	1.532	146	153	166	rVB	74837	85594	14.57%	1.737%
3	2.060	307	317	332	rBV	157296	232560	39.60%	4.721%
4	2.449	428	438	449	rBV2	11062	17858	3.04%	0.362%
5	2.712	507	520	540	rVB4	9276	22121	3.77%	0.449%
6	3.835	854	869	909	rBV4	44241	218229	37.16%	4.430%
7	4.256	983	1000	1022	rBV	99815	265534	45.21%	5.390%
8	4.963	1202	1220	1251	rBV2	225664	587296	100.00%	11.921%
9	5.542	1385	1400	1423	rBV	150979	320812	54.63%	6.512%
10	5.844	1482	1494	1506	rBV6	18544	42040	7.16%	0.853%
11	5.998	1529	1542	1560	rBV2	131405	285310	48.58%	5.791%
12	6.921	1819	1829	1848	rBV2	50570	101443	17.27%	2.059%
13	7.249	1920	1931	1960	rBV	233967	434470	73.98%	8.819%
14	7.564	2018	2029	2048	rBV	33661	66016	11.24%	1.340%
15	7.912	2123	2137	2155	rBV	246316	425218	72.40%	8.631%
16	8.040	2166	2177	2210	rBV	201185	482829	82.21%	9.801%
17	8.793	2400	2411	2432	rBV	234863	401164	68.31%	8.143%
18	10.159	2825	2836	2856	rBV	93985	153452	26.13%	3.115%
19	11.191	3146	3157	3179	rBV	208973	342027	58.24%	6.943%
20	11.567	3263	3274	3292	rBV	217962	354587	60.38%	7.198%




Sum of corrected areas: 4926447

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031350.D
Acq On : 05 Jun 2023 16:25
Operator : SY/MD
Sample : 02990-02 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

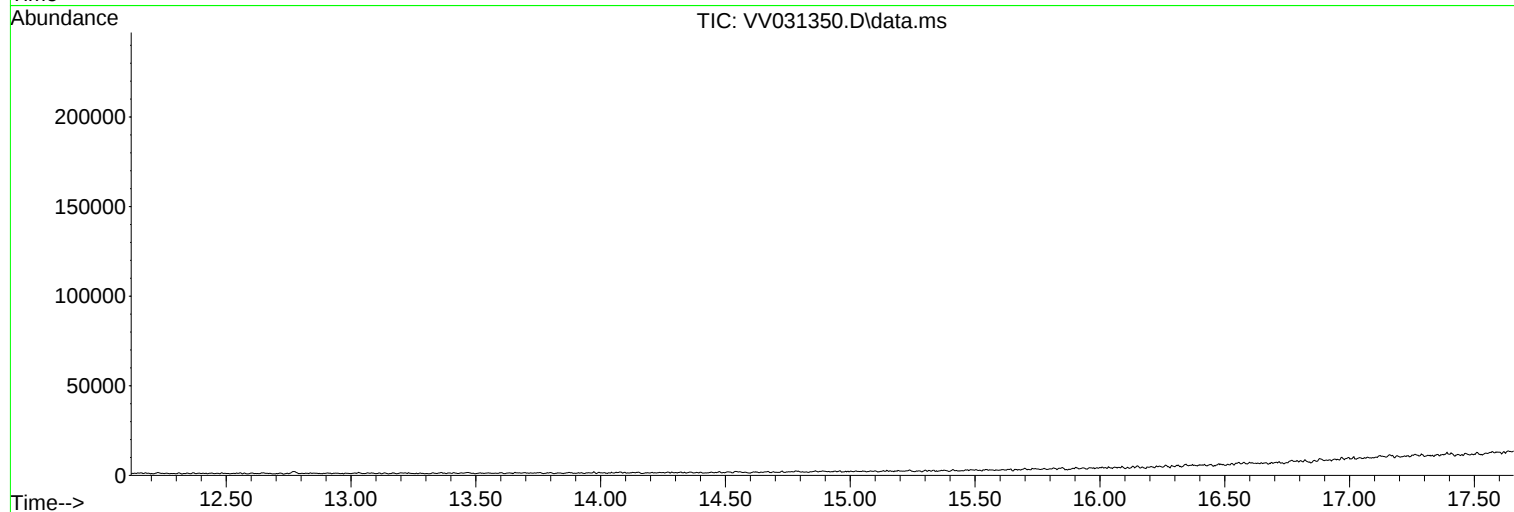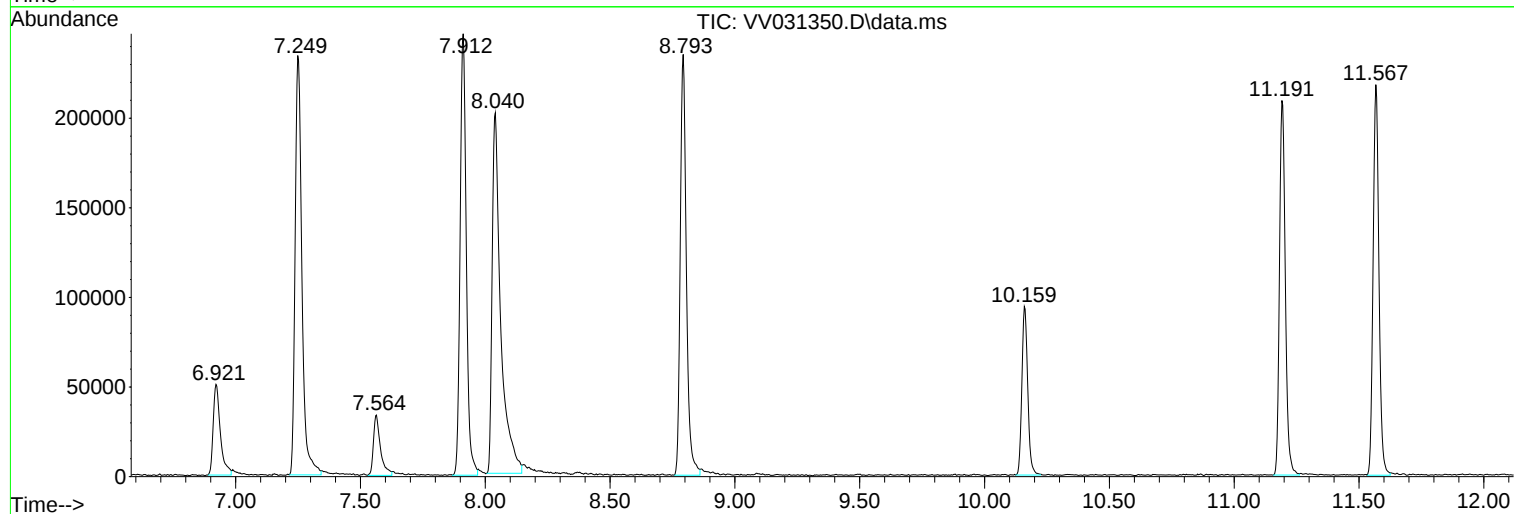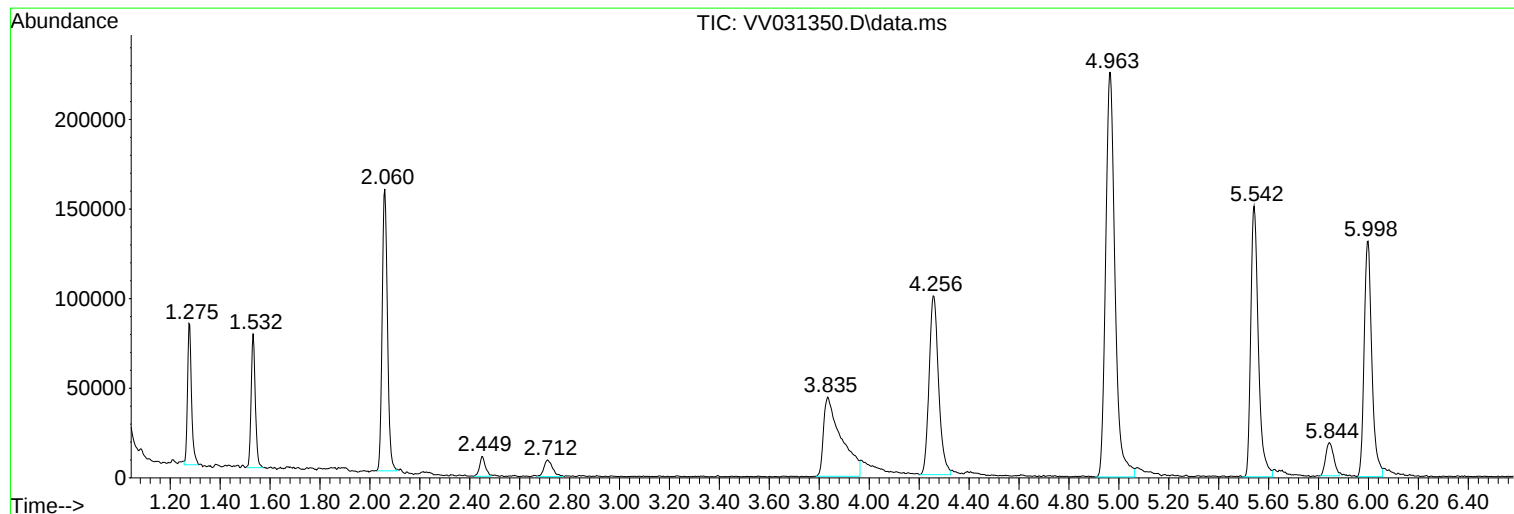

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031350.D
Acq On : 05 Jun 2023 16:25
Operator : SY/MD
Sample : 02990-02 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031350.D
Acq On : 05 Jun 2023 16:25
Operator : SY/MD
Sample : 02990-02 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc