

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031351.D
 Acq On : 05 Jun 2023 16:50
 Operator : SY/MD
 Sample : 02990-05 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C30

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031351.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	96	rVB	75878	90358	17.07%	1.994%
2	1.532	145	153	166	rVB	65818	78853	14.90%	1.740%
3	1.597	166	173	181	rBV4	6838	8786	1.66%	0.194%
4	2.060	306	317	332	rBV	140249	209133	39.51%	4.616%
5	2.449	425	438	454	rBV4	10317	21345	4.03%	0.471%
6	2.700	506	516	529	rBV6	8972	18126	3.42%	0.400%
7	3.825	851	866	886	rBV3	108064	316611	59.81%	6.988%
8	4.256	984	1000	1026	rBV	88513	234396	44.28%	5.173%
9	4.963	1204	1220	1249	rBV2	202772	529357	100.00%	11.683%
10	5.542	1386	1400	1421	rBV	152469	321360	60.71%	7.093%
11	5.841	1480	1493	1513	rBV2	65541	139828	26.41%	3.086%
12	5.995	1529	1541	1575	rBV	118013	264494	49.97%	5.838%
13	6.921	1819	1829	1847	rBV	44484	93438	17.65%	2.062%
14	7.249	1919	1931	1962	rBV	207658	385401	72.81%	8.506%
15	7.561	2019	2028	2044	rBV3	28489	54406	10.28%	1.201%
16	7.912	2126	2137	2156	rVB2	58677	105601	19.95%	2.331%
17	8.040	2165	2177	2216	rBV	173753	436252	82.41%	9.628%
18	8.793	2400	2411	2435	rBV	234272	407751	77.03%	8.999%
19	10.159	2826	2836	2853	rBV	81834	137401	25.96%	3.033%
20	11.191	3146	3157	3182	rBV	216672	354132	66.90%	7.816%
21	11.567	3260	3274	3294	rBV	199963	323873	61.18%	7.148%




Sum of corrected areas: 4530902

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031351.D
Acq On : 05 Jun 2023 16:50
Operator : SY/MD
Sample : 02990-05 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

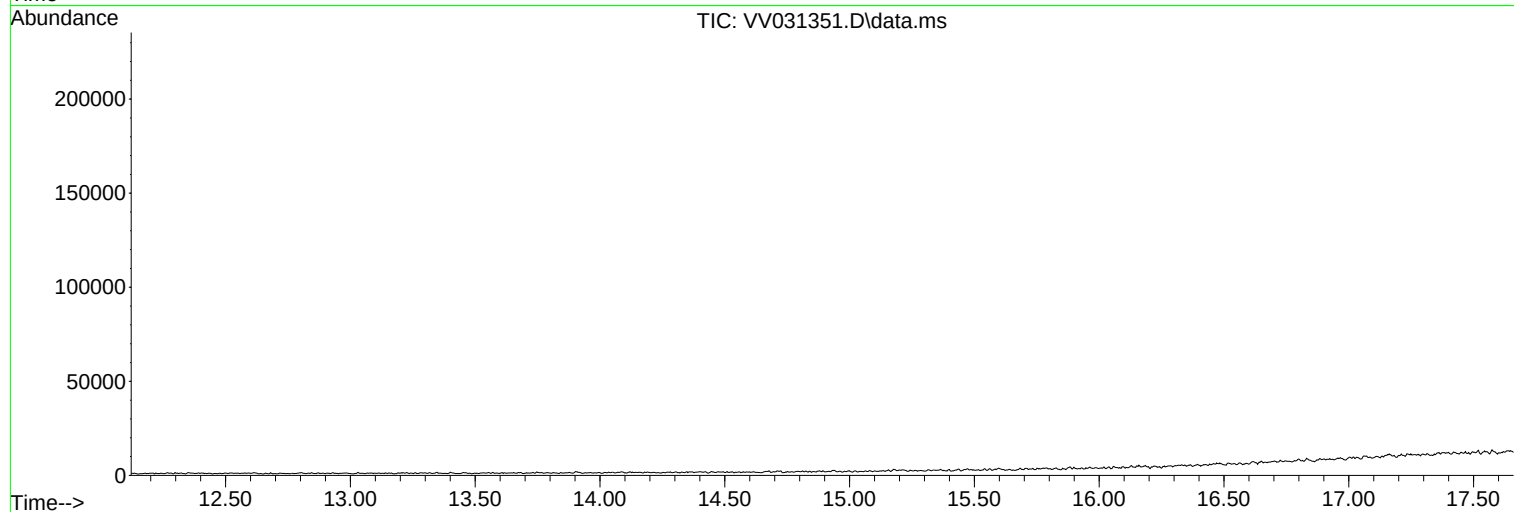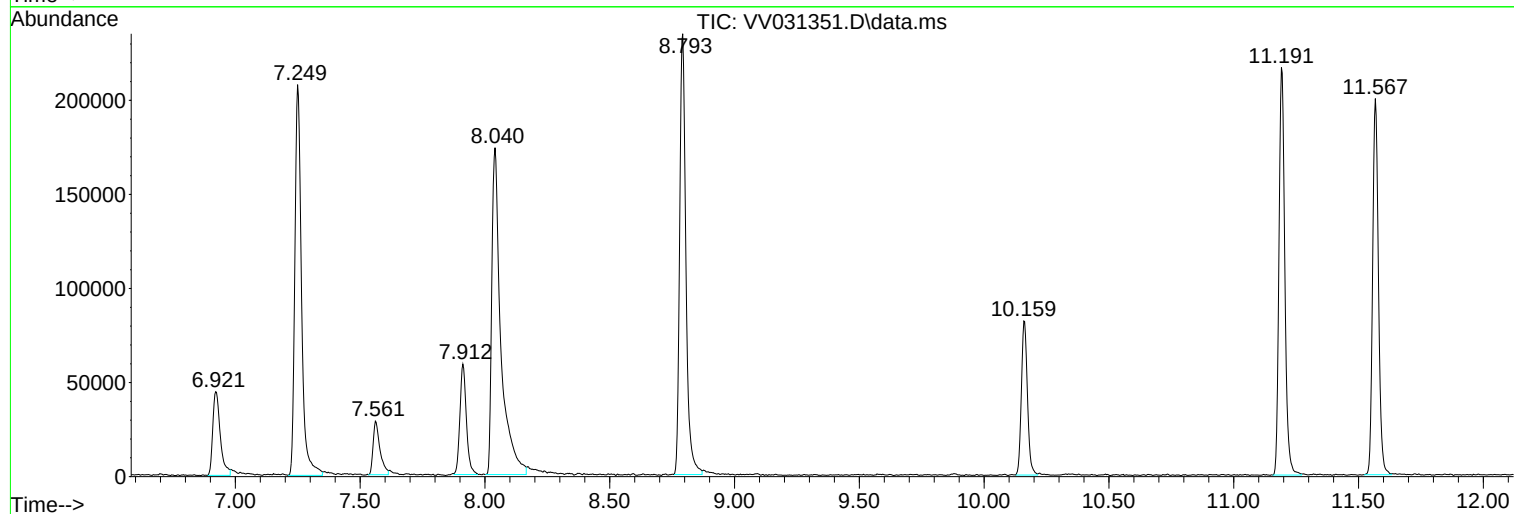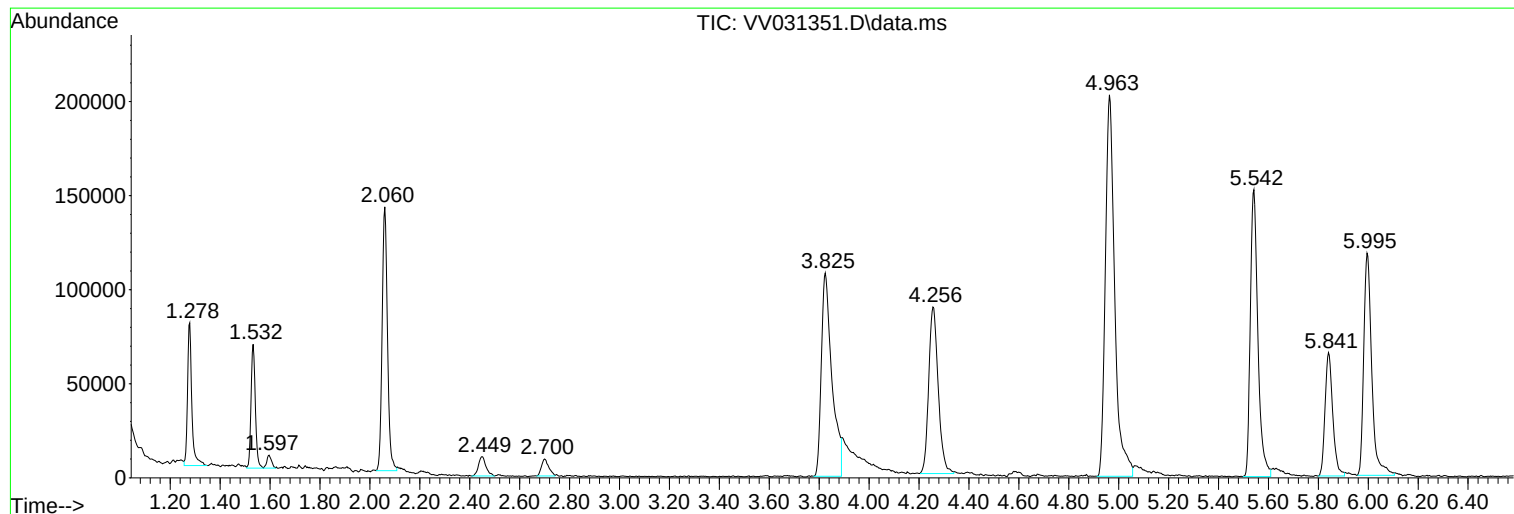

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031351.D
Acq On : 05 Jun 2023 16:50
Operator : SY/MD
Sample : 02990-05 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031351.D
Acq On : 05 Jun 2023 16:50
Operator : SY/MD
Sample : 02990-05 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc