

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031352.D
 Acq On : 05 Jun 2023 17:14
 Operator : SY/MD
 Sample : 02990-07 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C32

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	68935	77986	13.20%	1.628%
2	1.532	146	153	166	rVB	65818	74646	12.63%	1.558%
3	2.060	306	317	335	rBV	141152	207056	35.03%	4.323%
4	2.452	430	439	453	rVB3	9159	15539	2.63%	0.324%
5	3.834	857	869	917	rBV4	31832	183220	31.00%	3.825%
6	4.256	983	1000	1020	rBV2	90750	234645	39.70%	4.899%
7	4.963	1201	1220	1251	rBV2	198015	515517	87.22%	10.762%
8	5.539	1385	1399	1421	rBV	154916	333341	56.40%	6.959%
9	5.841	1480	1493	1512	rBV4	49701	106608	18.04%	2.226%
10	5.995	1528	1541	1565	rBV2	117882	257128	43.51%	5.368%
11	6.921	1819	1829	1854	rBV2	45310	93342	15.79%	1.949%
12	7.249	1920	1931	1955	rBV	202899	375598	63.55%	7.841%
13	7.564	2019	2029	2049	rBV2	27243	56203	9.51%	1.173%
14	7.911	2125	2137	2159	rBV	346413	591026	100.00%	12.339%
15	8.040	2167	2177	2215	rBV2	172589	427174	72.28%	8.918%
16	8.792	2400	2411	2437	rBV	242339	420865	71.21%	8.786%
17	10.162	2822	2837	2853	rBV	81828	134886	22.82%	2.816%
18	11.191	3145	3157	3181	rBV	224288	365317	61.81%	7.627%
19	11.567	3259	3274	3293	rBV	194372	319888	54.12%	6.678%




Sum of corrected areas: 4789985

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031352.D
Acq On : 05 Jun 2023 17:14
Operator : SY/MD
Sample : 02990-07 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

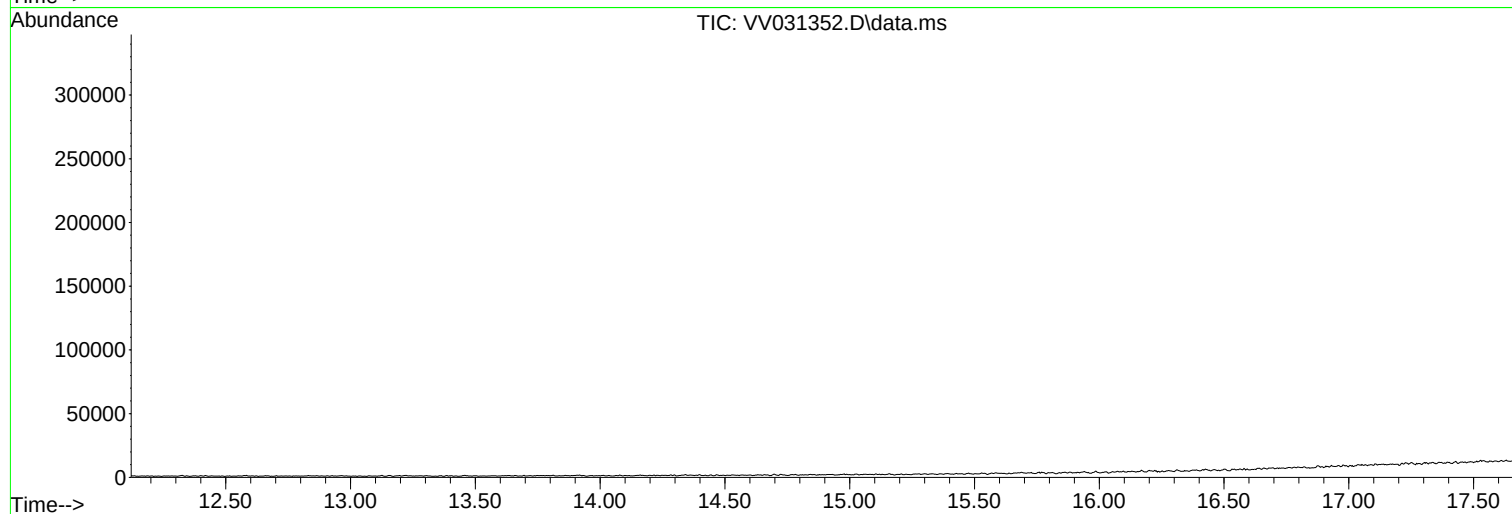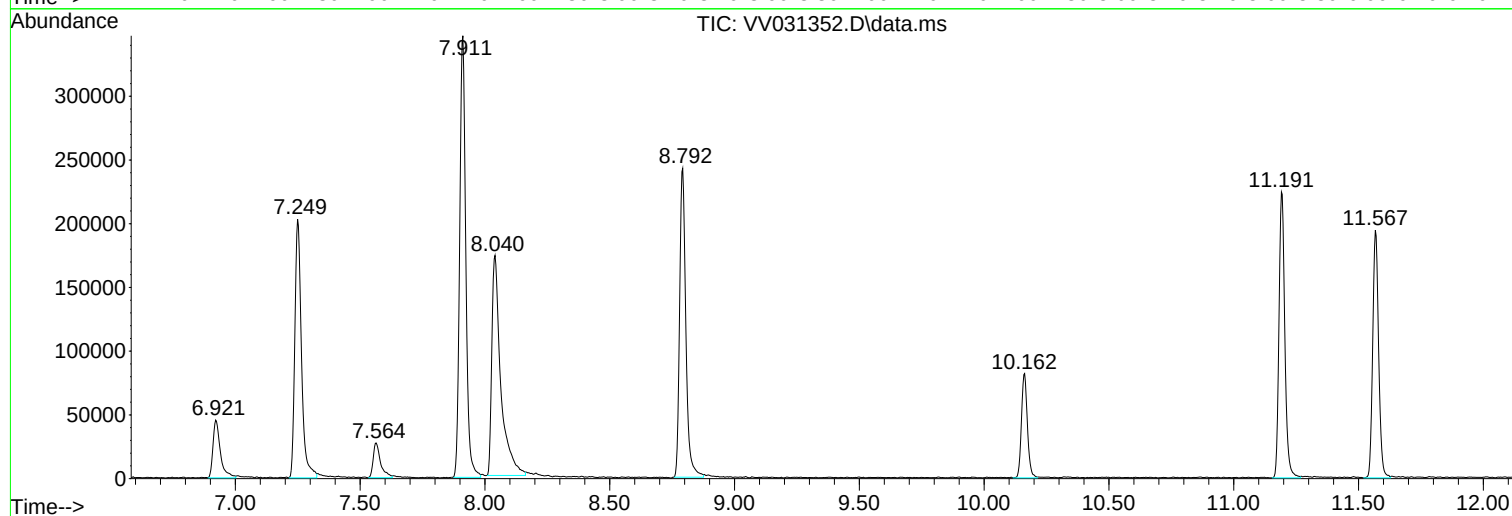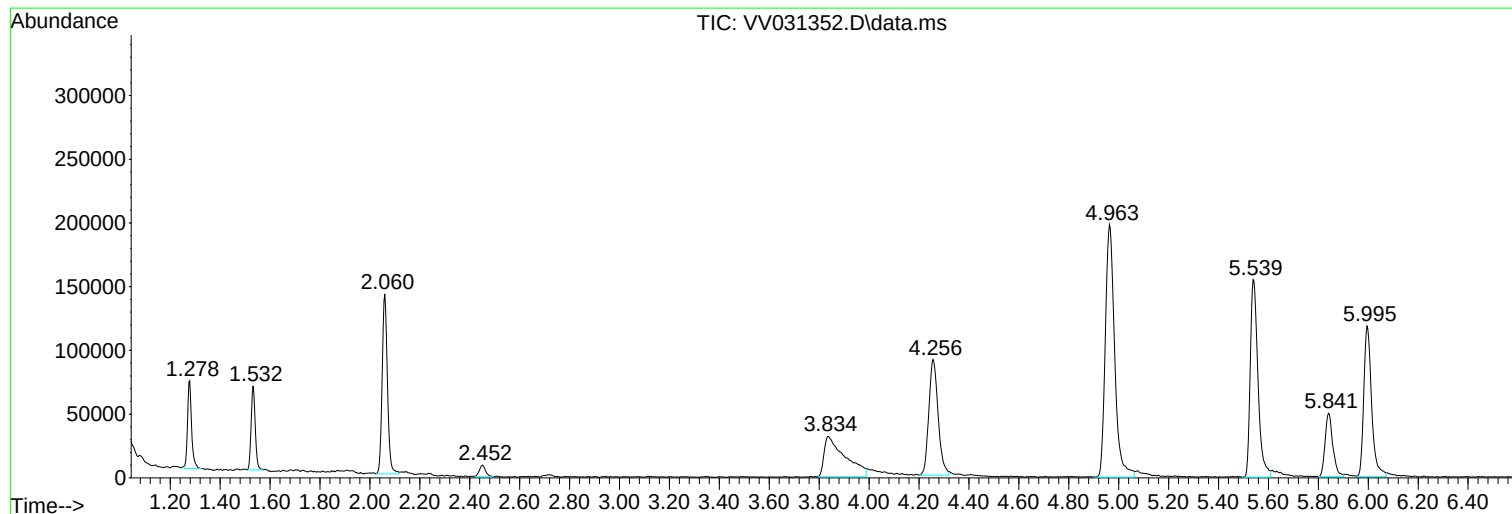

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031352.D
Acq On : 05 Jun 2023 17:14
Operator : SY/MD
Sample : 02990-07 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031352.D
Acq On : 05 Jun 2023 17:14
Operator : SY/MD
Sample : 02990-07 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc