

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031353.D
 Acq On : 05 Jun 2023 17:39
 Operator : SY/MD
 Sample : 02990-14DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C44DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031353.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	93	rVB	71792	83132	16.29%	1.897%
2	1.532	145	153	169	rVB	70204	84895	16.64%	1.937%
3	2.060	306	317	327	rBV	139436	203104	39.80%	4.635%
4	2.449	424	438	452	rBV	29288	51578	10.11%	1.177%
5	3.838	853	870	913	rBV3	40178	216952	42.51%	4.951%
6	4.256	985	1000	1024	rBV	90509	235075	46.06%	5.364%
7	4.963	1205	1220	1245	rBV2	199112	510335	100.00%	11.646%
8	5.542	1386	1400	1420	rBV	141385	300839	58.95%	6.865%
9	5.844	1482	1494	1508	rBV6	21532	47472	9.30%	1.083%
10	5.995	1528	1541	1566	rBV	118627	258084	50.57%	5.889%
11	6.921	1817	1829	1848	rBV2	44715	90683	17.77%	2.069%
12	7.249	1919	1931	1959	rBV	199919	373975	73.28%	8.534%
13	7.564	2018	2029	2044	rBV	28450	55459	10.87%	1.266%
14	7.912	2125	2137	2161	rBV	160940	277474	54.37%	6.332%
15	8.040	2166	2177	2215	rBV	175771	442364	86.68%	10.095%
16	8.793	2398	2411	2435	rBV	221267	384040	75.25%	8.764%
17	10.162	2826	2837	2858	rBV	83048	137830	27.01%	3.145%
18	11.191	3144	3157	3176	rBV	197891	320410	62.78%	7.312%
19	11.567	3262	3274	3289	rBV	191718	308510	60.45%	7.040%




Sum of corrected areas: 4382211

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031353.D
Acq On : 05 Jun 2023 17:39
Operator : SY/MD
Sample : 02990-14DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

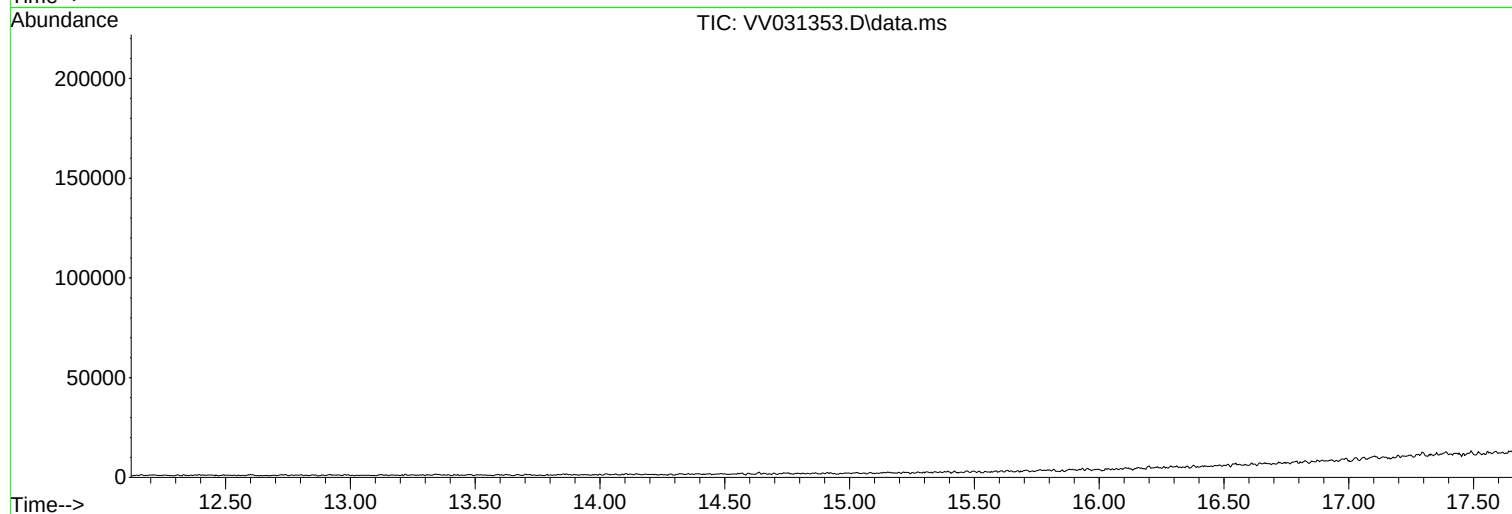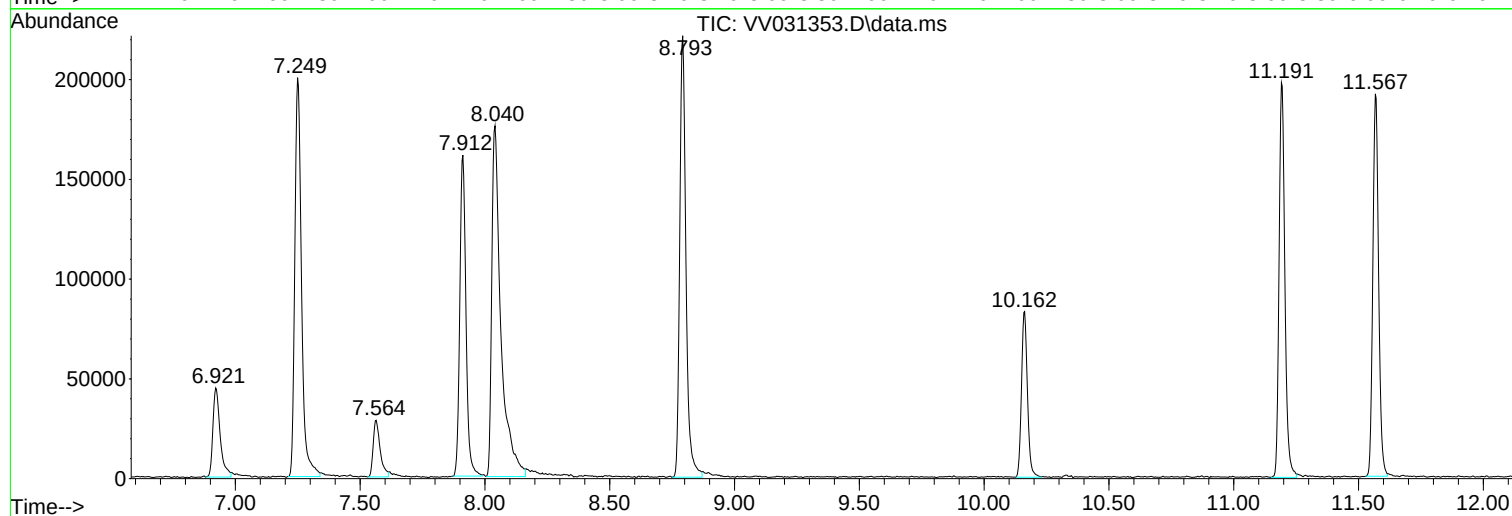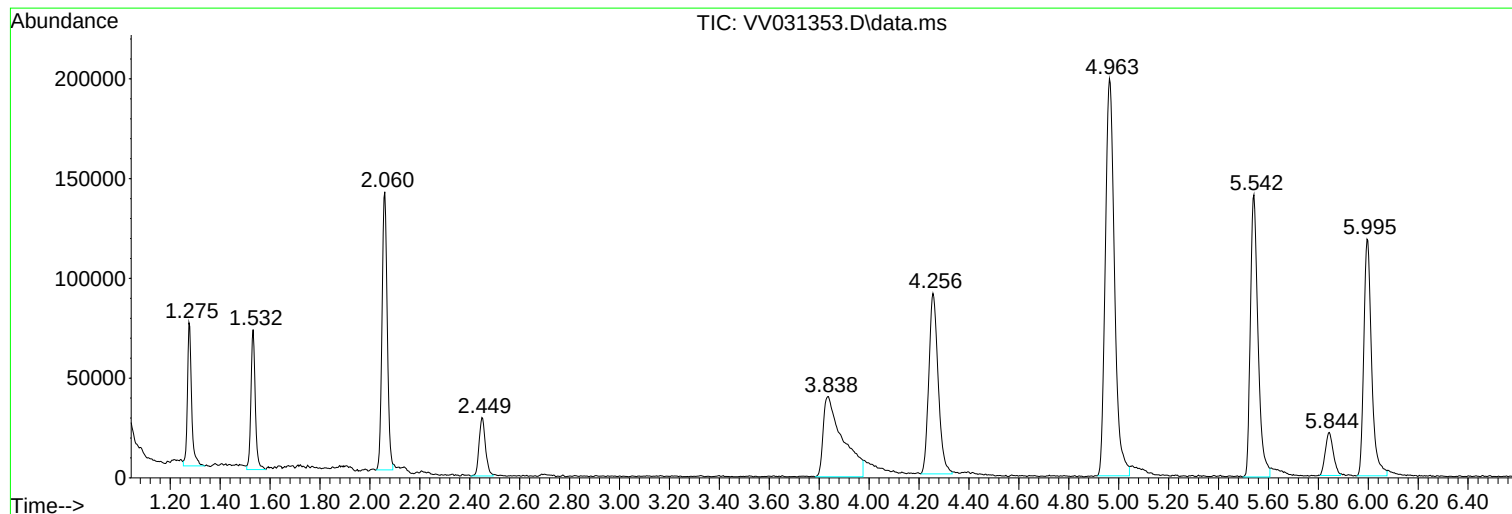

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031353.D
Acq On : 05 Jun 2023 17:39
Operator : SY/MD
Sample : 02990-14DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031353.D
Acq On : 05 Jun 2023 17:39
Operator : SY/MD
Sample : 02990-14DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C44DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------