

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031354.D
 Acq On : 05 Jun 2023 18:03
 Operator : SY/MD
 Sample : 02990-15 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C45

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031354.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	78978	89391	9.88%	1.662%
2	1.532	145	153	165	rVB	73702	87114	9.62%	1.620%
3	2.060	306	317	334	rBV	152046	222311	24.56%	4.133%
4	2.449	427	438	452	rBV2	22983	40376	4.46%	0.751%
5	3.831	851	868	901	rBV4	44200	200052	22.10%	3.719%
6	4.256	983	1000	1023	rBV	97869	250171	27.64%	4.651%
7	4.963	1204	1220	1249	rBV2	212194	551211	60.90%	10.248%
8	5.542	1389	1400	1422	rBV	140025	298236	32.95%	5.545%
9	5.838	1480	1492	1509	rBV3	104173	219293	24.23%	4.077%
10	5.995	1529	1541	1566	rBV2	127339	272152	30.07%	5.060%
11	6.921	1817	1829	1846	rBV	48147	96317	10.64%	1.791%
12	7.249	1916	1931	1965	rBV	222951	415145	45.86%	7.718%
13	7.564	2019	2029	2054	rBV	29919	59432	6.57%	1.105%
14	7.911	2123	2137	2158	rBV	523879	905155	100.00%	16.829%
15	8.040	2166	2177	2215	rBV	200217	475273	52.51%	8.836%
16	8.792	2399	2411	2434	rBV	219707	383220	42.34%	7.125%
17	10.159	2826	2836	2854	rBV	89607	146444	16.18%	2.723%
18	11.191	3147	3157	3183	rBV	203723	325779	35.99%	6.057%
19	11.567	3263	3274	3297	rBV	211595	341517	37.73%	6.350%




Sum of corrected areas: 5378589

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031354.D
Acq On : 05 Jun 2023 18:03
Operator : SY/MD
Sample : 02990-15 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

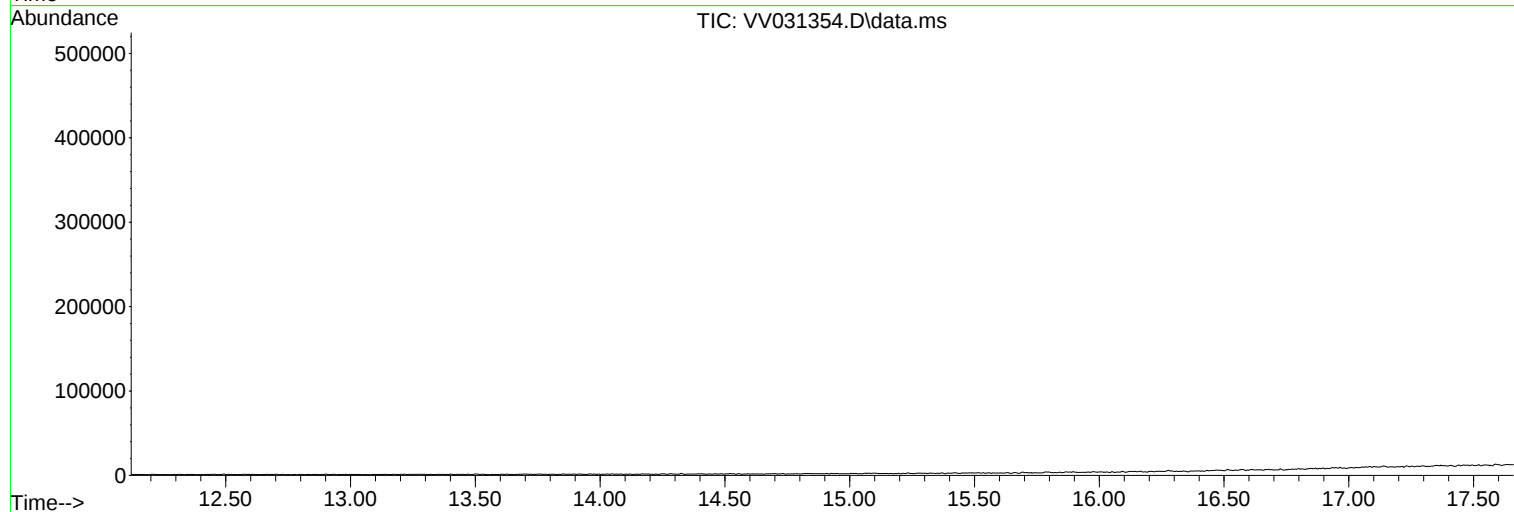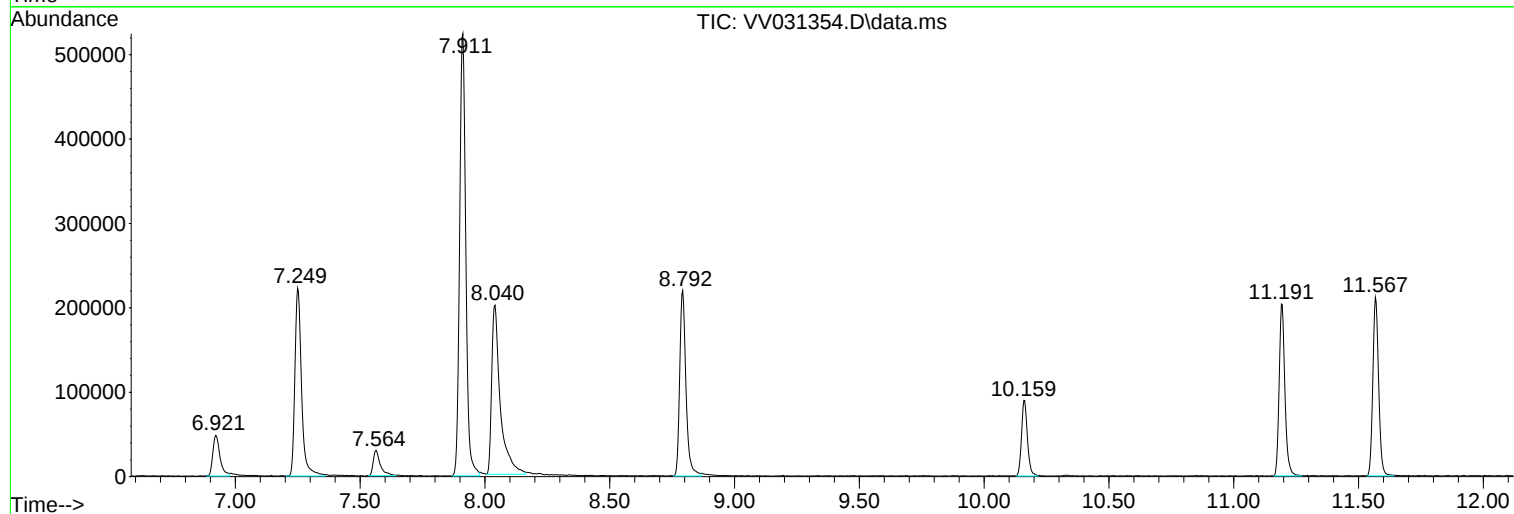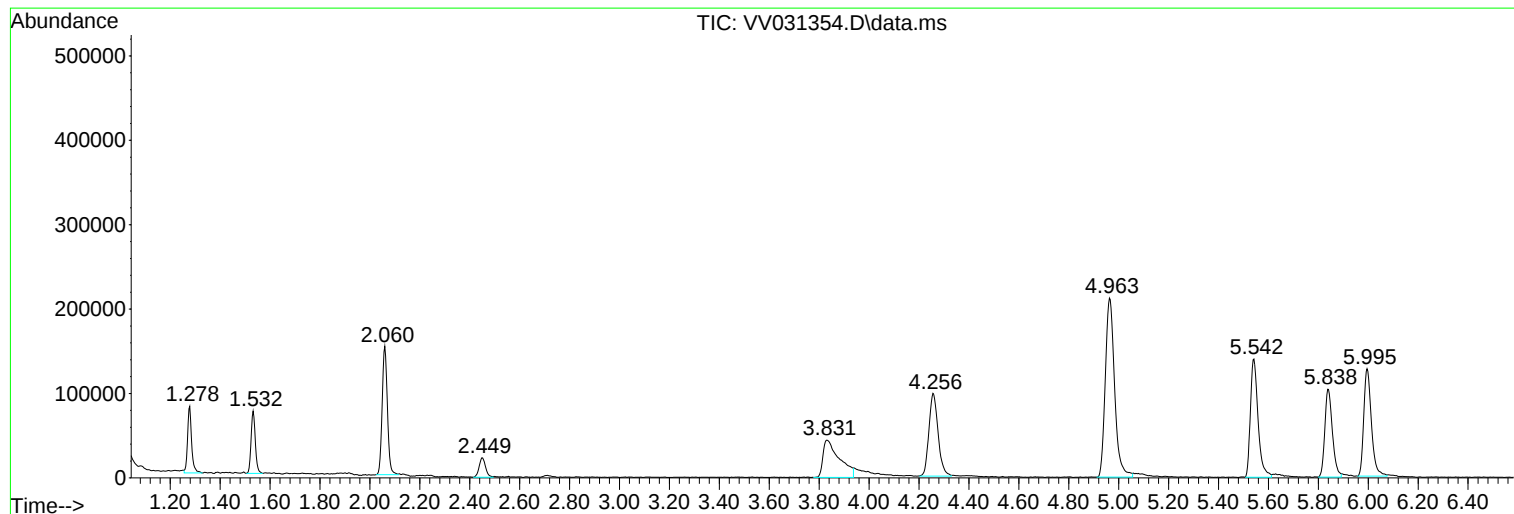

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031354.D
Acq On : 05 Jun 2023 18:03
Operator : SY/MD
Sample : 02990-15 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031354.D
Acq On : 05 Jun 2023 18:03
Operator : SY/MD
Sample : 02990-15 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------