

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
 Data File : VV031355.D
 Acq On : 05 Jun 2023 18:28
 Operator : SY/MD
 Sample : VIBLK301
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK301

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031355.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	87	rVB	74885	81011	16.02%	2.024%
2	1.532	145	153	164	rVB	68400	78870	15.60%	1.970%
3	2.060	305	317	330	rBV	143672	208593	41.26%	5.210%
4	2.449	428	438	452	rVB2	8660	15857	3.14%	0.396%
5	3.834	856	869	899	rBV2	38225	158141	31.28%	3.950%
6	4.256	984	1000	1025	rVB	87798	228369	45.17%	5.704%
7	4.963	1205	1220	1246	rBV3	198558	505554	100.00%	12.628%
8	5.542	1388	1400	1423	rBV	137402	292008	57.76%	7.294%
9	5.838	1481	1492	1500	rBV9	4893	10286	2.03%	0.257%
10	5.995	1525	1541	1564	rBV2	116056	254438	50.33%	6.355%
11	6.921	1815	1829	1846	rBV	45086	89909	17.78%	2.246%
12	7.249	1918	1931	1959	rBV	198957	369396	73.07%	9.227%
13	7.564	2019	2029	2047	rBV	27344	55851	11.05%	1.395%
14	7.911	2130	2137	2148	rVB7	3907	6963	1.38%	0.174%
15	8.037	2165	2176	2219	rBV	178328	479167	94.78%	11.969%
16	8.365	2270	2278	2291	rBV4	6023	12224	2.42%	0.305%
17	8.792	2400	2411	2432	rBV	220035	372453	73.67%	9.303%
18	10.159	2825	2836	2857	rBV2	84381	139006	27.50%	3.472%
19	11.194	3147	3158	3183	rBV	194564	324781	64.24%	8.112%
20	11.567	3262	3274	3292	rBV	195872	320613	63.42%	8.008%




Sum of corrected areas: 4003490

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031355.D
Acq On : 05 Jun 2023 18:28
Operator : SY/MD
Sample : VIBLK301
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK301

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

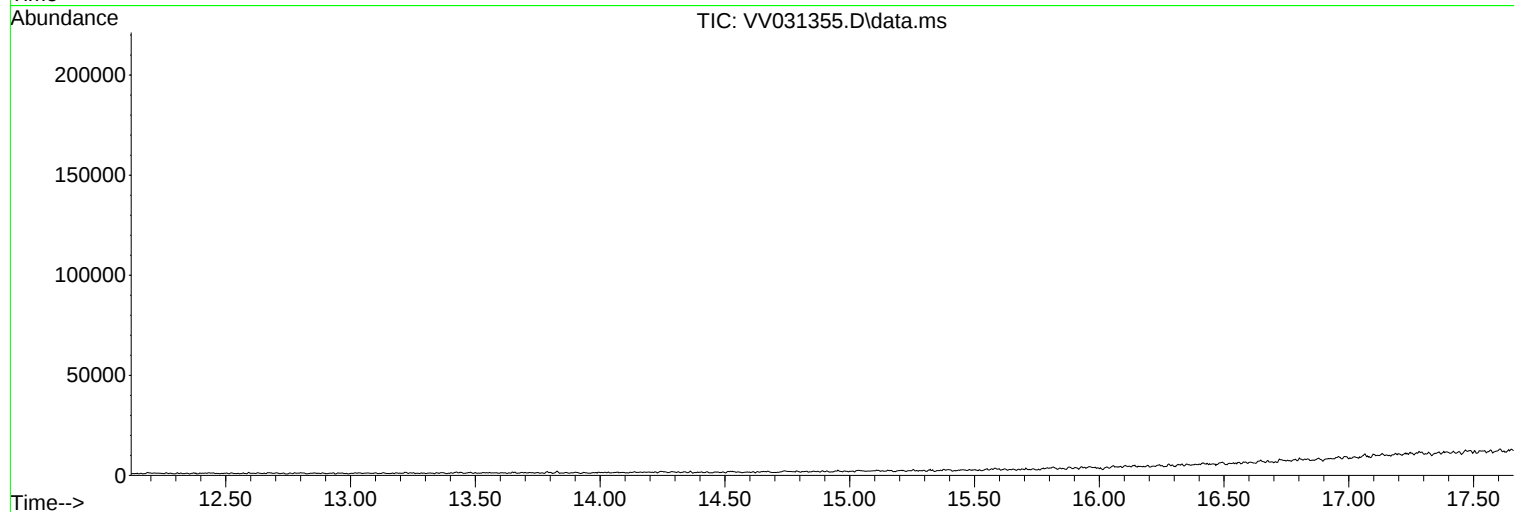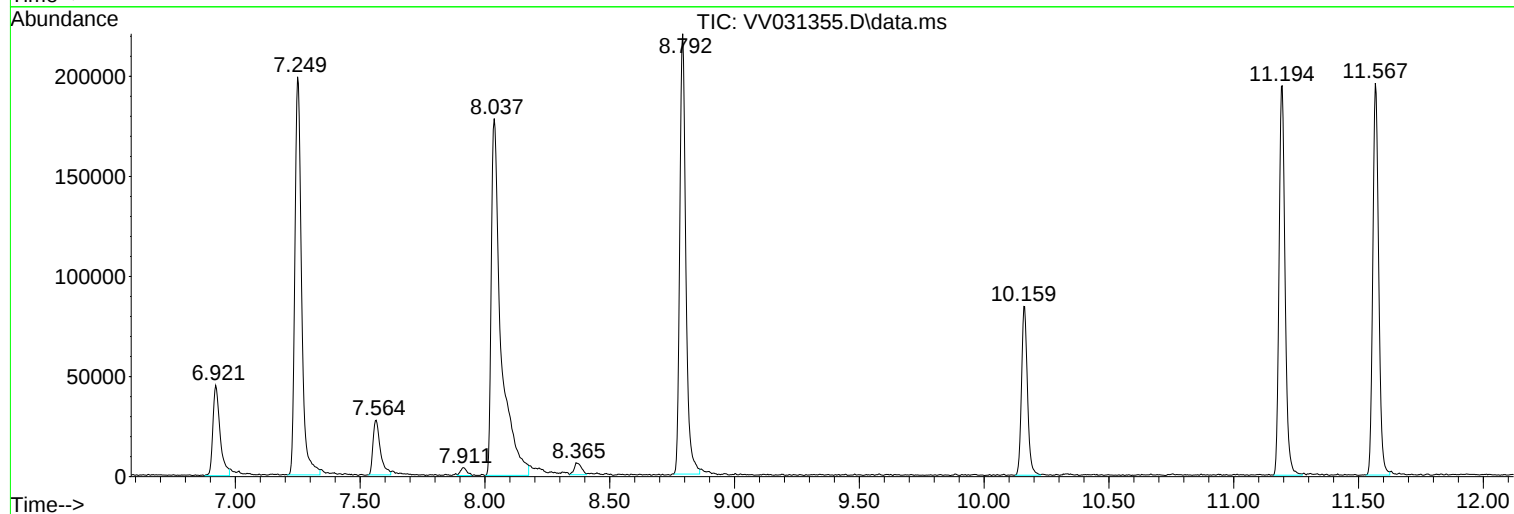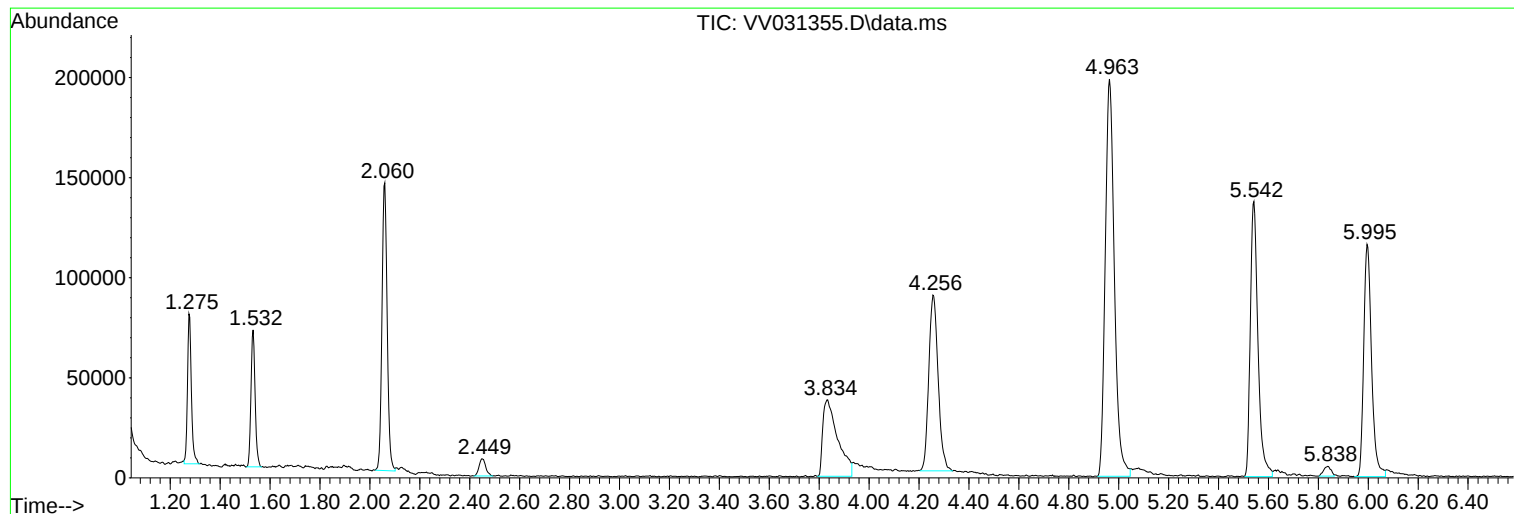

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031355.D
Acq On : 05 Jun 2023 18:28
Operator : SY/MD
Sample : VIBLK301
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK301

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031355.D
Acq On : 05 Jun 2023 18:28
Operator : SY/MD
Sample : VIBLK301
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK301

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------