


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060523\
Data File : VV031336.D
Acq On : 05 Jun 2023 09:15
Operator : SY/MD
Sample : BFB270
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB270

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Jun 07 01:59:39 2023

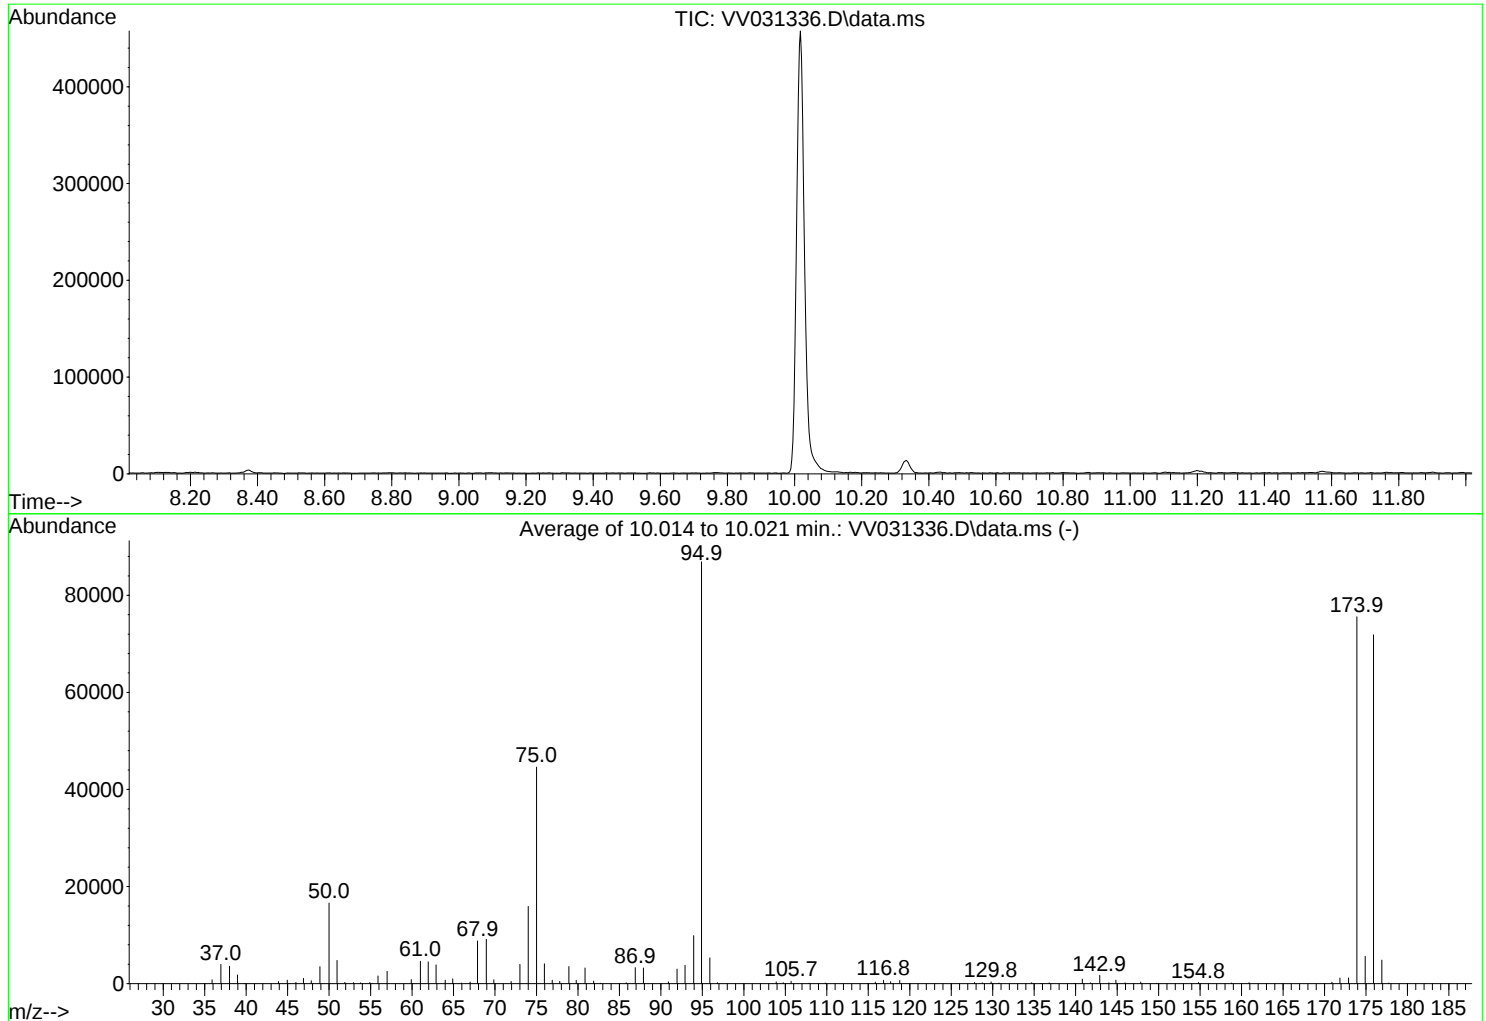

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	16626	PASS
75	95	30	80	51.3	44613	PASS
95	95	100	100	100.0	86893	PASS
96	95	5	9	6.1	5305	PASS
173	174	0.00	2	1.6	1196	PASS
174	95	50	120	87.0	75571	PASS
175	174	5	9	7.4	5625	PASS
176	174	95	105	95.1	71848	PASS
177	176	5	10	6.7	4846	PASS

m/z	Abundance
39.90	538.0
44.00	256.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270

m/z	Abundance
35.90	817.0
36.90	3975.0
38.00	3599.0
39.00	1745.0
39.80	594.0
43.90	715.0
44.90	776.0
46.00	199.0
46.90	1061.0
47.90	561.0
48.90	3488.0
50.00	16888.0
50.90	4774.0
51.90	244.0
52.90	180.0
53.80	120.0
54.90	246.0
55.90	1734.0
57.00	2550.0
59.90	896.0
61.00	4445.0
61.90	4394.0
62.90	3744.0
64.00	742.0
64.90	1018.0
66.00	148.0
67.00	247.0
67.90	9072.0
69.00	9134.0
69.80	769.0
71.90	503.0
73.00	3957.0
74.00	16332.0
75.00	44656.0
75.90	4251.0
76.90	666.0
77.80	506.0
78.90	3484.0
79.80	732.0
80.90	3251.0
81.90	526.0
82.70	130.0
85.80	210.0
86.90	3220.0
87.90	3296.0
90.90	370.0
92.00	2843.0
92.90	3800.0
93.90	9873.0
94.90	86960.0
95.90	5552.0
96.80	173.0
103.90	400.0
104.70	199.0
105.70	452.0
107.80	108.0
109.80	117.0
114.90	129.0
115.80	350.0
116.80	731.0
117.70	397.0
118.80	618.0
127.80	232.0
128.70	159.0
129.80	405.0
130.80	104.0
134.70	211.0
136.90	178.0
139.80	114.0
140.80	901.0
141.90	177.0
142.90	1696.0
144.00	139.0
144.80	667.0
145.90	146.0
147.80	261.0
149.70	126.0
154.80	208.0
158.70	161.0
161.00	158.0
170.90	249.0
171.80	1097.0
172.90	1190.0
173.90	74864.0
174.90	5683.0
175.90	71104.0
176.90	5018.0
177.70	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270

m/z	Abundance
35.90	829.0
37.00	3994.0
38.00	3692.0
38.90	1836.0
39.80	571.0
43.90	691.0
45.00	728.0
46.00	263.0
46.90	1151.0
47.90	592.0
48.90	3619.0
50.00	17336.0
50.90	4853.0
51.90	290.0
52.90	200.0
53.80	187.0
54.90	240.0
55.90	1683.0
57.00	2656.0
59.90	842.0
61.00	4828.0
61.90	4624.0
62.90	3988.0
64.00	698.0
64.90	1037.0
65.90	154.0
67.00	245.0
67.90	9049.0
68.90	9416.0
69.80	825.0
72.00	486.0
73.00	4073.0
74.00	16576.0
75.00	46136.0
75.90	4245.0
76.90	731.0
77.80	500.0
78.90	3663.0
79.80	720.0
80.80	3277.0
81.90	531.0
82.80	128.0
85.80	197.0
86.90	3377.0
87.90	3401.0
90.90	391.0
91.90	3133.0
92.90	3858.0
93.90	10218.0
94.90	89448.0
95.90	5410.0
96.80	200.0
103.90	387.0
104.70	197.0
105.70	517.0
107.80	119.0
109.80	127.0
115.80	348.0
116.80	692.0
117.70	408.0
118.80	685.0
127.80	255.0
128.80	170.0
129.80	369.0
130.70	149.0
134.70	225.0
136.80	153.0
139.80	109.0
140.80	935.0
141.80	155.0
142.90	1741.0
144.00	164.0
144.80	744.0
145.90	176.0
147.90	341.0
149.80	116.0
154.80	221.0
158.80	140.0
160.90	219.0
170.90	290.0
171.90	1201.0
172.90	1222.0
173.90	77968.0
174.90	5786.0
175.90	74368.0
176.90	4978.0
177.70	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270

m/z	Abundance
35.90	785.0
36.90	3869.0
38.00	3472.0
38.90	1756.0
39.80	533.0
43.90	625.0
44.90	657.0
46.00	318.0
46.90	1097.0
47.80	611.0
48.90	3415.0
50.00	15655.0
51.00	4751.0
51.90	236.0
53.00	207.0
53.80	201.0
54.90	238.0
55.90	1312.0
57.00	2457.0
59.90	779.0
61.00	4578.0
62.00	4482.0
62.90	3828.0
64.00	753.0
64.90	947.0
65.90	138.0
66.90	233.0
67.10	237.0
67.90	8272.0
68.90	8872.0
69.90	741.0
72.00	429.0
73.00	3817.0
74.00	14891.0
75.00	43048.0
76.00	3764.0
76.90	730.0
77.80	390.0
78.90	3406.0
79.80	643.0
80.80	3199.0
81.90	540.0
85.80	148.0
86.90	3256.0
87.90	3018.0
90.90	366.0
91.90	3004.0
92.90	3681.0
94.00	9617.0
94.90	84272.0
95.90	4954.0
96.80	193.0
103.90	354.0
104.80	182.0
105.70	471.0
107.90	103.0
109.80	115.0
115.90	312.0
116.90	653.0
117.70	368.0
118.80	706.0
127.80	245.0
128.80	176.0
129.80	325.0
130.70	174.0
134.70	201.0
135.80	129.0
136.70	144.0
140.80	941.0
141.70	157.0
142.90	1668.0
144.00	161.0
144.90	751.0
146.00	221.0
147.90	365.0
154.80	219.0
158.80	123.0
160.80	219.0
170.90	315.0
171.90	1193.0
172.90	1176.0
173.90	73880.0
174.90	5406.0
175.90	70072.0
176.90	4541.0
177.80	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB270