




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV060525\  
Data File : VV038753.D  
Acq On : 05 Jun 2025 10:26  
Operator : SY/MD  
Sample : VSTDCCC005  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
LabSampleId :  
VSTDCCC005

Manual IntegrationsAPPROVED

Quant Time: Jun 09 08:03:49 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR060625WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Fri Jun 06 12:50:11 2025  
Response via : Initial Calibration

Reviewed By :John Carlone 06/11/2025  
Supervised By :Mahesh Dadoda 06/11/2025

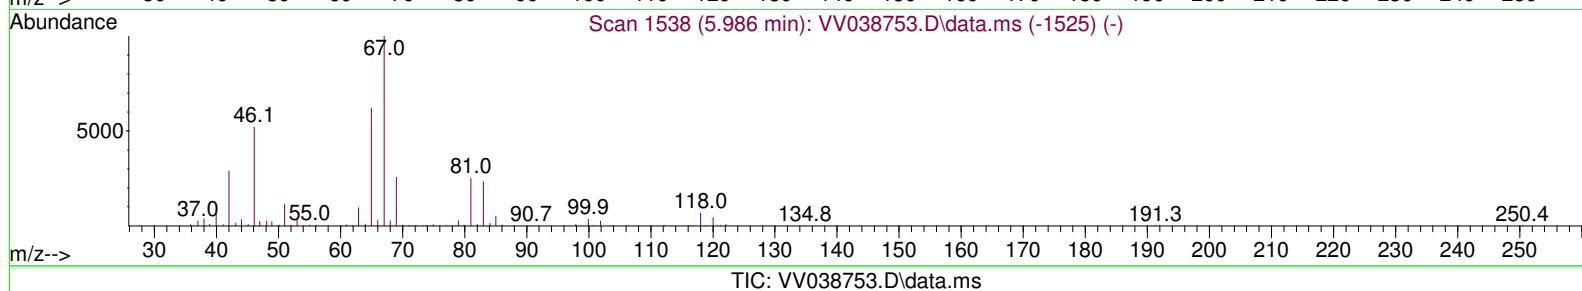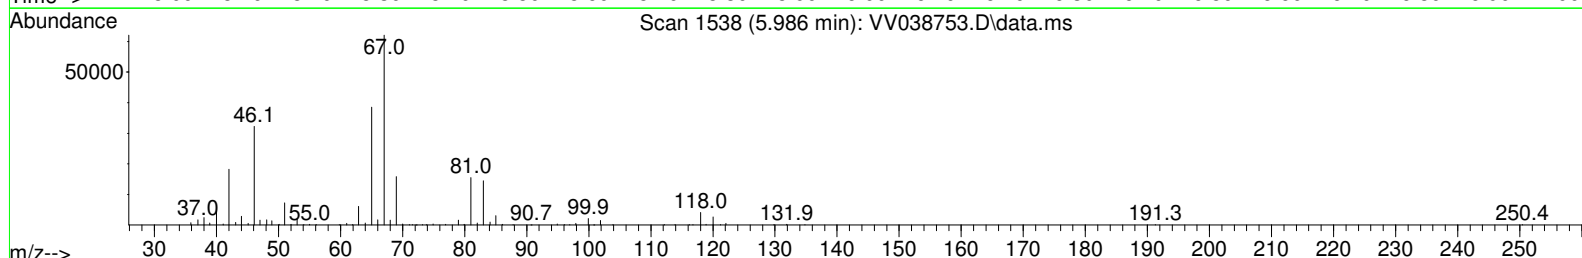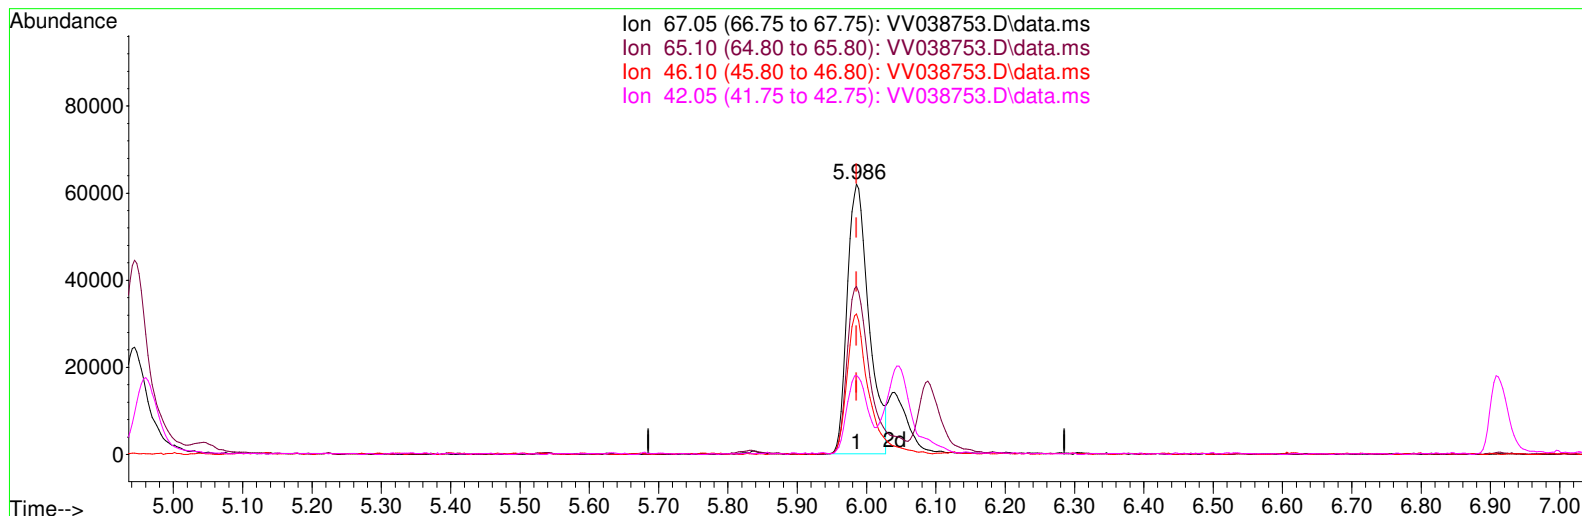

(36) 1,2-Dichloropropane-d6 (S)

5.986min (+ 0.000) 3.98 ug/L

response 135420

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 67.05 | 100.00 | 100.00 |
| 65.10 | 69.80  | 68.36  |
| 46.10 | 50.70  | 51.17  |
| 42.05 | 27.70  | 28.33  |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV060525\  
Data File : VV038753.D  
Acq On : 05 Jun 2025 10:26  
Operator : SY/MD  
Sample : VSTDCCC005  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
LabSampleId :  
VSTDCCC005

Manual IntegrationsAPPROVED

Quant Time: Jun 09 08:03:49 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR060625WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Fri Jun 06 12:50:11 2025  
Response via : Initial Calibration

Reviewed By :John Carlone 06/11/2025  
Supervised By :Mahesh Dadoda 06/11/2025

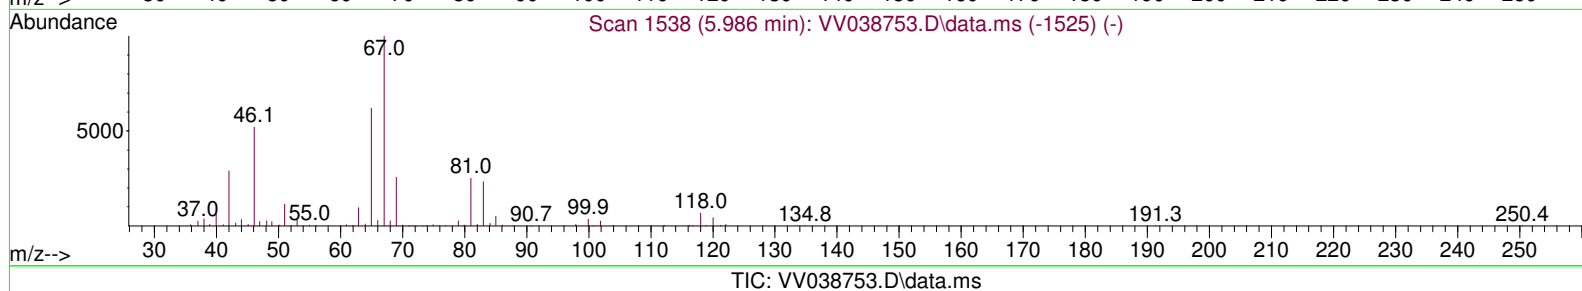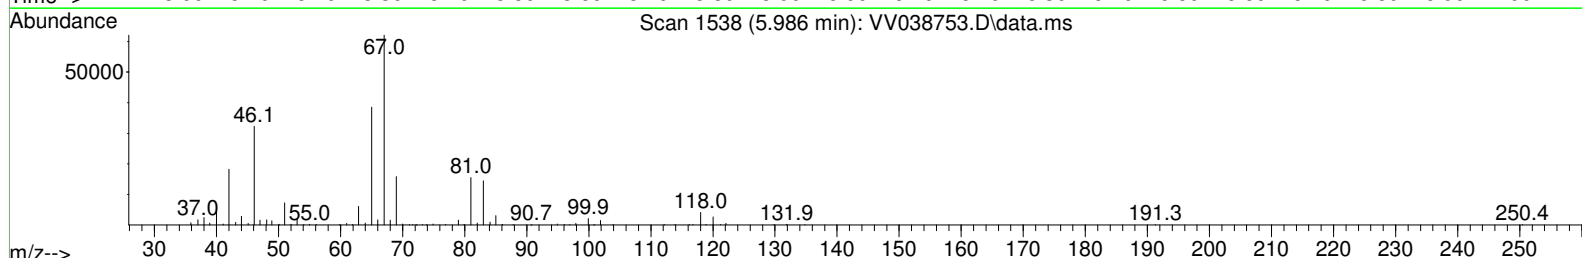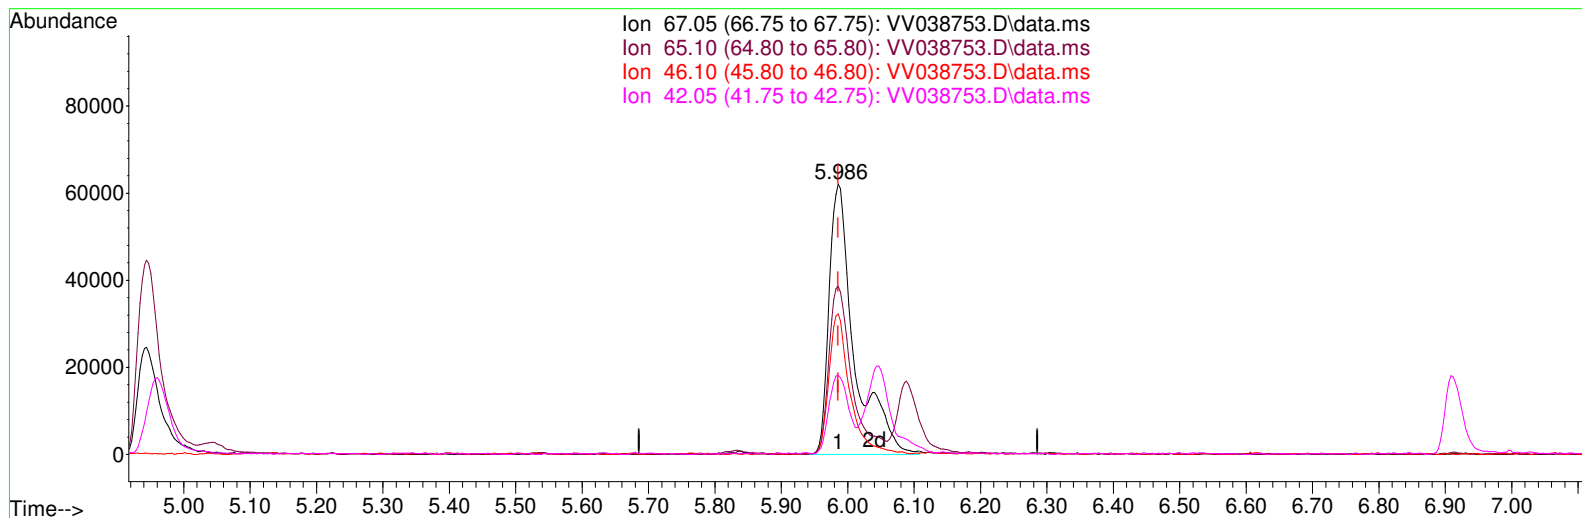

(36) 1,2-Dichloropropane-d6 (S)

5.986min (+ 0.000) 4.84 ug/L m

response 164700

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 67.05 | 100.00 | 100.00 |
| 65.10 | 69.80  | 56.21  |
| 46.10 | 50.70  | 42.07  |
| 42.05 | 27.70  | 23.29  |