
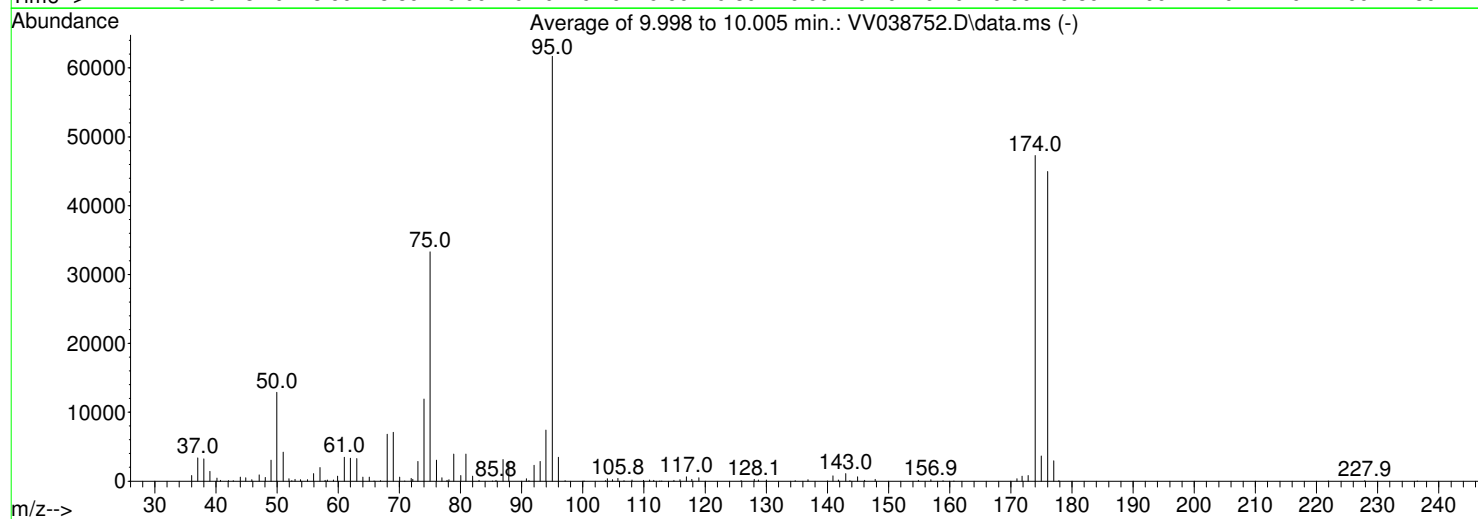


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060525\
Data File : VV038752.D
Acq On : 05 Jun 2025 09:20
Operator : SY/MD
Sample : BFB207
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB207

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jun 13 08:57:28 2025

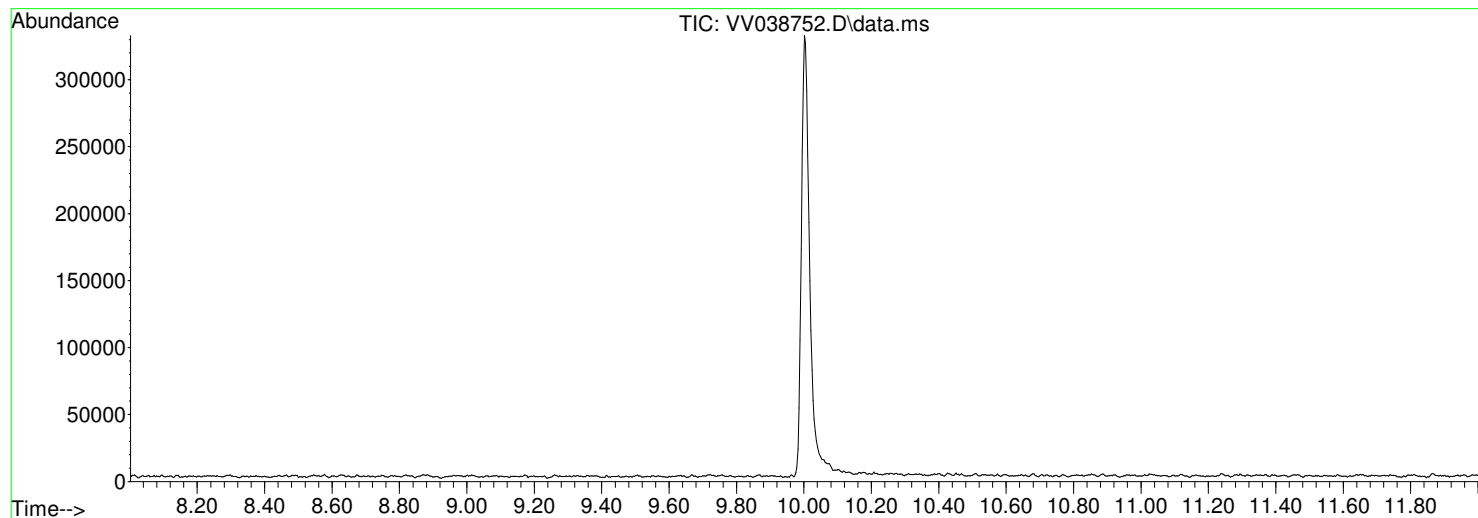

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2776

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	12904	PASS
75	95	30	80	53.9	33280	PASS
95	95	100	100	100.0	61691	PASS
96	95	5	9	5.6	3480	PASS
173	174	0.00	2	1.8	829	PASS
174	95	50	120	76.6	47283	PASS
175	174	5	9	7.7	3634	PASS
176	174	95	105	95.0	44941	PASS
177	176	5	10	6.6	2961	PASS

m/z	Abundance
36.10	151.0
37.00	105.0
37.50	118.0
38.60	102.0
39.20	120.0
39.90	565.0
41.00	291.0
41.60	186.0
42.70	118.0
44.00	841.0
44.70	180.0
47.80	198.0
49.90	103.0
55.90	100.0
58.80	107.0
65.10	100.0
65.80	104.0
73.80	151.0
77.00	143.0
93.80	101.0
99.50	126.0
102.80	109.0
111.20	116.0
124.50	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	847.0
37.00	3433.0
38.00	3000.0
39.00	1539.0
40.20	371.0
41.00	182.0
42.10	138.0
42.90	182.0
44.00	1421.0
44.90	636.0
45.90	177.0
47.10	858.0
48.00	524.0
49.00	2912.0
50.00	12836.0
51.00	3971.0
51.90	330.0
52.40	199.0
53.00	194.0
53.80	203.0
55.00	181.0
56.00	1020.0
57.00	1911.0
57.90	124.0
58.20	137.0
59.20	144.0
59.90	738.0
61.00	3439.0
62.00	3180.0
63.00	3263.0
64.00	667.0
65.10	622.0
68.00	6202.0
69.00	6761.0
70.00	484.0
71.90	340.0
73.00	2664.0
74.00	11582.0
75.00	31680.0
76.00	2839.0
76.90	672.0
78.10	293.0
78.90	3874.0
80.00	843.0
80.90	3638.0
81.90	642.0
83.10	107.0
85.20	108.0
85.80	152.0
86.90	2666.0
87.90	2852.0
90.70	300.0
91.20	239.0
92.00	2416.0
93.00	2653.0
94.00	7469.0
95.00	58672.0
96.00	3542.0
97.10	148.0
103.00	129.0
103.90	404.0
104.80	220.0
105.70	339.0
108.10	136.0
109.80	110.0
110.90	192.0
111.60	119.0
112.90	119.0
115.00	146.0
115.90	183.0
117.00	623.0
117.80	282.0
119.00	472.0
128.00	286.0
128.70	127.0
130.10	173.0
136.80	176.0
140.90	798.0
141.80	169.0
143.00	1063.0
143.70	120.0
145.00	583.0
147.80	236.0
156.90	176.0
171.00	296.0
171.90	618.0
172.80	767.0
174.00	43296.0
175.00	3529.0
176.00	41696.0
177.00	2951.0
177.80	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

236.50

117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	1016.0
37.00	3607.0
38.00	3340.0
39.00	1626.0
40.10	457.0
40.70	181.0
42.00	112.0
42.90	173.0
44.00	1472.0
44.90	685.0
45.80	212.0
47.00	926.0
48.00	561.0
49.00	3173.0
50.00	13451.0
51.00	4268.0
51.90	350.0
52.90	249.0
53.80	238.0
55.00	192.0
56.00	1194.0
57.00	2115.0
57.80	148.0
58.20	187.0
59.20	196.0
59.90	747.0
61.00	3661.0
62.00	3475.0
63.10	3379.0
64.00	617.0
65.10	730.0
66.00	152.0
68.00	7029.0
69.00	7359.0
70.10	563.0
71.90	391.0
72.20	372.0
73.00	2963.0
74.00	12298.0
75.00	34416.0
76.10	3239.0
76.90	642.0
78.10	288.0
78.90	4053.0
80.10	883.0
80.90	4103.0
81.90	737.0
82.90	124.0
85.80	127.0
87.00	3280.0
87.90	2943.0
90.70	340.0
92.00	2362.0
93.00	2966.0
94.00	7757.0
95.00	63896.0
96.00	3595.0
100.20	104.0
103.00	113.0
104.00	317.0
104.90	236.0
105.70	408.0
106.80	123.0
108.00	167.0
109.90	129.0
110.90	175.0
111.60	153.0
112.60	104.0
114.90	129.0
115.90	191.0
116.90	600.0
117.80	286.0
119.00	503.0
125.90	129.0
128.00	280.0
128.70	171.0
130.00	180.0
134.80	110.0
136.80	271.0
140.90	790.0
141.80	193.0
143.00	1143.0
143.70	123.0
144.90	632.0
146.10	184.0
147.80	245.0
154.90	131.0
156.90	223.0
158.90	106.0
171.00	385.0
171.90	762.0
172.90	867.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

174.00	49120.0
175.00	3737.0
176.00	46584.0
177.00	3141.0
177.90	119.0
227.90	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	1045.0
37.00	3429.0
38.00	3325.0
39.00	1496.0
40.10	558.0
40.80	239.0
41.60	134.0
42.90	144.0
44.00	1378.0
44.90	683.0
45.80	208.0
47.00	885.0
48.10	513.0
49.00	3059.0
50.00	12734.0
51.00	4325.0
52.00	357.0
53.00	298.0
53.80	224.0
54.90	194.0
56.00	1312.0
57.00	1935.0
57.80	141.0
58.20	190.0
59.20	191.0
59.90	683.0
61.00	3263.0
62.00	3380.0
63.10	3185.0
64.00	516.0
65.00	665.0
65.90	218.0
66.90	164.0
68.00	7195.0
69.00	7212.0
70.10	729.0
70.90	118.0
71.90	393.0
72.20	387.0
73.00	2904.0
74.00	11936.0
75.00	33744.0
76.10	3122.0
77.00	585.0
77.80	306.0
78.90	3893.0
80.00	769.0
80.90	3979.0
82.00	745.0
83.00	128.0
85.80	106.0
87.00	3532.0
87.90	2805.0
90.80	358.0
92.00	2117.0
93.00	2939.0
94.00	7377.0
95.00	62504.0
96.00	3304.0
103.70	251.0
104.10	295.0
104.90	195.0
105.80	415.0
106.70	138.0
108.00	154.0
110.00	123.0
110.80	119.0
111.60	128.0
114.80	129.0
115.90	208.0
116.90	612.0
117.80	247.0
119.00	546.0
125.90	152.0
128.10	247.0
128.70	150.0
129.90	186.0
134.70	162.0
136.80	246.0
140.00	112.0
140.90	656.0
141.80	170.0
143.00	1108.0
144.90	659.0
146.10	229.0
147.80	225.0
154.90	189.0
156.90	206.0
158.90	179.0
160.70	131.0
171.00	397.0
171.80	751.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

172.90	852.0
174.00	49432.0
175.00	3635.0
176.00	46544.0
177.00	2791.0
221.90	115.0
227.90	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207