

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011247.D
 Acq On : 06 Jun 2019 16:14
 Operator : SY/MD
 Sample : K3228-11
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P10

Quant Time: Jun 07 01:57:07 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 07 01:28:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	164821	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	149991	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	62097	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	57130	4.57	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.40%
7) Chloroethane-d5	1.56	69	44853	4.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.40%
11) 1,1-Dichloroethene-d2	2.12	63	87153	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	3.94	46	129339	46.00	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.00%
24) Chloroform-d	4.40	84	97713	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.00%
26) 1,2-Dichloroethane-d4	5.08	65	53187	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.60%
32) Benzene-d6	5.09	84	202708	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
36) 1,2-Dichloropropane-d6	6.12	67	61534	4.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.00%
41) Toluene-d8	7.36	98	184175	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.40%
43) trans-1,3-Dichloropropene-	7.66	79	20310	3.85	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.00%
46) 2-Hexanone-d5	8.13	63	107968	48.51	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.02%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	41725	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	56786	4.63	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.60%


Target Compounds					Ovalue
13) Acetone	2.19	43	5291	2.807 ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011247.D
Acq On : 06 Jun 2019 16:14
Operator : SY/MD
Sample : K3228-11
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P10

Quant Time: Jun 07 01:57:07 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 07 01:28:31 2019
Response via : Initial Calibration

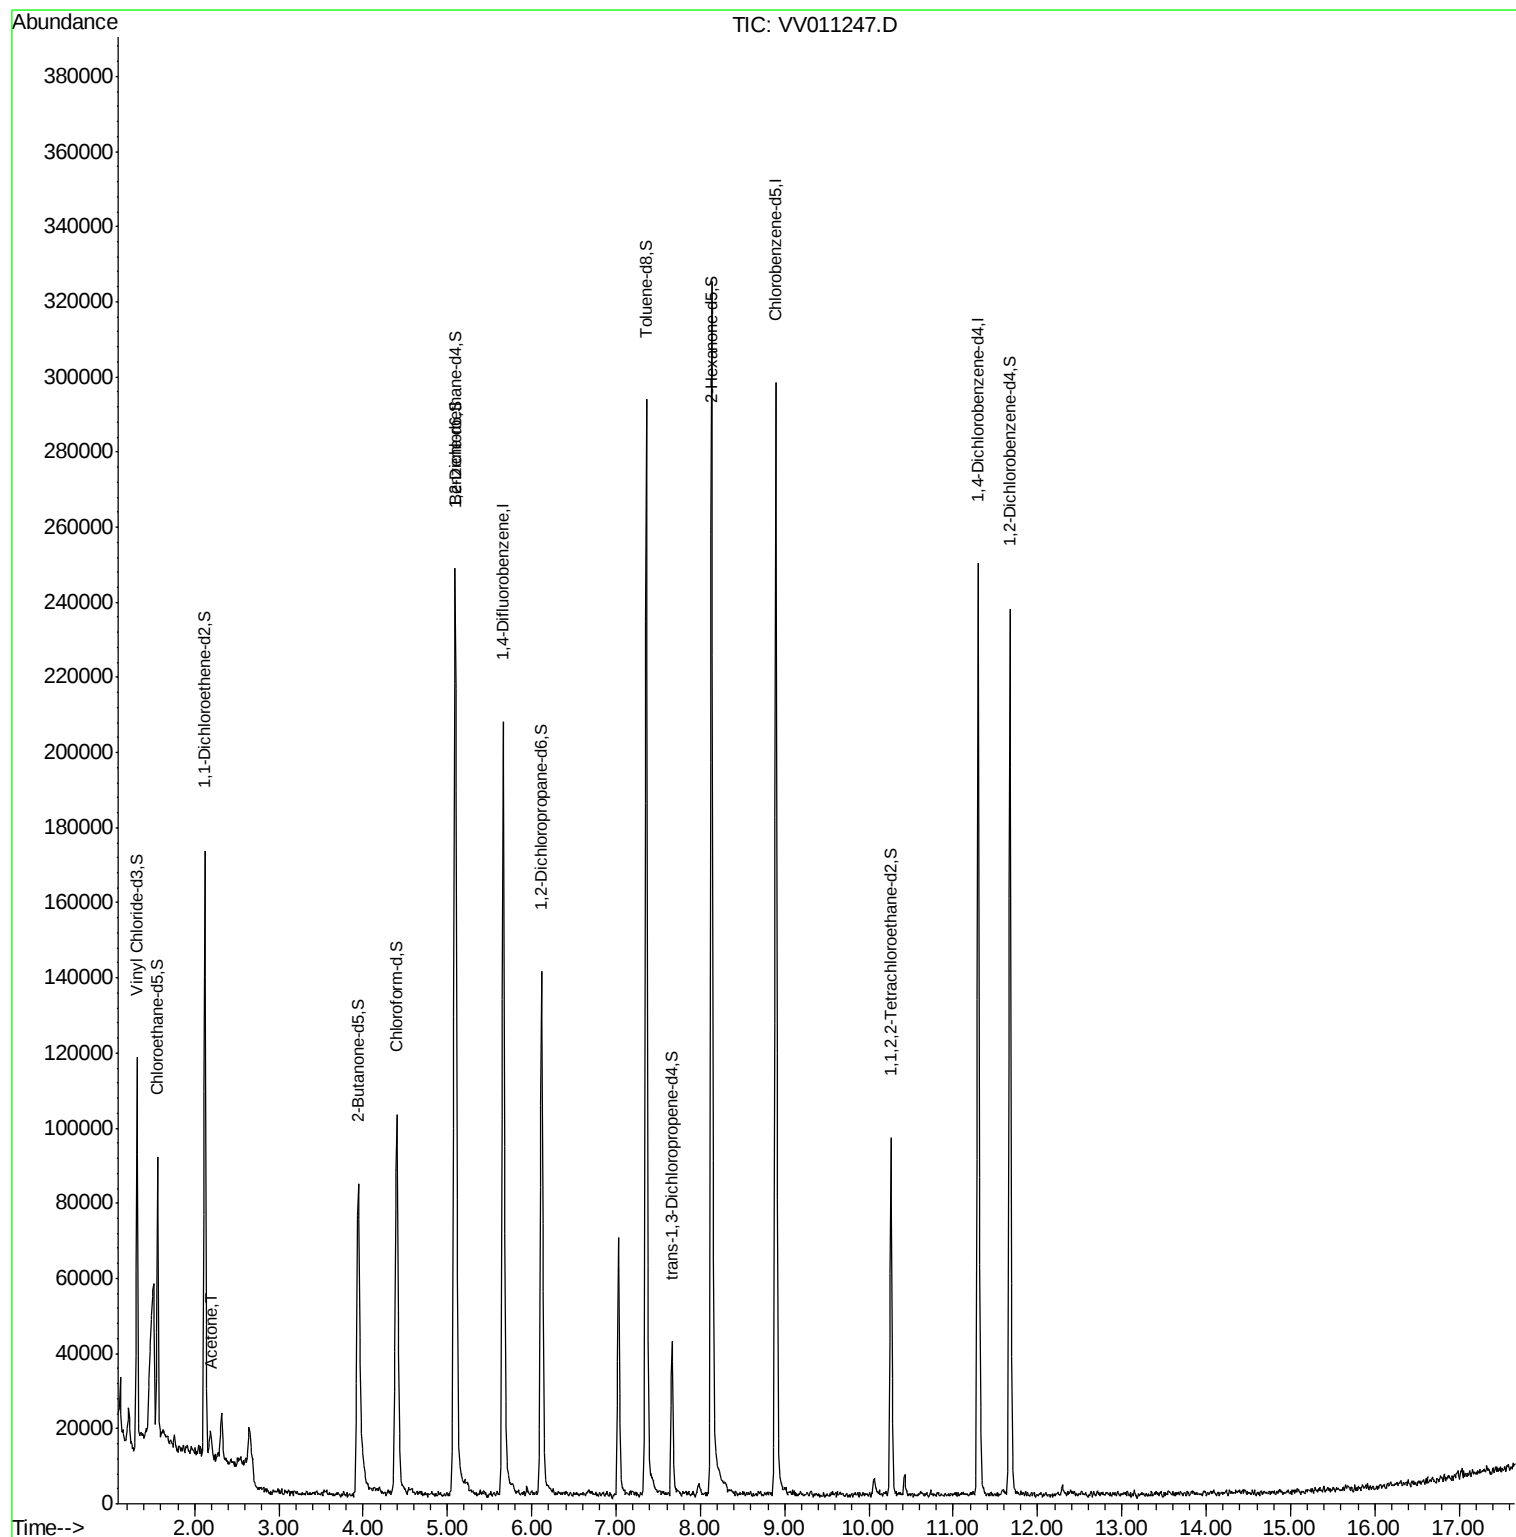

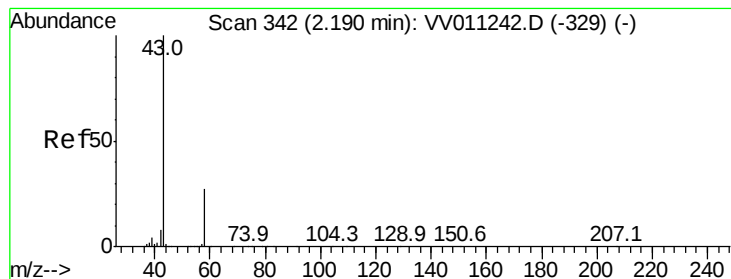

#13

Acetone

Concen: 2.807 ug/L

RT: 2.19 min Scan# 342

Delta R.T. 0.00 min

Lab File: VV011247.D

Acq: 06 Jun 2019 16:14

Instrument :
MSVOA_V
ClientSampleId :
F9P10

Tot Ion: 43 Resp: 5291

Ion Ratio Lower Upper

43 100

58 39.0 0.0 55.2

