

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011248.D
 Acq On : 06 Jun 2019 16:40
 Operator : SY/MD
 Sample : K3226-07
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCS2

Quant Time: Jun 07 02:03:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 07 01:28:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	163189	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	152289	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	61640	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	58502	4.73	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.60%
7) Chloroethane-d5	1.56	69	46713	4.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.80%
11) 1,1-Dichloroethene-d2	2.12	63	92557	3.75	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.00%
20) 2-Butanone-d5	3.94	46	131450	47.22	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.44%
24) Chloroform-d	4.40	84	100330	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.20%
26) 1,2-Dichloroethane-d4	5.08	65	55694	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
32) Benzene-d6	5.09	84	215830	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
36) 1,2-Dichloropropane-d6	6.12	67	64616	4.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.00%
41) Toluene-d8	7.36	98	197073	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.20%
43) trans-1,3-Dichloropropene-	7.66	79	20973	3.92	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.40%
46) 2-Hexanone-d5	8.13	63	107149	47.41	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.82%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	44086	4.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	59584	4.90	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.00%


Target Compounds					Ovalue
13) Acetone	2.19	43	4467	2.393 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011248.D
Acq On : 06 Jun 2019 16:40
Operator : SY/MD
Sample : K3226-07
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCS2

Quant Time: Jun 07 02:03:58 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 07 01:28:31 2019
Response via : Initial Calibration

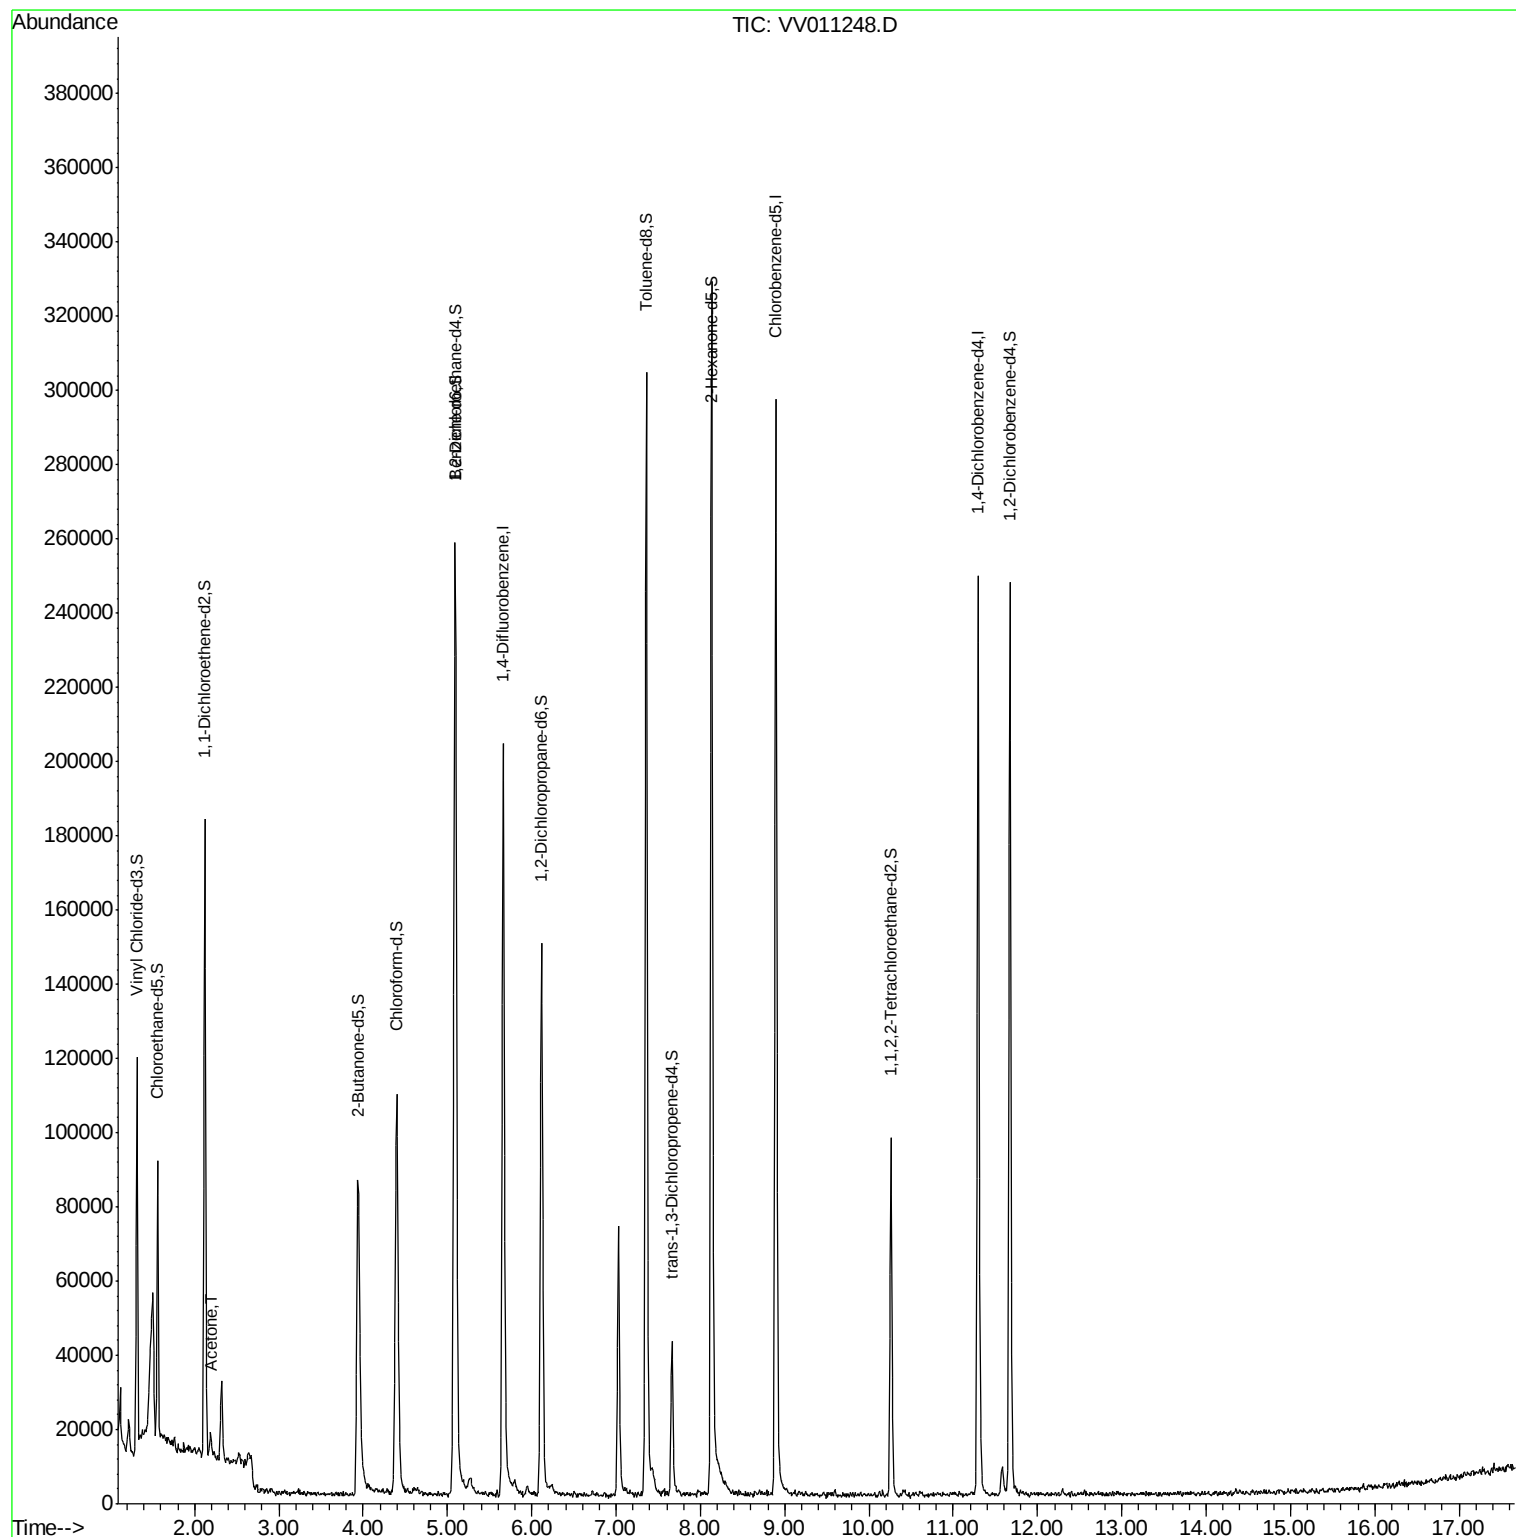

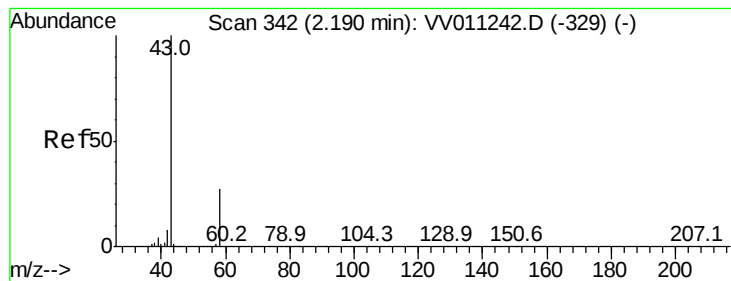

#13
 Acetone
 Concen: 2.393 ug/L
 RT: 2.19 min Scan# 342
 Delta R.T. 0.00 min
 Lab File: VV011248.D
 Acq: 06 Jun 2019 16:40

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCS2

Tot Ion: 43 Resp: 4467
 Ion Ratio Lower Upper
 43 100
 58 34.3 0.0 55.2

