

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011274.D
 Acq On : 07 Jun 2019 06:00
 Operator : SY/MD
 Sample : K3197-19
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P27

Quant Time: Jun 09 21:27:19 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 07 08:11:19 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	153820	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	137800	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	57409	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	52407	4.50	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.00%
7) Chloroethane-d5	1.57	69	37535	3.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.40%
11) 1,1-Dichloroethene-d2	2.12	63	83265	3.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.60%
20) 2-Butanone-d5	3.95	46	149401	56.94	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.88%
24) Chloroform-d	4.40	84	96535	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
26) 1,2-Dichloroethane-d4	5.08	65	55187	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
32) Benzene-d6	5.09	84	196189	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.20%
36) 1,2-Dichloropropane-d6	6.12	67	62018	4.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.60%
41) Toluene-d8	7.36	98	172415	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
43) trans-1,3-Dichloropropene-	7.67	79	18633	3.85	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.00%
46) 2-Hexanone-d5	8.13	63	113818	55.66	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.32%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	42585	4.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	55170	4.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	8026	4.562 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011274.D
Acq On : 07 Jun 2019 06:00
Operator : SY/MD
Sample : K3197-19
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P27

Quant Time: Jun 09 21:27:19 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 07 08:11:19 2019
Response via : Initial Calibration

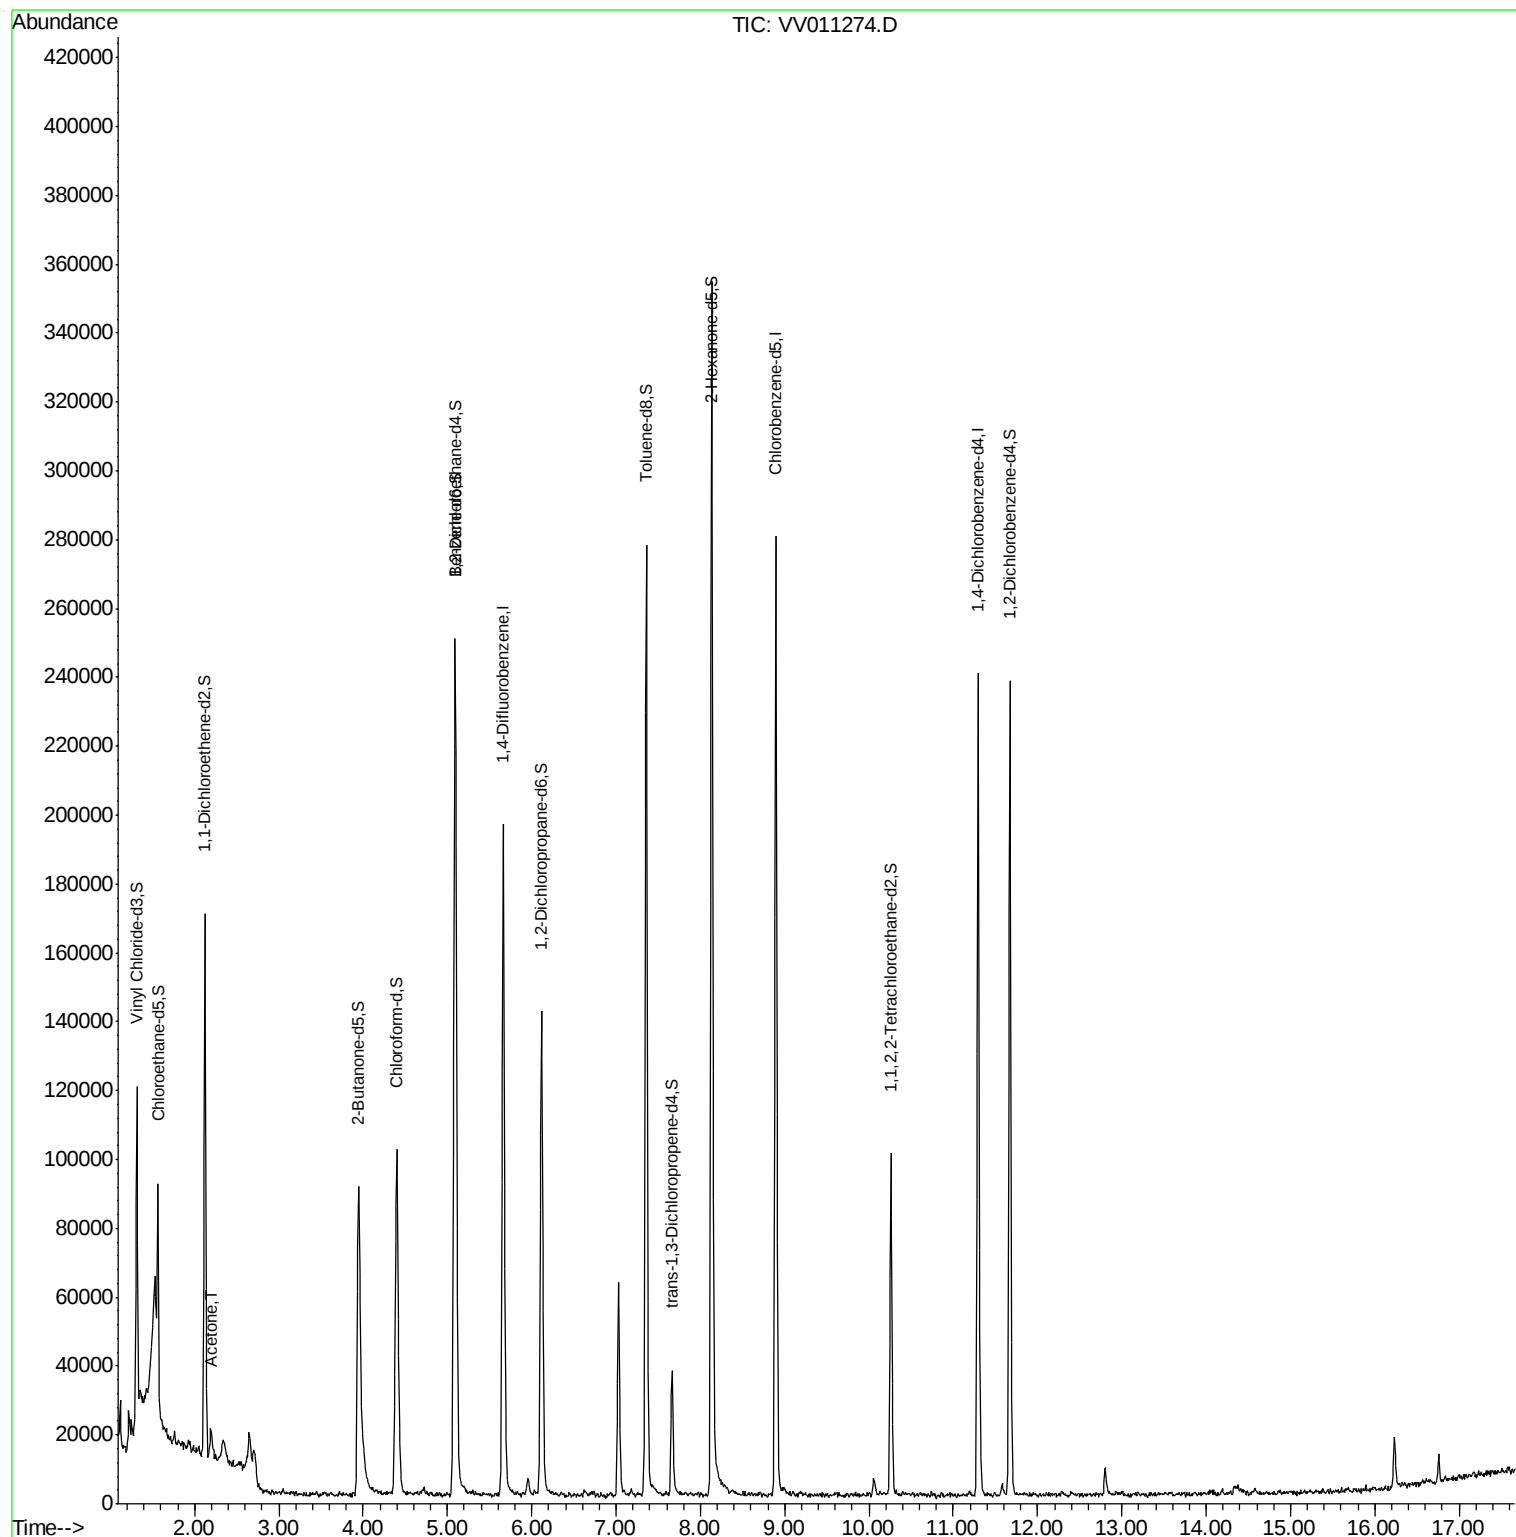

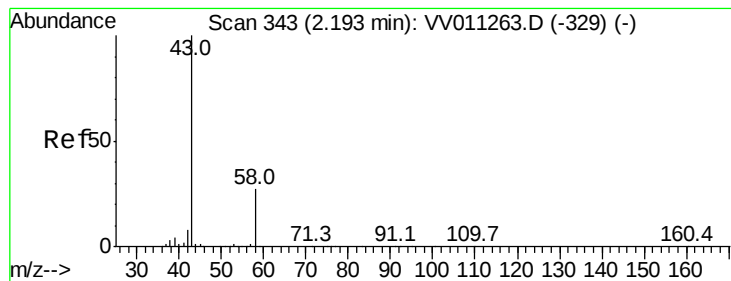

#13

Acetone

Concen: 4.562 ug/L

RT: 2.20 min Scan# 345

Delta R.T. 0.01 min

Lab File: VV011274.D

Acq: 07 Jun 2019 06:00

Instrument :
MSVOA_V
ClientSampleId :
F9P27

Tot Ion: 43 Resp: 8026

Ion Ratio Lower Upper

43 100

58 33.6 0.0 55.2

