

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011278.D
 Acq On : 07 Jun 2019 07:46
 Operator : SY/MD
 Sample : K3228-02
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P01

Quant Time: Jun 07 08:53:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 07 08:11:19 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	156099	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	144133	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	61398	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	53217	4.50	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.00%
7) Chloroethane-d5	1.56	69	44176	4.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.80%
11) 1,1-Dichloroethene-d2	2.12	63	86673	3.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.40%
20) 2-Butanone-d5	3.94	46	159154	59.77	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.54%
24) Chloroform-d	4.40	84	104640	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	5.08	65	58387	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.80%
32) Benzene-d6	5.09	84	208692	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
36) 1,2-Dichloropropane-d6	6.12	67	64808	4.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.60%
41) Toluene-d8	7.36	98	184049	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.00%
43) trans-1,3-Dichloropropene-	7.66	79	19522	3.86	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.20%
46) 2-Hexanone-d5	8.13	63	124026	57.98	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	115.96%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	47070	5.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	61284	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%


Target Compounds					Ovalue
13) Acetone	2.19	43	10196	5.711 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011278.D
Acq On : 07 Jun 2019 07:46
Operator : SY/MD
Sample : K3228-02
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P01

Quant Time: Jun 07 08:53:13 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 07 08:11:19 2019
Response via : Initial Calibration

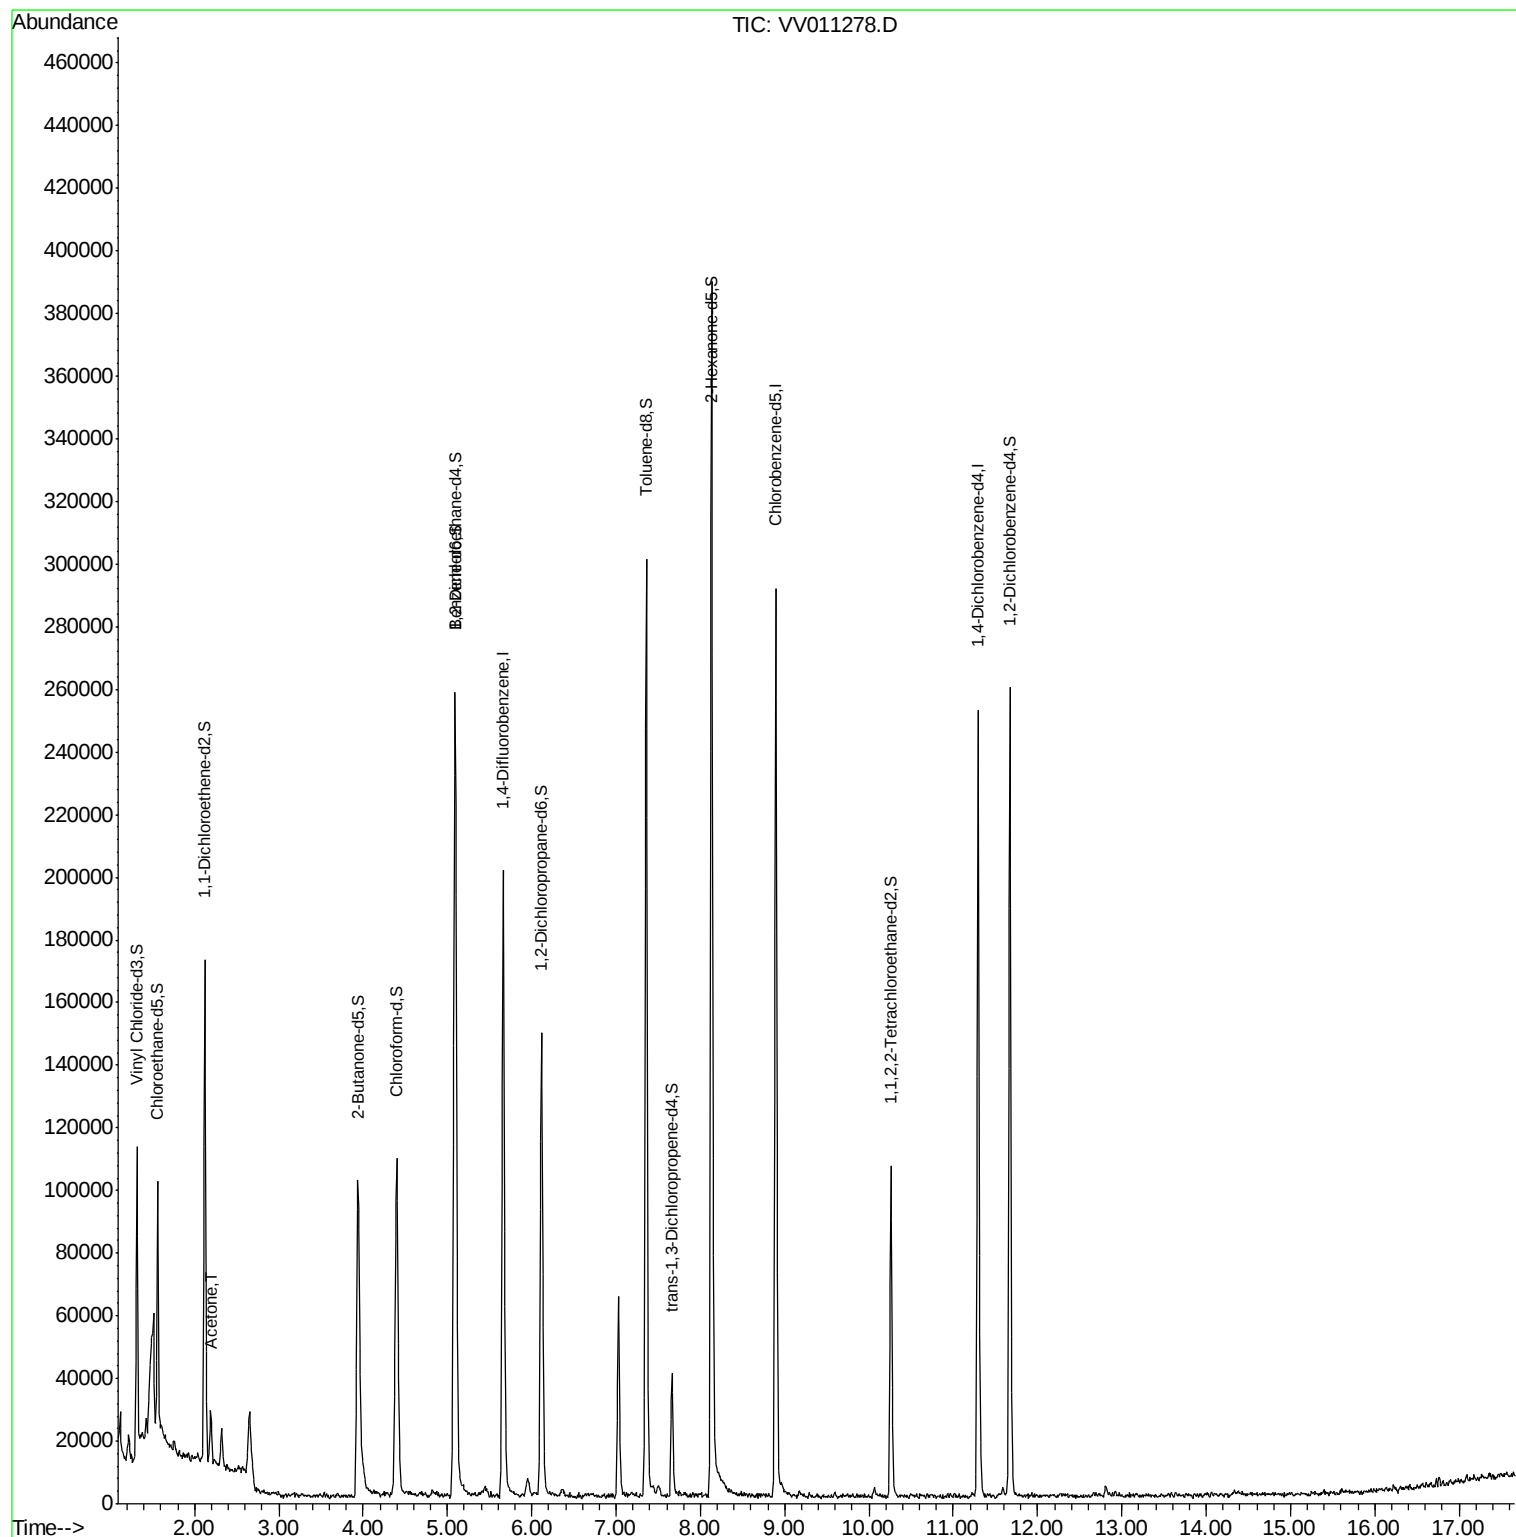

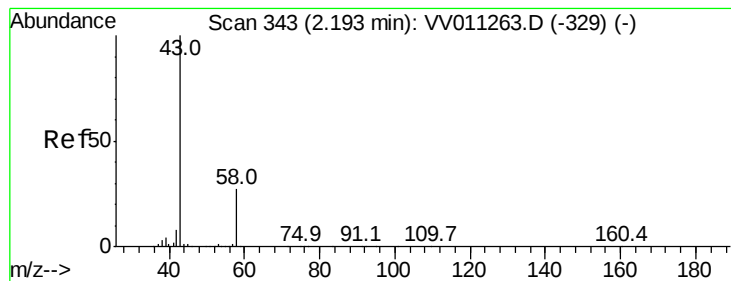

#13

Acetone

Concen: 5.711 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.00 min

Lab File: VV011278.D

Acq: 07 Jun 2019 07:46

Instrument :
MSVOA_V
ClientSampleId :
F9P01

Tot Ion: 43 Resp: 10196

Ion Ratio Lower Upper

43 100

58 31.0 0.0 55.2

