

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011283.D
 Acq On : 07 Jun 2019 10:03
 Operator : SY/MD
 Sample : K3228-07
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P06

Quant Time: Jun 08 00:36:26 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 08 00:01:28 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	158499	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	145810	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	57144	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	51815	4.31	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.20%
7) Chloroethane-d5	1.55	69	41425	4.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.00%
11) 1,1-Dichloroethene-d2	2.12	63	81384	3.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.80%
20) 2-Butanone-d5	3.94	46	148617	54.96	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.92%
24) Chloroform-d	4.40	84	95579	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
26) 1,2-Dichloroethane-d4	5.08	65	54944	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.20%
32) Benzene-d6	5.09	84	191910	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.00%
36) 1,2-Dichloropropane-d6	6.12	67	59827	4.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.00%
41) Toluene-d8	7.36	98	169286	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.60%
43) trans-1,3-Dichloropropene-	7.66	79	17199	3.36	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	67.20%
46) 2-Hexanone-d5	8.13	63	116030	53.62	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.24%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	43906	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	55077	4.88	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.60%


Target Compounds				Ovalue
13) Acetone	2.19	43	12040	6.641 ug/L 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011283.D
Acq On : 07 Jun 2019 10:03
Operator : SY/MD
Sample : K3228-07
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P06

Quant Time: Jun 08 00:36:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 08 00:01:28 2019
Response via : Initial Calibration

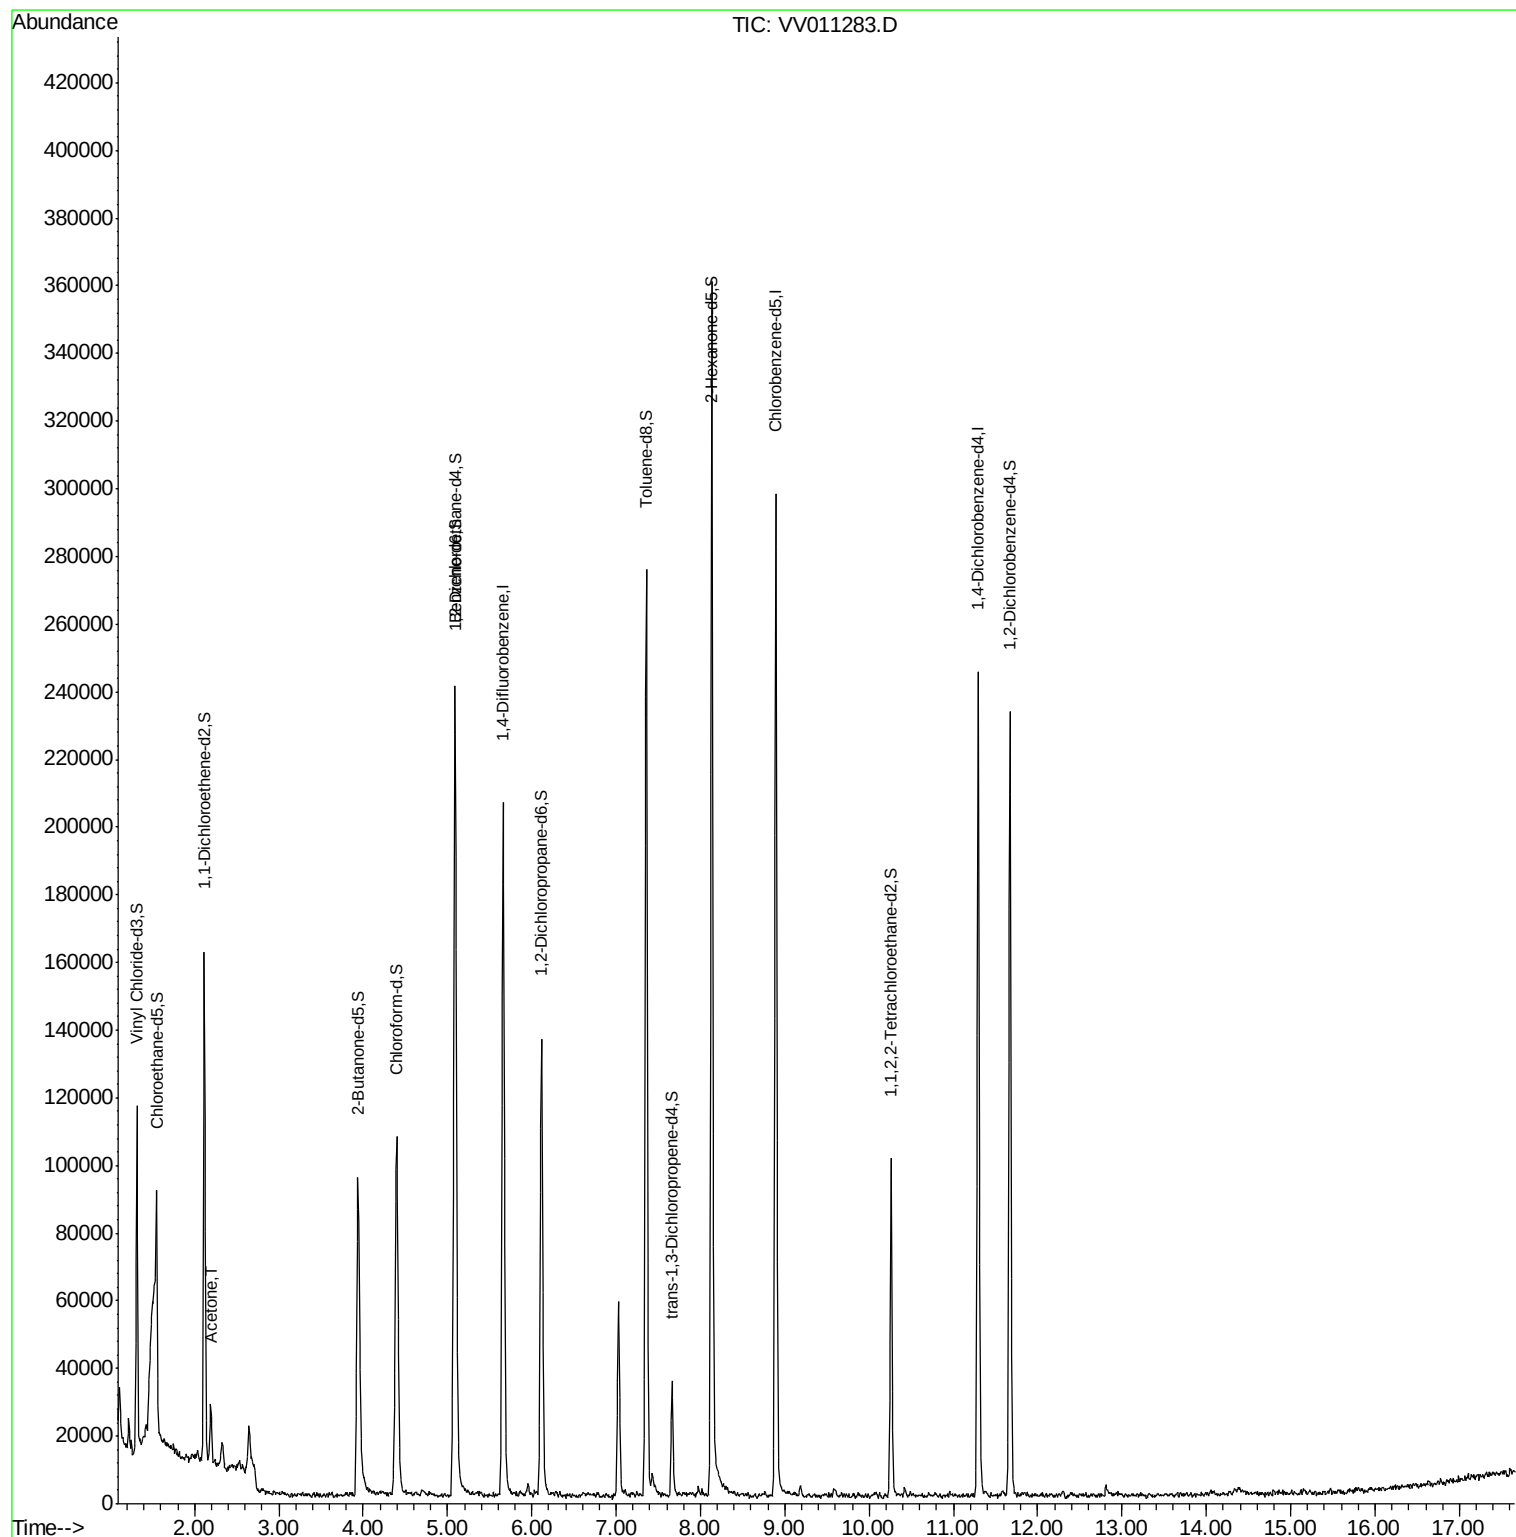

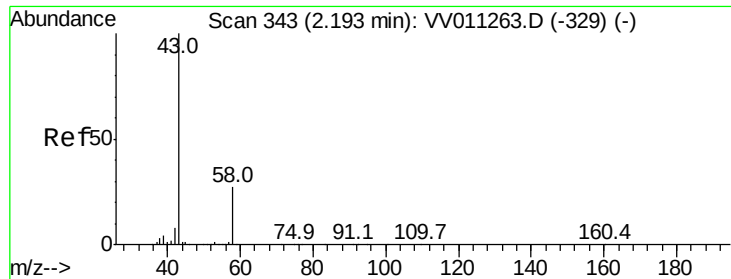

#13

Acetone

Concen: 6.641 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.00 min

Lab File: VV011283.D

Acq: 07 Jun 2019 10:03

Instrument :
MSVOA_V
ClientSampleId :
F9P06

Tot Ion: 43 Resp: 12040

Ion Ratio Lower Upper

43 100

58 28.2 0.0 55.2

