

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011287.D
 Acq On : 07 Jun 2019 14:40
 Operator : SY/MD
 Sample : K3230-07
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jun 08 00:57:00 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 08 00:40:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	166750	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	147875	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	60388	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	47573	3.77	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.40%
7) Chloroethane-d5	1.57	69	41880	3.99	ug/L	0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.80%
11) 1,1-Dichloroethene-d2	2.12	63	77318	3.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.20%
20) 2-Butanone-d5	3.95	46	129966	45.69	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.38%
24) Chloroform-d	4.40	84	93700	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.20%
26) 1,2-Dichloroethane-d4	5.08	65	51905	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.40%
32) Benzene-d6	5.09	84	183905	4.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.20%
36) 1,2-Dichloropropane-d6	6.12	67	58099	4.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.20%
41) Toluene-d8	7.36	98	161899	3.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.80%
43) trans-1,3-Dichloropropene-	7.66	79	17754	3.42	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.40%
46) 2-Hexanone-d5	8.14	63	97606	44.48	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.96%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	39091	4.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	50100	4.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.00%


Target Compounds					Ovalue
13) Acetone	2.20	43	4219	2.212 ug/L	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011287.D
Acq On : 07 Jun 2019 14:40
Operator : SY/MD
Sample : K3230-07
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jun 08 00:57:00 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 08 00:40:24 2019
Response via : Initial Calibration

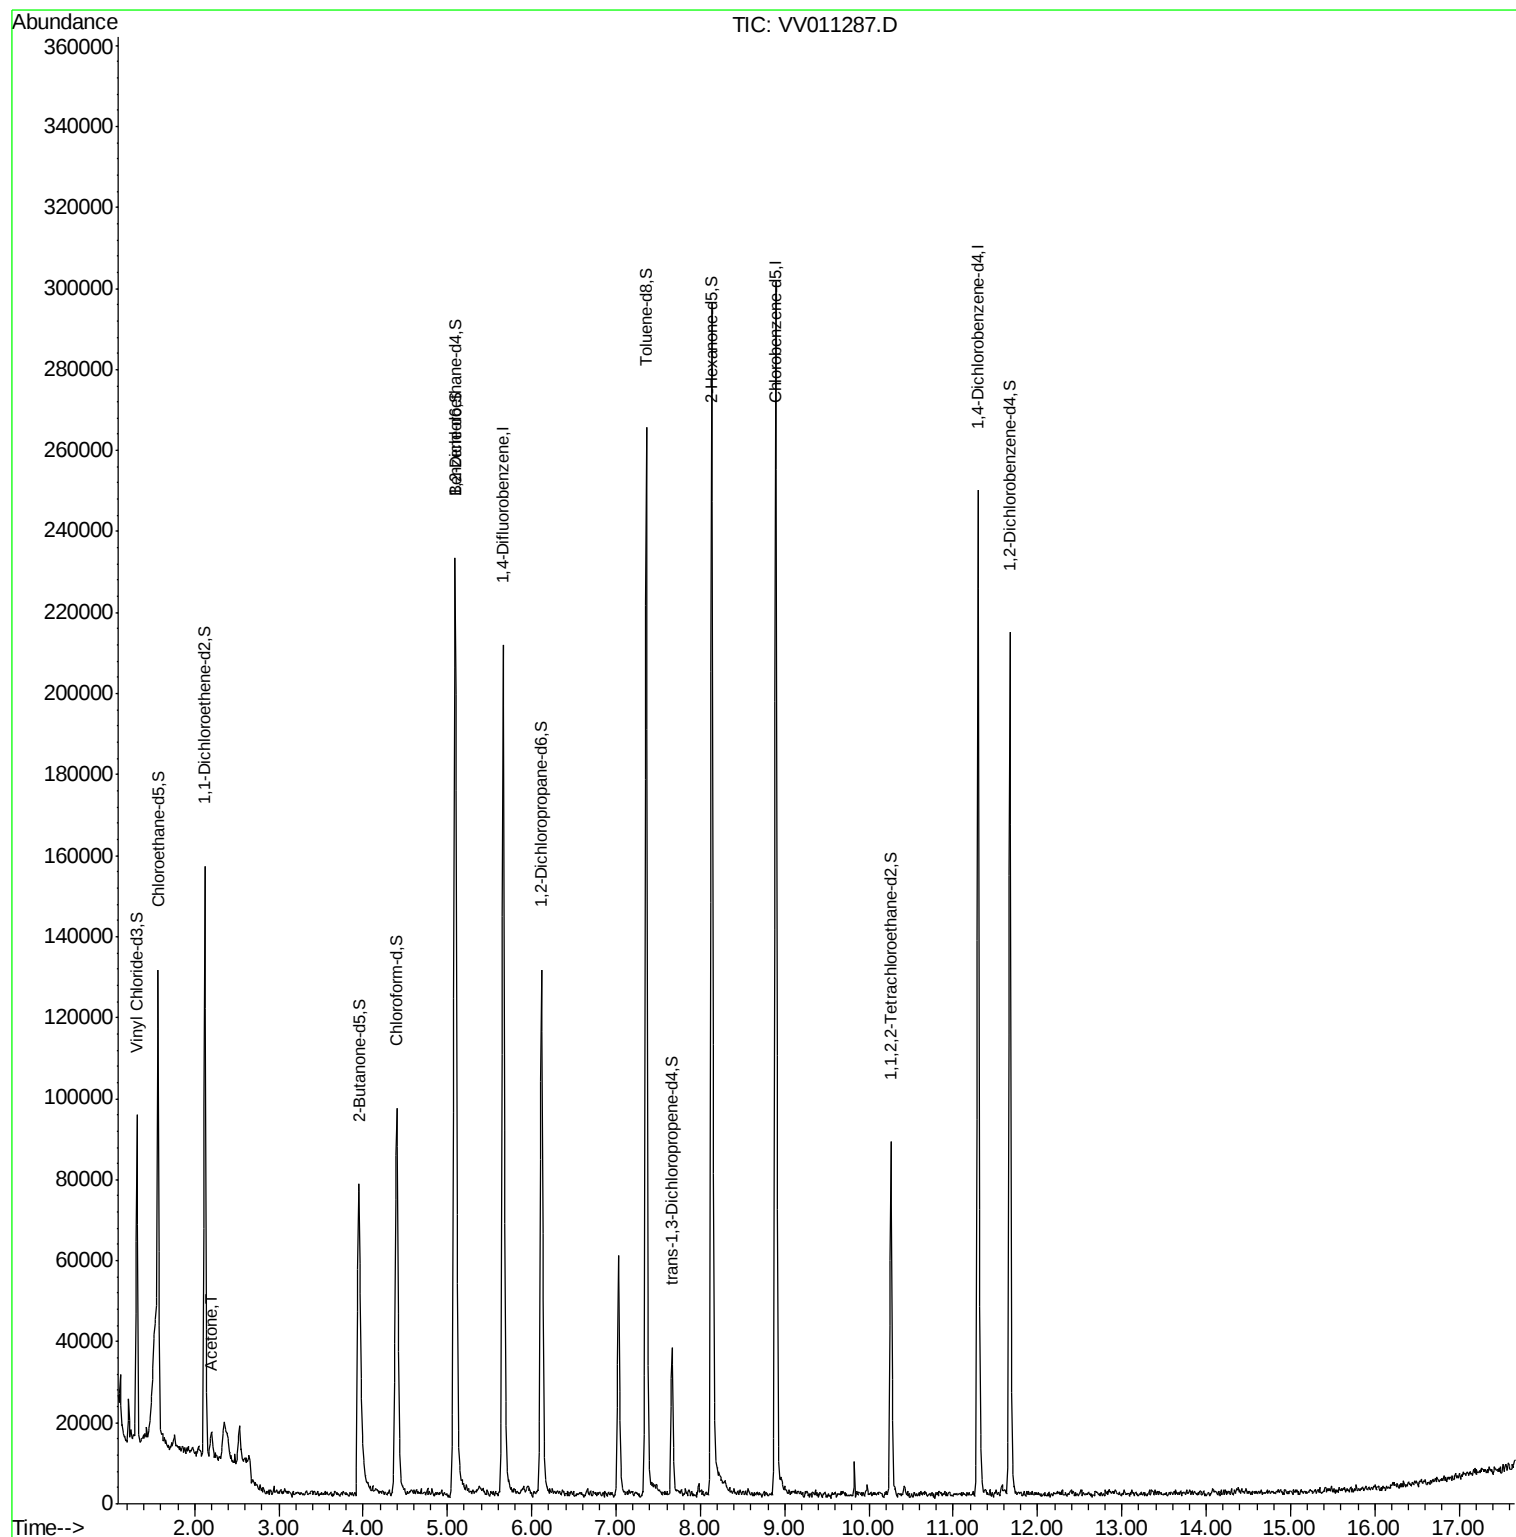

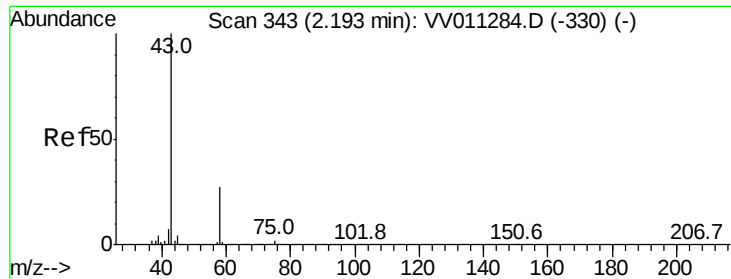

#13

Acetone

Concen: 2.212 ug/L

RT: 2.20 min Scan# 346

Delta R.T. 0.01 min

Lab File: VV011287.D

Acq: 07 Jun 2019 14:40

Instrument :

MSVOA_V

ClientSampleId :

VHBLK01

Tot Ion: 43 Resp: 4219

Ion Ratio Lower Upper

43 100

58 46.0 0.0 55.2

