

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011293.D
 Acq On : 07 Jun 2019 17:38
 Operator : SY/MD
 Sample : K3197-13
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P57

Quant Time: Jun 08 01:34:55 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 08 00:40:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	160461	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	148663	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	63618	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	45975	3.78	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.60%
7) Chloroethane-d5	1.58	69	38314	3.79	ug/L	0.03
Spiked Amount	5.000	Range	65 - 130	Recovery	=	75.80%
11) 1,1-Dichloroethene-d2	2.12	63	78138	3.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.40%
20) 2-Butanone-d5	3.98	46	123324	45.05	ug/L	0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.10%
24) Chloroform-d	4.40	84	92916	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.80%
26) 1,2-Dichloroethane-d4	5.08	65	51432	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.00%
32) Benzene-d6	5.09	84	190528	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.60%
36) 1,2-Dichloropropane-d6	6.12	67	58573	4.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.60%
41) Toluene-d8	7.36	98	166808	4.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.60%
43) trans-1,3-Dichloropropene-	7.66	79	17759	3.40	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.00%
46) 2-Hexanone-d5	8.14	63	101976	46.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.44%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	38829	4.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	58005	4.62	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.40%


Target Compounds					Ovalue
13) Acetone	2.23	43	30838	16.802	ug/L 58
14) Carbon disulfide	2.31	76	16728	0.545	ug/L 99
15) Methyl Acetate	2.48	43	12092	2.481	ug/L 99
48) 2-Hexanone	8.19	43	11433	2.186	ug/L # 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011293.D
Acq On : 07 Jun 2019 17:38
Operator : SY/MD
Sample : K3197-13
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P57

Quant Time: Jun 08 01:34:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 08 00:40:24 2019
Response via : Initial Calibration

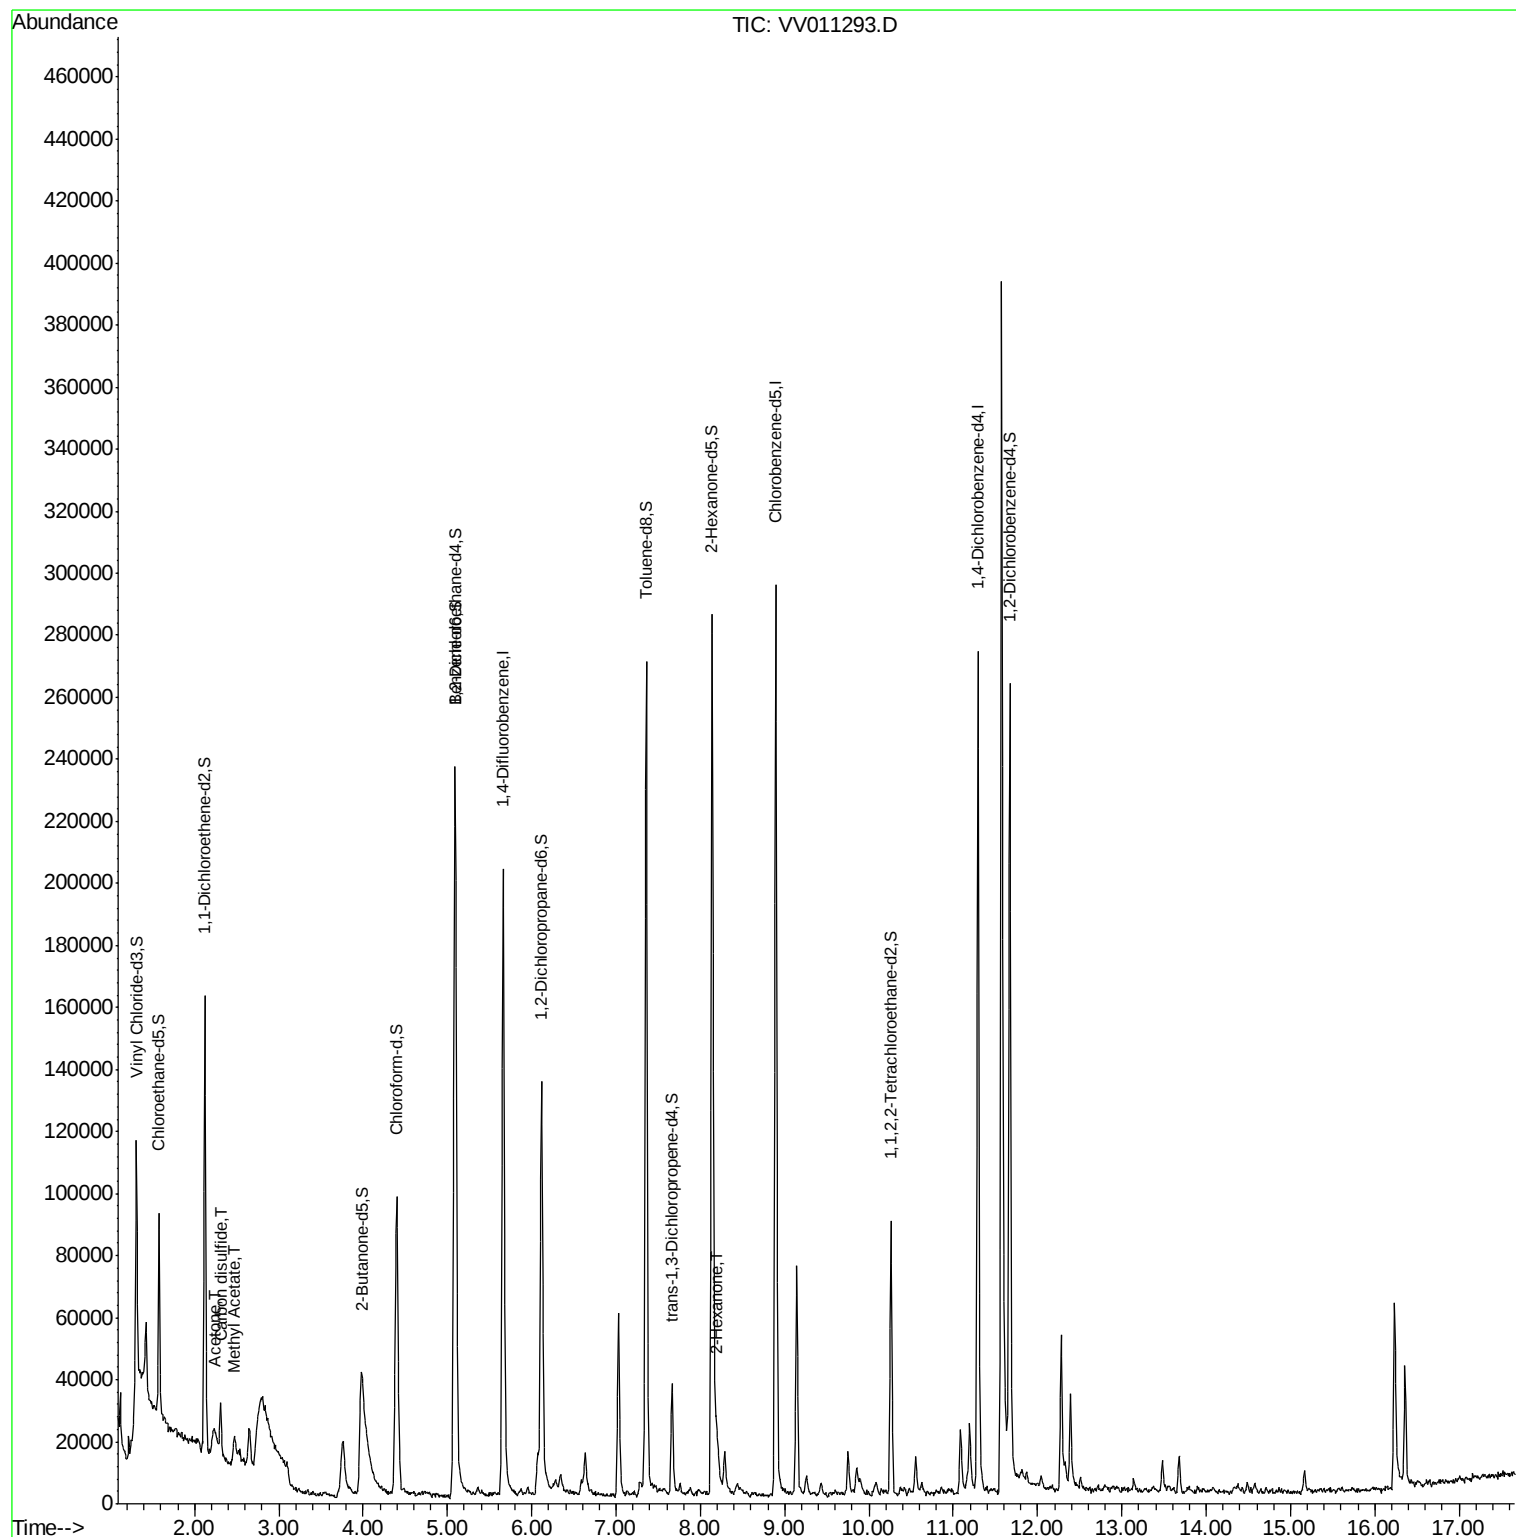

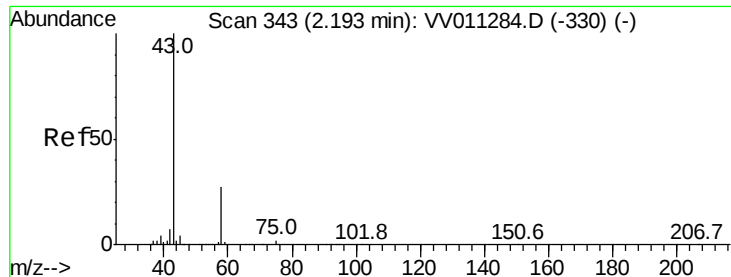

#13

Acetone

Concen: 16.802 ug/L

RT: 2.23 min Scan# 356

Delta R.T. 0.04 min

Lab File: VV011293.D

Acq: 07 Jun 2019 17:38

Instrument :

MSVOA_V

ClientSampleId :


F9P57

Tot Ion: 43 Resp: 30838

Ion Ratio Lower Upper




43 100

58 5.5 0.0 55.2

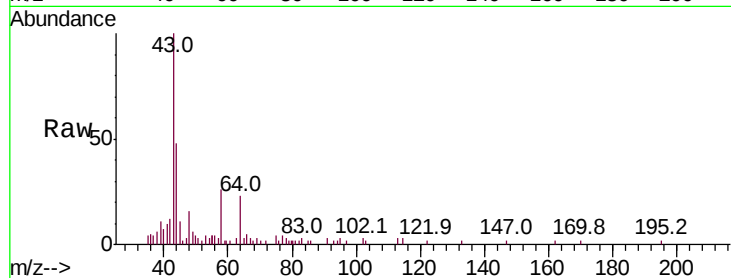

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

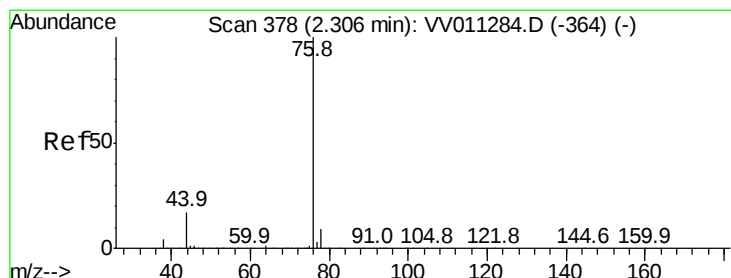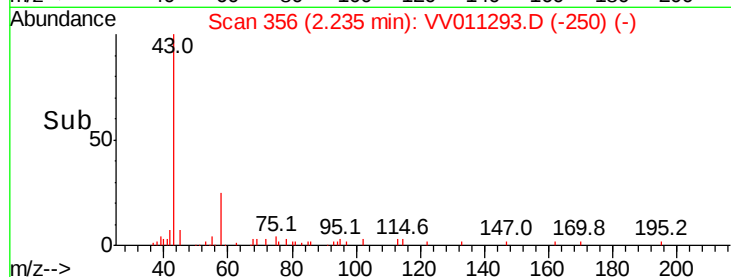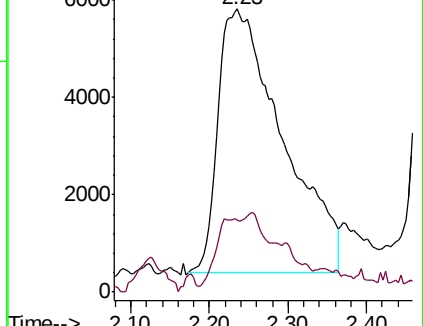

#14

Carbon disulfide

Concen: 0.545 ug/L

RT: 2.31 min Scan# 379

Delta R.T. 0.00 min

Lab File: VV011293.D


Acq: 07 Jun 2019 17:38

Tgt Ion: 76 Resp: 16728

Ion Ratio Lower Upper



76 100


78 8.8 7.3 10.9

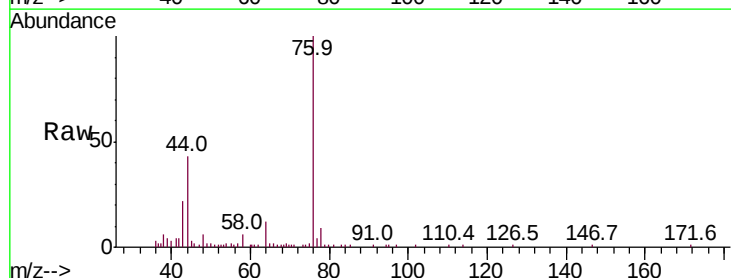

Abundance Ion 76.05 (75.75 to 76.75): VV0

Ion 78.00 (77.70 to 78.70): VV0



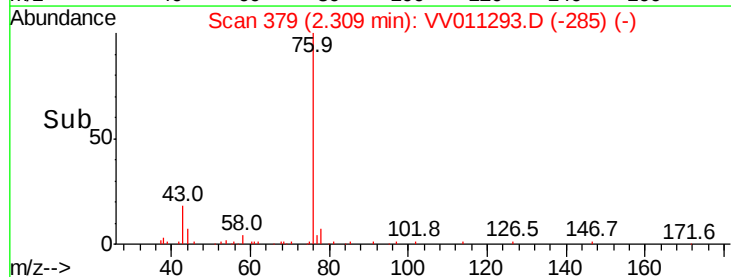
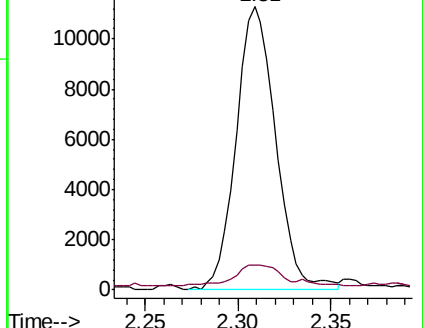


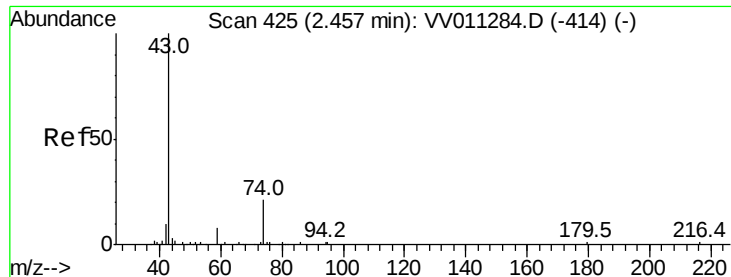

#15
Methvl Acetate
Concen: 2.481 ug/L
RT: 2.48 min Scan# 431
Delta R.T. 0.02 min
Lab File: VV011293.D
Acq: 07 Jun 2019 17:38

Instrument :
MSVOA_V
ClientSampleId :
F9P57

Tot Ion: 43 Resp: 12092
Ion Ratio Lower Upper
43 100
74 23.5 18.5 27.7

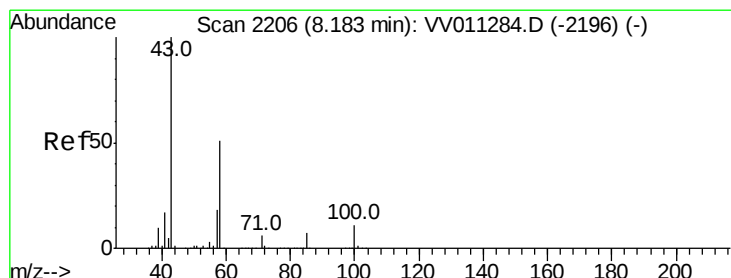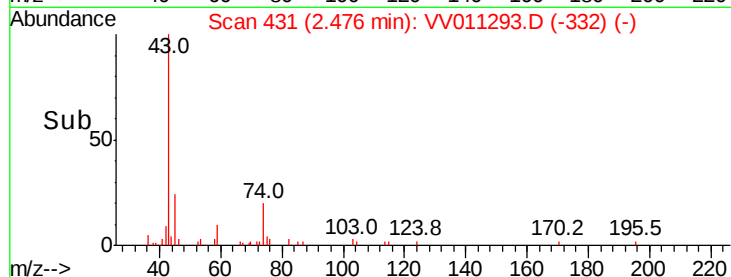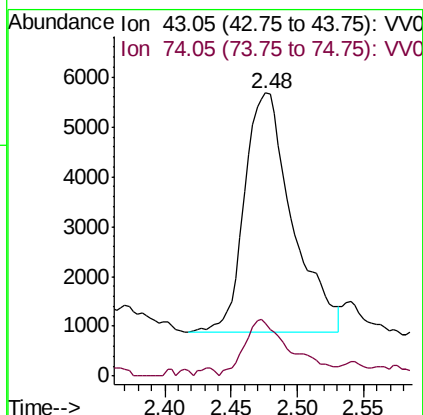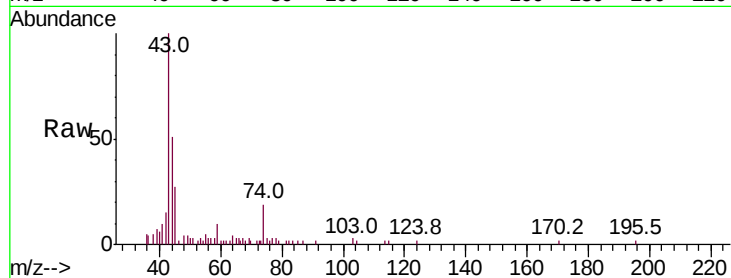

#48
2-Hexanone
Concen: 2.186 ug/L
RT: 8.19 min Scan# 2209
Delta R.T. 0.01 min
Lab File: VV011293.D
Acq: 07 Jun 2019 17:38

Tgt Ion: 43 Resp: 11433
Ion Ratio Lower Upper
43 100
58 45.2 41.4 62.0
57 7.0 15.0 22.4#
100 11.3 9.0 13.4

