

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011297.D
 Acq On : 07 Jun 2019 19:30
 Operator : SY/MD
 Sample : K3226-10
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCQ7

Quant Time: Jun 08 01:49:27 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 08 00:40:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	157220	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	145632	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	57091	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	47538	3.99	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.80%
7) Chloroethane-d5	1.56	69	41060	4.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.00%
11) 1,1-Dichloroethene-d2	2.12	63	76303	3.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.20%
20) 2-Butanone-d5	3.94	46	126811	47.28	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.56%
24) Chloroform-d	4.40	84	93837	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.60%
26) 1,2-Dichloroethane-d4	5.08	65	52548	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
32) Benzene-d6	5.09	84	188442	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.60%
36) 1,2-Dichloropropane-d6	6.12	67	58824	4.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.60%
41) Toluene-d8	7.36	98	165987	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.00%
43) trans-1,3-Dichloropropene-	7.66	79	17947	3.51	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.20%
46) 2-Hexanone-d5	8.13	63	105103	48.63	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.26%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	40623	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	52440	4.65	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.00%


Target Compounds					Ovalue
13) Acetone	2.19	43	4253	2.365 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011297.D
Acq On : 07 Jun 2019 19:30
Operator : SY/MD
Sample : K3226-10
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCQ7

Quant Time: Jun 08 01:49:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 08 00:40:24 2019
Response via : Initial Calibration

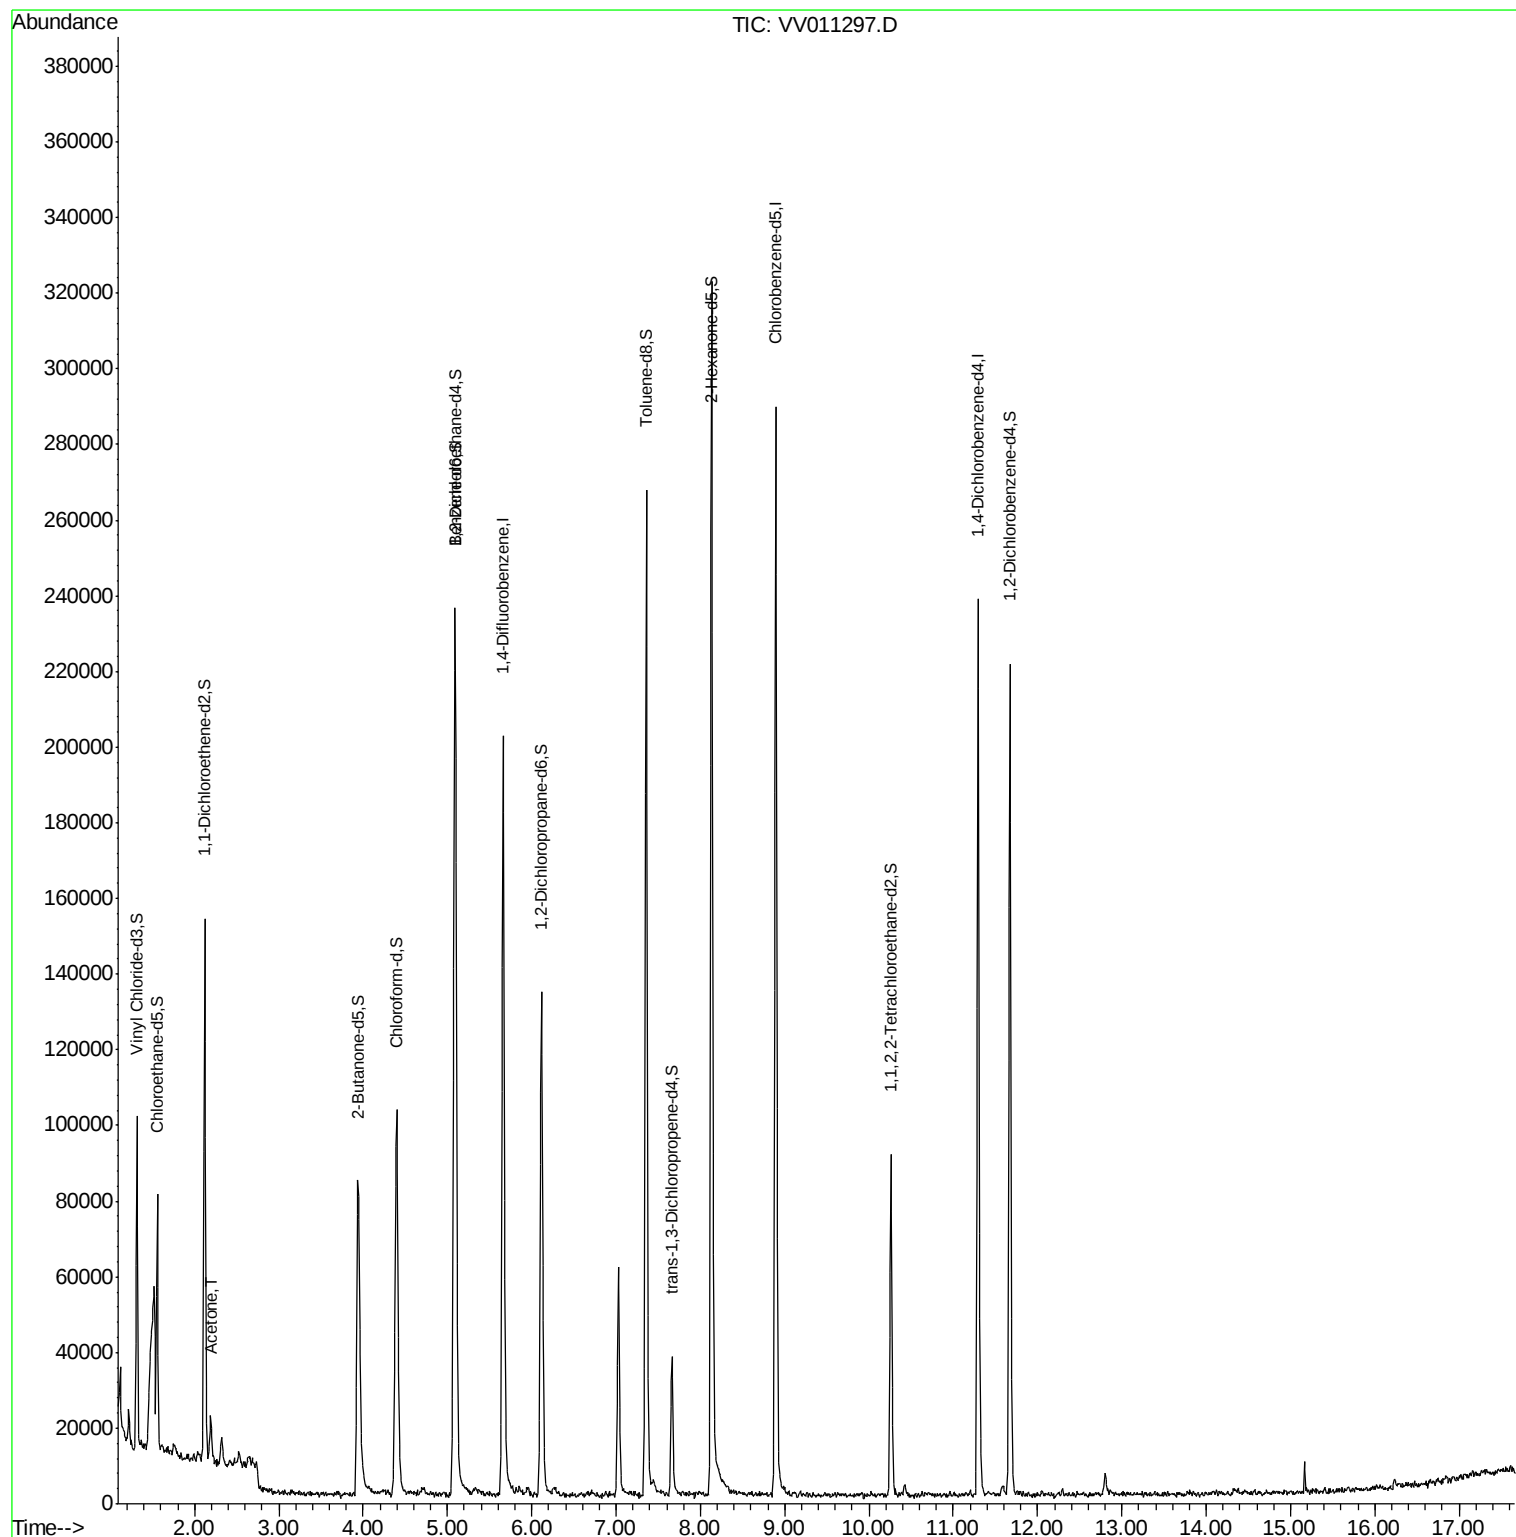

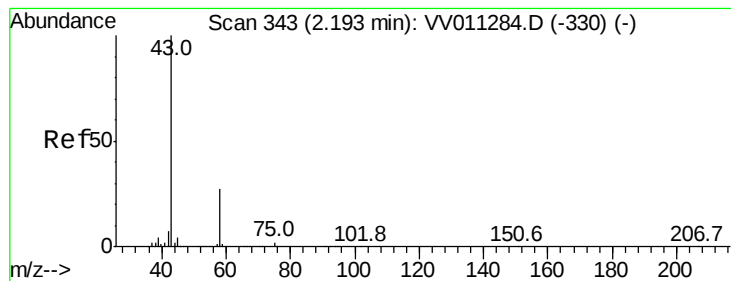

#13

Acetone

Concen: 2.365 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.00 min

Lab File: VV011297.D

Acq: 07 Jun 2019 19:30

Instrument :
MSVOA_V
ClientSampleId :
BFCQ7

Tot Ion: 43 Resp: 4253

Ion Ratio Lower Upper

43 100

58 30.6 0.0 55.2

