

Data File : VV011305.D
Acq On : 08 Jun 2019 00:38
Operator : SY/MD
Sample : K3226-11DL 4X
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCT6DL

Quant Time: Jun 11 03:41:09 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 08 02:09:28 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	164940	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	148478	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	57819	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	43882	3.51	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	70.20%
7) Chloroethane-d5	1.55	69	39968	3.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.00%
11) 1,1-Dichloroethene-d2	2.12	63	69344	2.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.60%#
20) 2-Butanone-d5	3.94	46	151909	53.99	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.98%
24) Chloroform-d	4.40	84	93136	4.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.80%
26) 1,2-Dichloroethane-d4	5.08	65	54717	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.00%
32) Benzene-d6	5.09	84	183095	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.40%
36) 1,2-Dichloropropane-d6	6.11	67	58869	4.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.00%
41) Toluene-d8	7.36	98	155292	3.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.20%
43) trans-1,3-Dichloropropene-	7.66	79	17303	3.32	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	66.40%
46) 2-Hexanone-d5	8.13	63	119156	54.08	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.16%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	45319	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	51935	4.55	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.00%


Target Compounds					Qvalue
22) cis-1,2-Dichloroethene	3.95	96	6868	0.533 ug/L	88
34) Trichloroethene	5.96	95	82653	6.772 ug/L	97
47) Tetrachloroethene	8.02	164	19134	2.169 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV011305.D
Acq On : 08 Jun 2019 00:38
Operator : SY/MD
Sample : K3226-11DL 4X
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCT6DL

Quant Time: Jun 11 03:41:09 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 08 02:09:28 2019
Response via : Initial Calibration

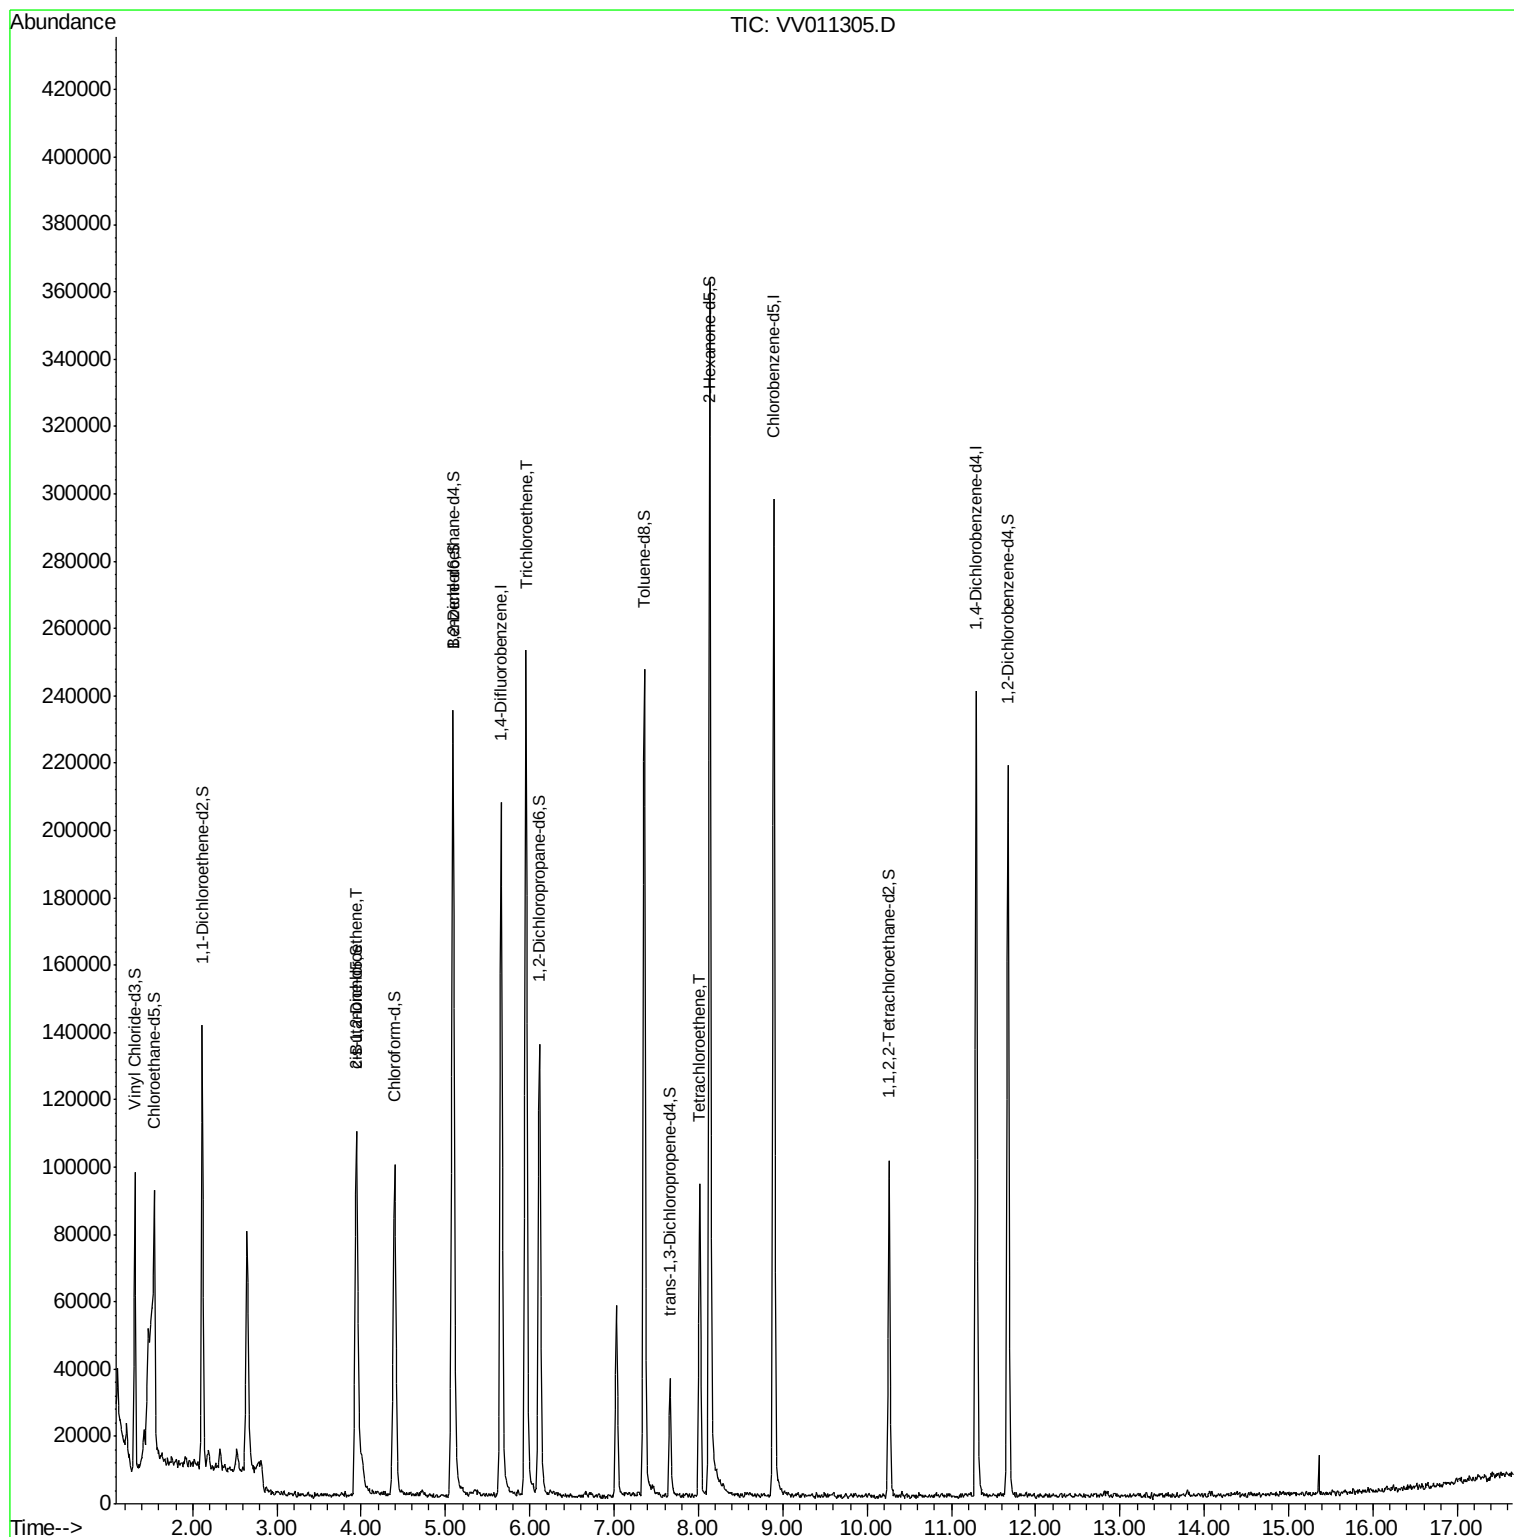




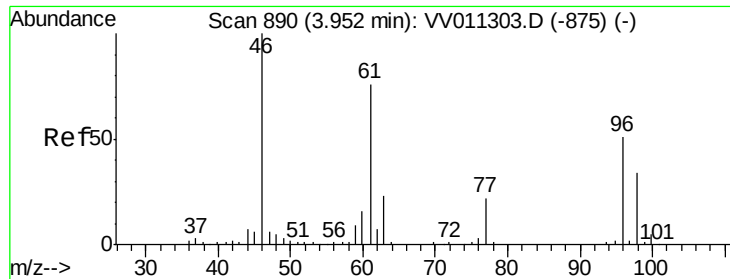


#22

cis-1,2-Dichloroethene
Concen: 0.533 ug/L
RT: 3.95 min Scan# 890
Delta R.T. 0.00 min
Lab File: VV011305.D
Acq: 08 Jun 2019 00:38

Instrument :
MSVOA_V
ClientSampleId :
BFCT6DL




Tgt Ion: 96 Resp: 6868
Ion Ratio Lower Upper
96 100
61 129.3 100.8 187.2
68 0.0 0.0 0.0

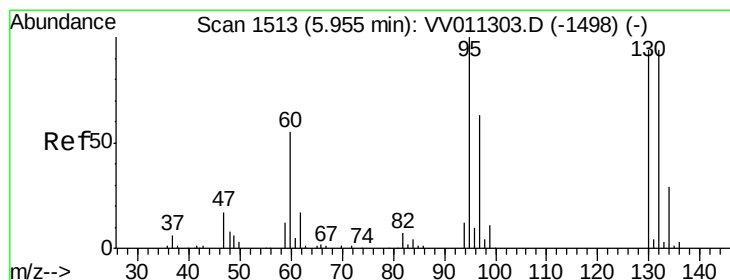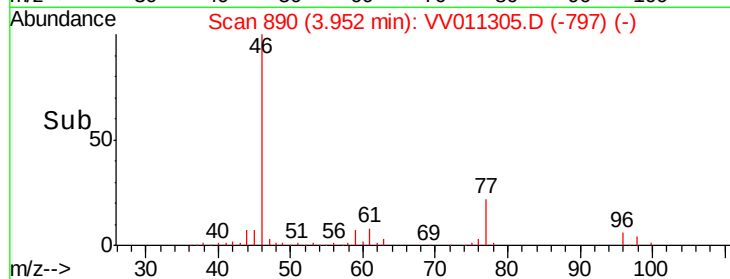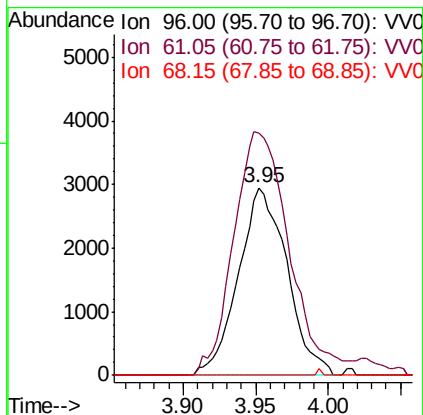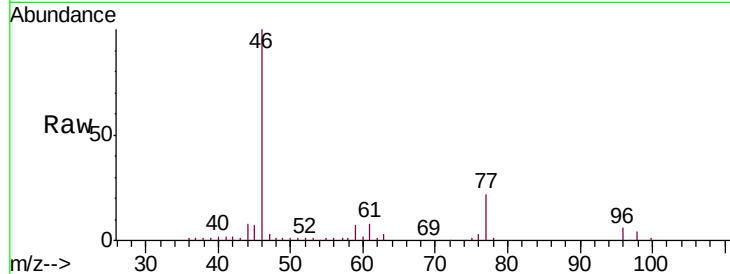


#34

Trichloroethene
Concen: 6.772 ug/L
RT: 5.96 min Scan# 1513
Delta R.T. 0.00 min
Lab File: VV011305.D
Acq: 08 Jun 2019 00:38

Tgt Ion: 95 Resp: 82653
Ion Ratio Lower Upper
95 100
97 67.0 45.8 85.2
132 96.6 66.4 123.2
130 102.8 68.3 126.8

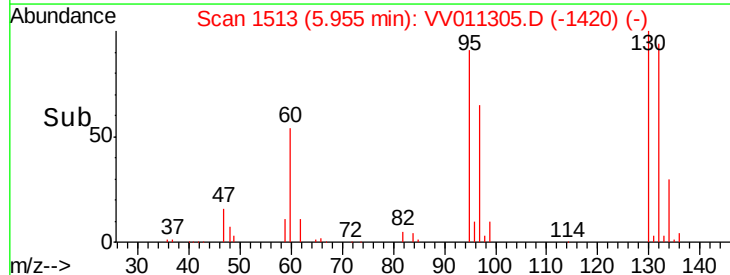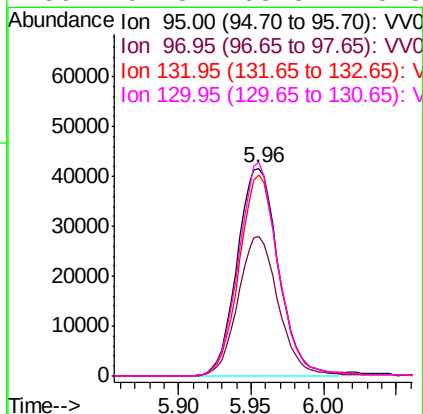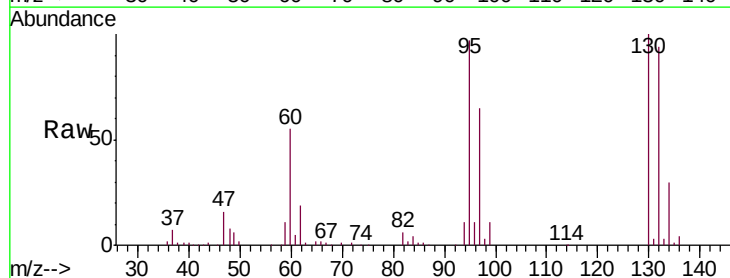

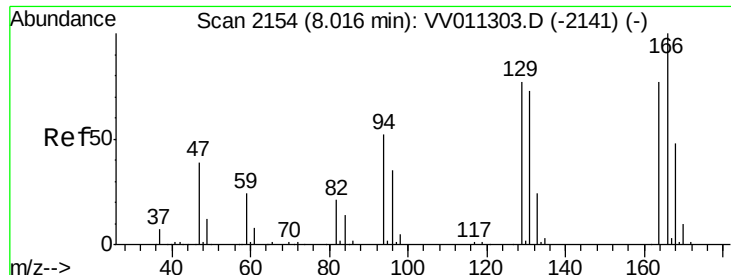

#47

Tetrachloroethene

Concen: 2.169 ug/L

RT: 8.02 min Scan# 2154

Delta R.T. 0.00 min

Lab File: VV011305.D


Acq: 08 Jun 2019 00:38

Instrument :

MSVOA_V

ClientSampleId :

BFCT6DL

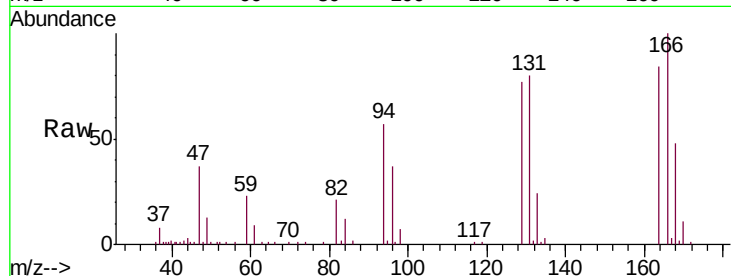

Tgt Ion:164 Resp: 19134

Ion Ratio Lower Upper

164 100

129 91.1 69.9 129.9

131 94.5 66.8 124.2

166 118.8 90.2 167.6

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

