

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011311.D
 Acq On : 08 Jun 2019 03:27
 Operator : SY/MD
 Sample : K3228-12
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P13

Quant Time: Jun 08 05:38:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 08 05:28:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	155490	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	147173	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	57763	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	42706	3.62	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.40%
7) Chloroethane-d5	1.55	69	37376	3.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.40%
11) 1,1-Dichloroethene-d2	2.12	63	69311	2.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.80%#
20) 2-Butanone-d5	3.94	46	143342	54.04	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.08%
24) Chloroform-d	4.40	84	90769	4.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.60%
26) 1,2-Dichloroethane-d4	5.08	65	52587	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
32) Benzene-d6	5.09	84	177181	4.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.40%
36) 1,2-Dichloropropane-d6	6.11	67	57056	4.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.20%
41) Toluene-d8	7.36	98	153400	3.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.80%
43) trans-1,3-Dichloropropene-	7.66	79	16347	3.16	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	63.20%
46) 2-Hexanone-d5	8.13	63	111246	50.94	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.88%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	42411	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	52177	4.58	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.60%


Target Compounds					Ovalue
13) Acetone	2.19	43	8700	4.892 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011311.D
Acq On : 08 Jun 2019 03:27
Operator : SY/MD
Sample : K3228-12
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P13

Quant Time: Jun 08 05:38:52 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 08 05:28:44 2019
Response via : Initial Calibration

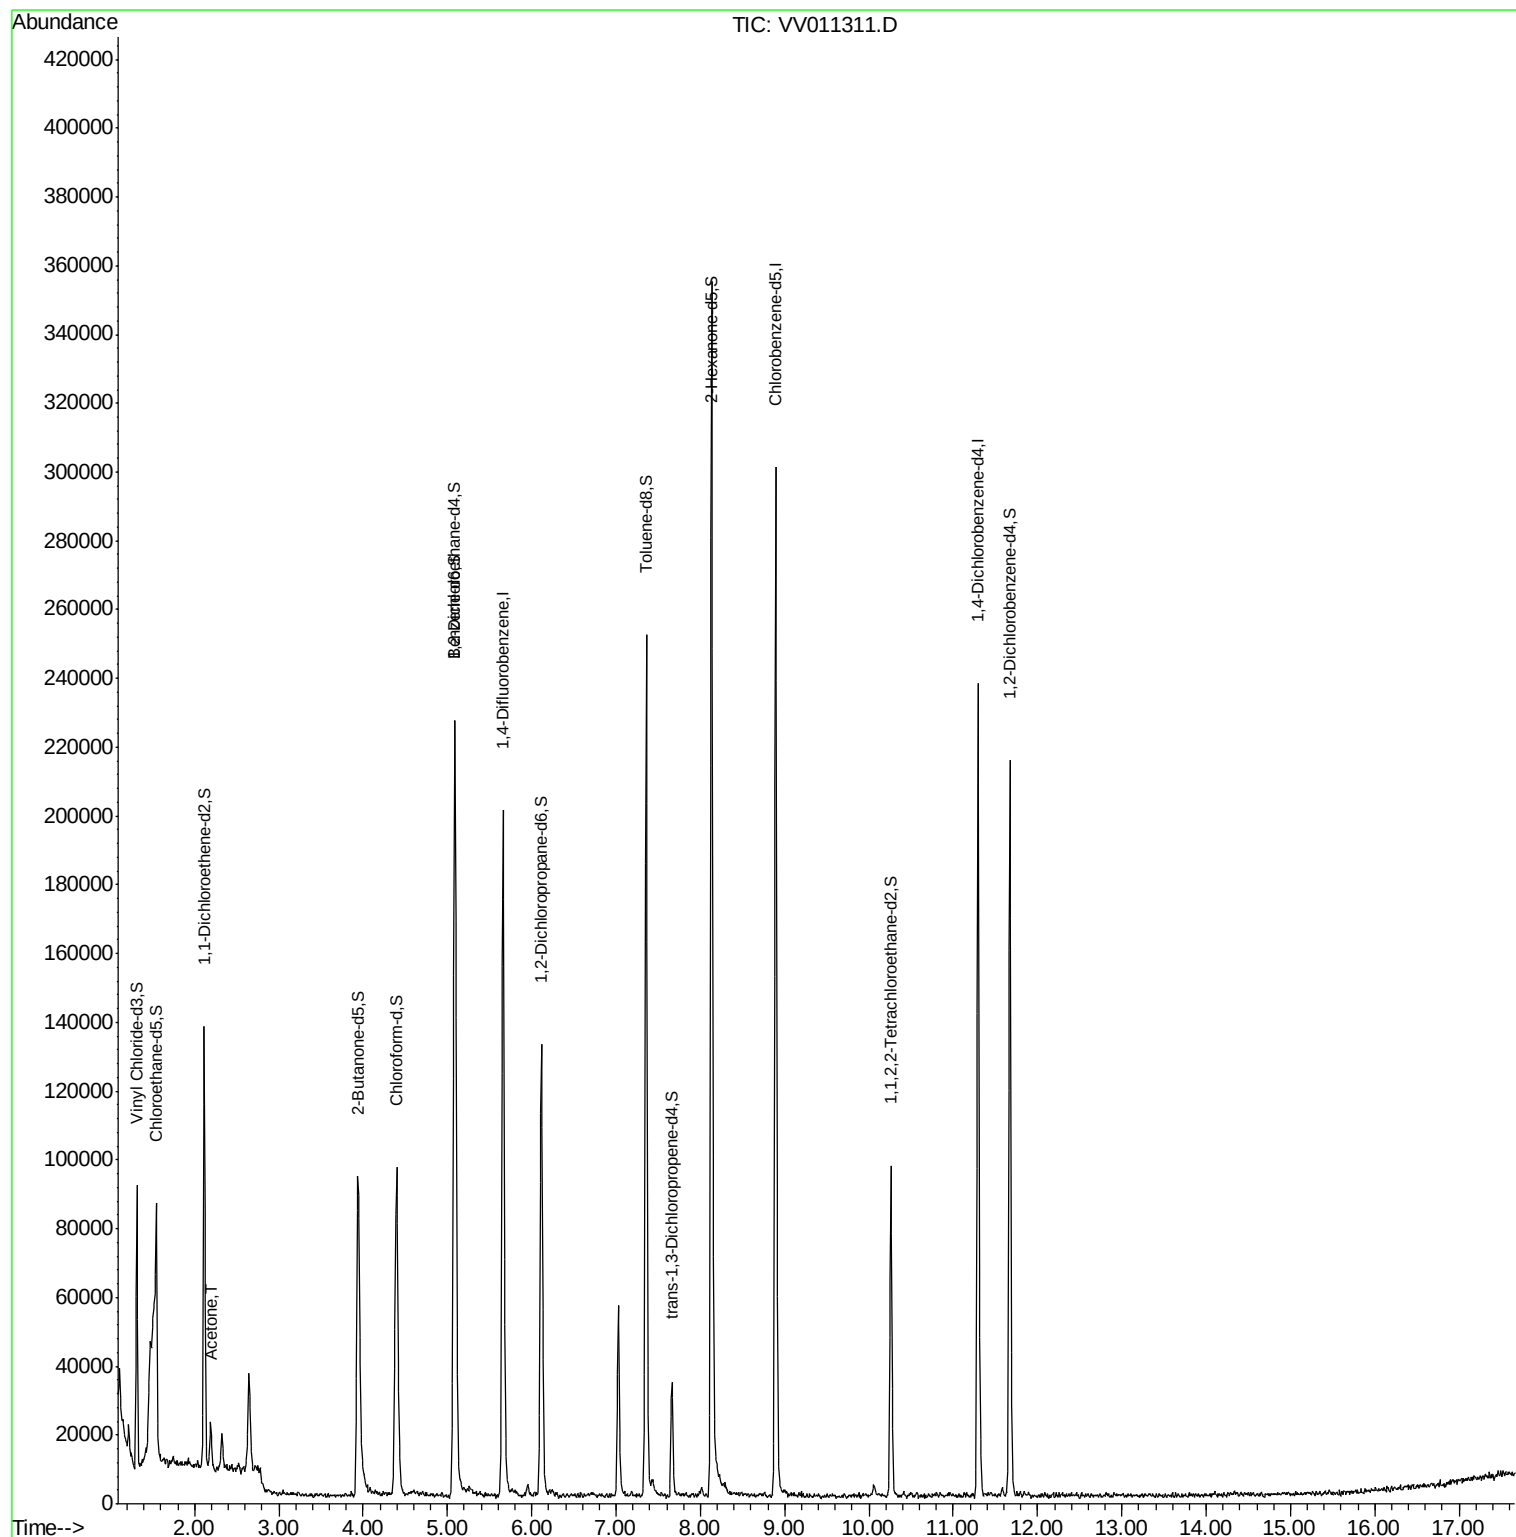

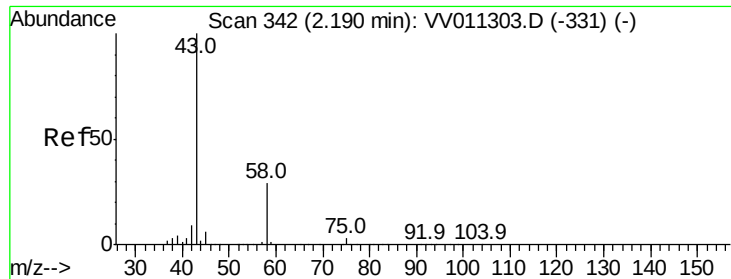

#13

Acetone

Concen: 4.892 ug/L

RT: 2.19 min Scan# 343

Delta R.T. 0.00 min

Lab File: VV011311.D

Acq: 08 Jun 2019 03:27

Instrument :
MSVOA_V
ClientSampleId :
F9P13

Tot Ion: 43 Resp: 8700

Ion Ratio Lower Upper

43 100

58 32.8 0.0 55.2

