

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011312.D
 Acq On : 08 Jun 2019 03:55
 Operator : SY/MD
 Sample : K3228-13
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P14

Quant Time: Jun 08 05:41:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 08 05:28:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	155755	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	147660	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	58760	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	42332	3.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.80%
7) Chloroethane-d5	1.55	69	38821	3.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.20%
11) 1,1-Dichloroethene-d2	2.12	63	69900	2.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.20%#
20) 2-Butanone-d5	3.94	46	146293	55.06	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.12%
24) Chloroform-d	4.40	84	90040	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.80%
26) 1,2-Dichloroethane-d4	5.08	65	52731	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.00%
32) Benzene-d6	5.09	84	178330	4.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.80%
36) 1,2-Dichloropropane-d6	6.11	67	56741	4.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.40%
41) Toluene-d8	7.36	98	154874	3.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.40%
43) trans-1,3-Dichloropropene-	7.66	79	16806	3.24	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	64.80%
46) 2-Hexanone-d5	8.13	63	115191	52.57	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.14%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	42985	4.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	53744	4.63	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.60%


Target Compounds					Ovalue
13) Acetone	2.19	43	6842	3.841 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011312.D
Acq On : 08 Jun 2019 03:55
Operator : SY/MD
Sample : K3228-13
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P14

Quant Time: Jun 08 05:41:10 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 08 05:28:44 2019
Response via : Initial Calibration

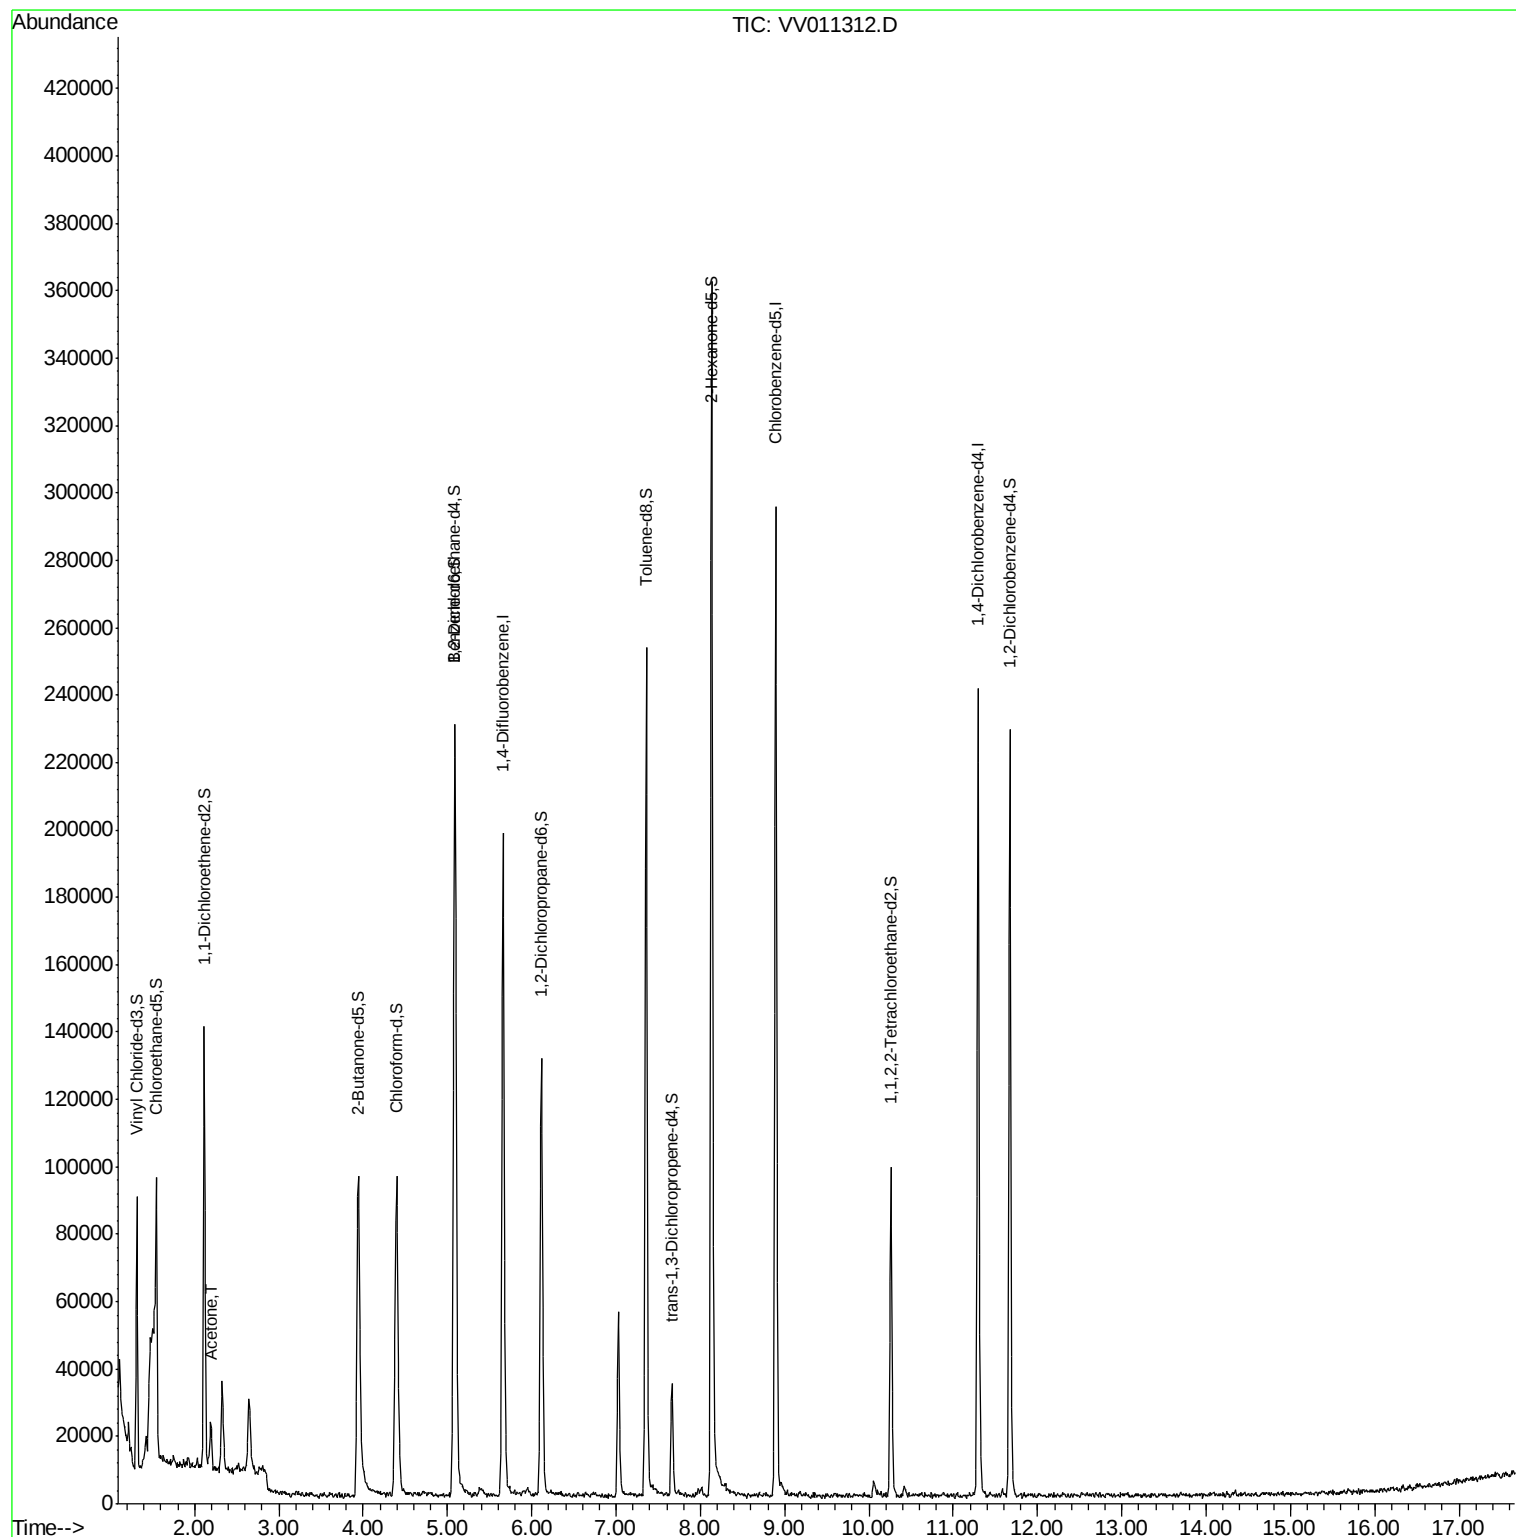

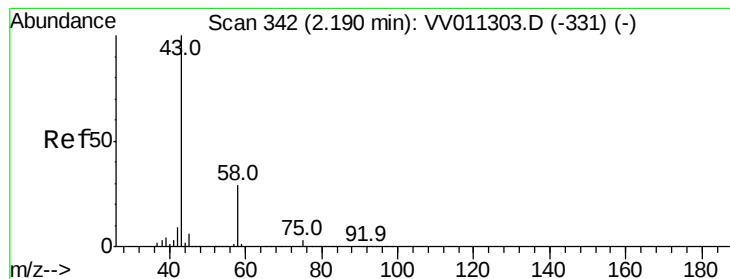

#13

Acetone

Concen: 3.841 ug/L

RT: 2.19 min Scan# 343

Delta R.T. 0.00 min

Lab File: VV011312.D

Acq: 08 Jun 2019 03:55

Instrument :
MSVOA_V
ClientSampleId :
F9P14

Tot Ion: 43 Resp: 6842

Ion Ratio Lower Upper

43 100

58 31.6 0.0 55.2

