

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011313.D
 Acq On : 08 Jun 2019 04:23
 Operator : SY/MD
 Sample : K3228-14
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P16

Quant Time: Jun 08 05:43:41 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 08 05:28:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	156598	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	144865	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	56617	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	41015	3.46	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	69.20%
7) Chloroethane-d5	1.55	69	36757	3.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	74.60%
11) 1,1-Dichloroethene-d2	2.12	63	68172	2.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.60%#
20) 2-Butanone-d5	3.94	46	139852	52.35	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.70%
24) Chloroform-d	4.40	84	87834	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.20%
26) 1,2-Dichloroethane-d4	5.08	65	49756	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.20%
32) Benzene-d6	5.09	84	171698	3.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.20%
36) 1,2-Dichloropropane-d6	6.12	67	53650	4.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.40%
41) Toluene-d8	7.36	98	149483	3.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.20%
43) trans-1,3-Dichloropropene-	7.66	79	15556	3.06	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	61.20%
46) 2-Hexanone-d5	8.13	63	105421	49.04	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.08%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	41157	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	49829	4.46	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.20%


Target Compounds					Ovalue
13) Acetone	2.19	43	8498	4.744 ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011313.D
Acq On : 08 Jun 2019 04:23
Operator : SY/MD
Sample : K3228-14
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P16

Quant Time: Jun 08 05:43:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 08 05:28:44 2019
Response via : Initial Calibration

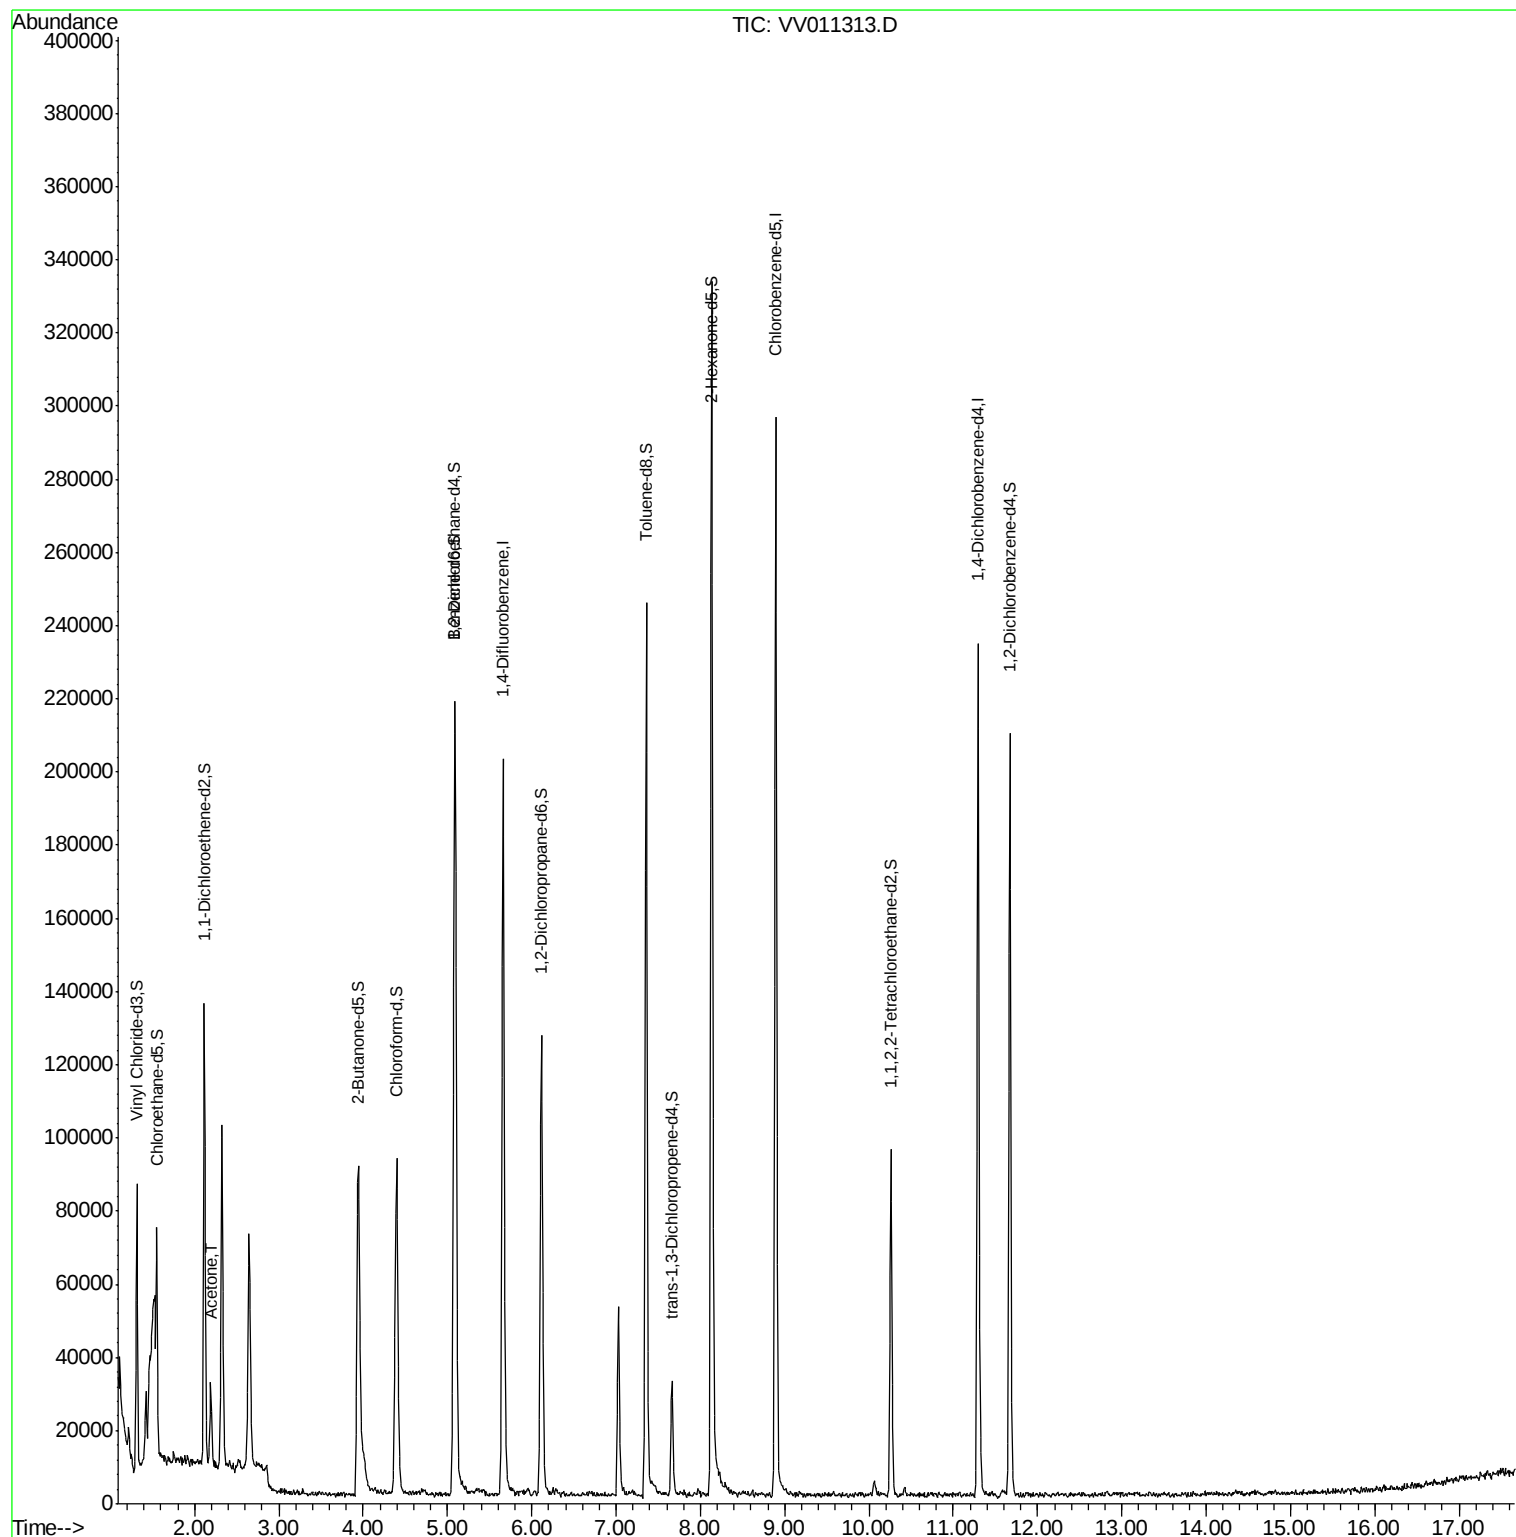

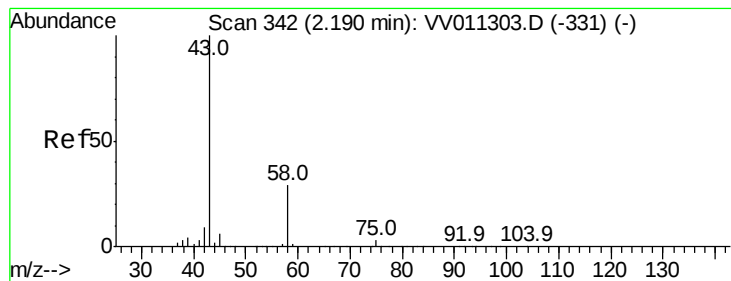

#13

Acetone

Concen: 4.744 ug/L

RT: 2.19 min Scan# 343

Delta R.T. 0.00 min

Lab File: VV011313.D

Acq: 08 Jun 2019 04:23

Instrument :
MSVOA_V
ClientSampleId :
F9P16

Tot Ion: 43 Resp: 8498

Ion Ratio Lower Upper

43 100

58 36.0 0.0 55.2

