

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011277.D
 Acq On : 07 Jun 2019 07:20
 Operator : SY/MD
 Sample : K3228-01
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P00

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.116	4	8	19	rVB	14546	15773	2.40%	0.300%
2	1.315	61	70	77	rBV	107798	111729	17.03%	2.128%
3	1.560	140	146	155	rVB	71717	80527	12.28%	1.534%
4	2.122	312	321	331	rVB	158377	220723	33.65%	4.204%
5	2.193	336	343	353	rVB2	22975	34873	5.32%	0.664%
6	2.318	375	382	394	rVB	12285	22061	3.36%	0.420%
7	2.646	476	484	498	rVB	19387	43038	6.56%	0.820%
8	3.936	874	885	915	rBV	100832	267648	40.81%	5.098%
9	4.396	1010	1028	1047	rBV2	105190	260702	39.75%	4.965%
10	5.090	1227	1244	1267	rBV2	258510	621475	94.75%	11.837%
11	5.659	1404	1421	1443	rBV	199137	402376	61.35%	7.664%
12	5.955	1501	1513	1528	rVB	6533	14763	2.25%	0.281%
13	6.116	1547	1563	1582	rBV	145758	300833	45.87%	5.730%
14	7.029	1835	1847	1863	rBV2	65081	117459	17.91%	2.237%
15	7.357	1938	1949	1964	rBV	295176	502725	76.65%	9.575%
16	7.662	2033	2044	2061	rBV	40488	69419	10.58%	1.322%
17	8.132	2179	2190	2210	rBV	386967	655902	100.00%	12.492%
18	8.894	2414	2427	2444	rBV	294993	478743	72.99%	9.118%
19	10.260	2838	2852	2869	rBV	106865	174701	26.64%	3.327%
20	11.292	3159	3173	3197	rBV	247594	422511	64.42%	8.047%
21	11.672	3278	3291	3306	rBV	256518	421658	64.29%	8.031%
22	16.762	4865	4874	4882	rBV8	6667	10855	1.65%	0.207%


Sum of corrected areas: 5250494

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011277.D
Acq On : 07 Jun 2019 07:20
Operator : SY/MD
Sample : K3228-01
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P00

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

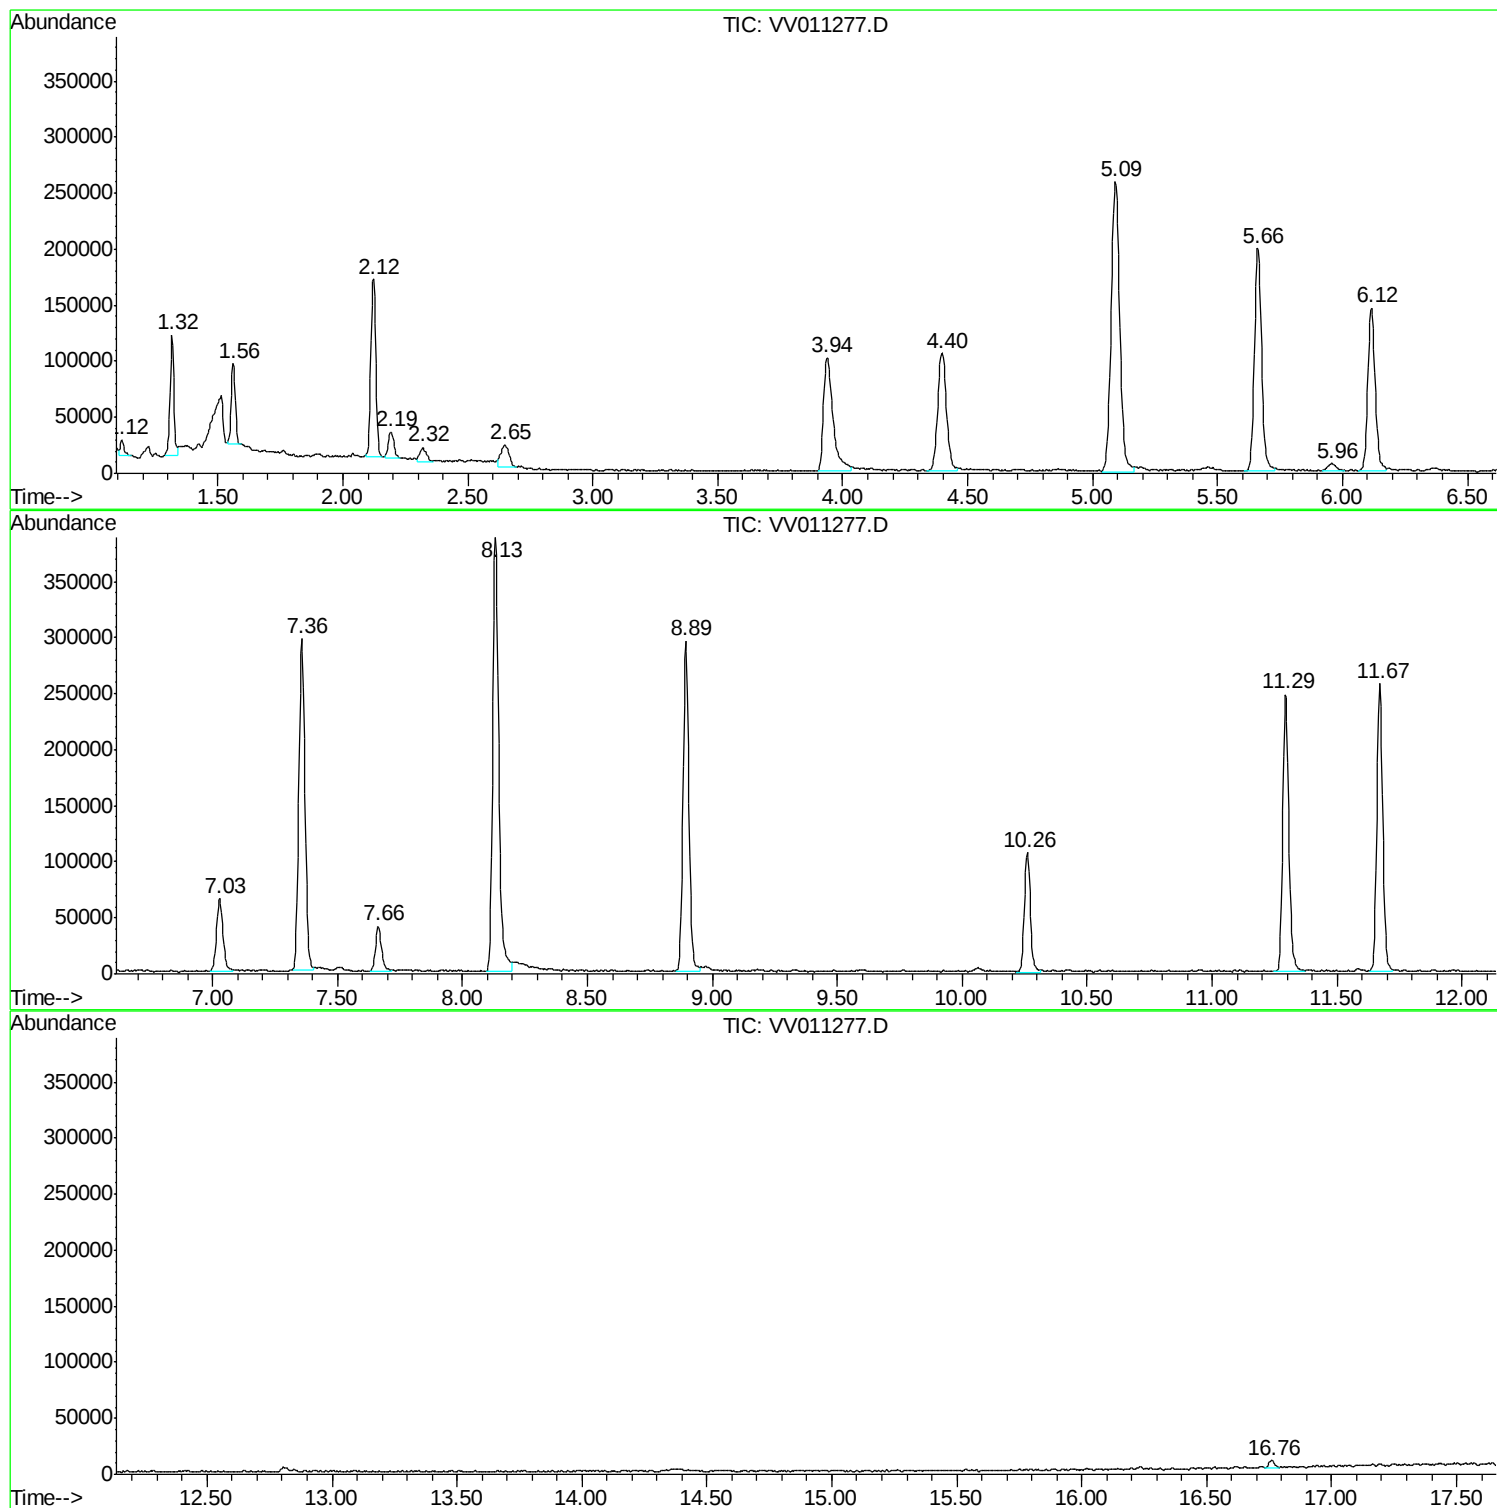

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011277.D
Acq On : 07 Jun 2019 07:20
Operator : SY/MD
Sample : K3228-01
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P00










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 10-Oxatetracyclo[5.5.2.0(1,... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.65	0.53 ug/L	43038	1,4-Difluorobenzene	5.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	10-Oxatetracyclo[5.5.2.0(1,5).0(...	352	C18H24O7	1000154-01-5	83
2		2-Cyclopentene, 1,4-bis(methoxyve...	276	C13H24O6	1000156-00-3	74
3		Silane, methoxyvtrimethyl-	104	C4H12OSi	001825-61-2	74
4		Tricyclo[5.2.2.0(2,6)]undecan-11...	352	C18H24O7	1000155-17-7	74
5		Silane, methoxytrimethyl-	104	C4H12OSi	001825-61-2	74

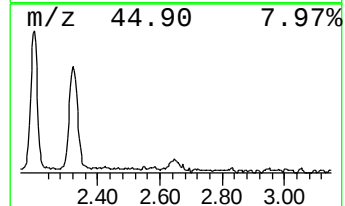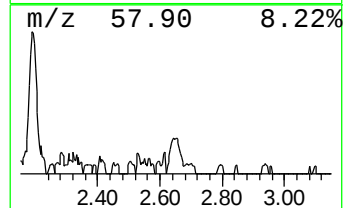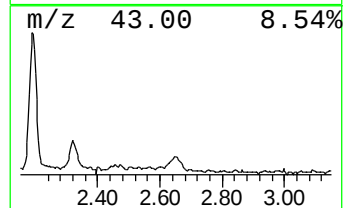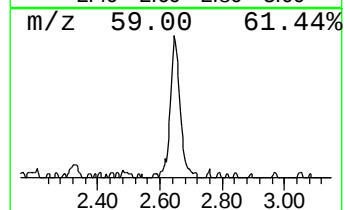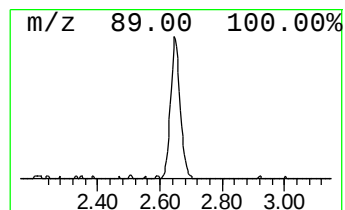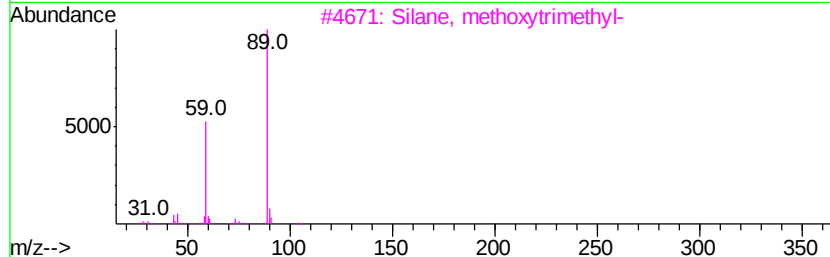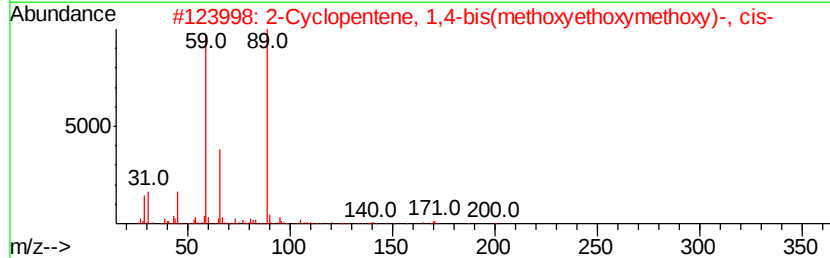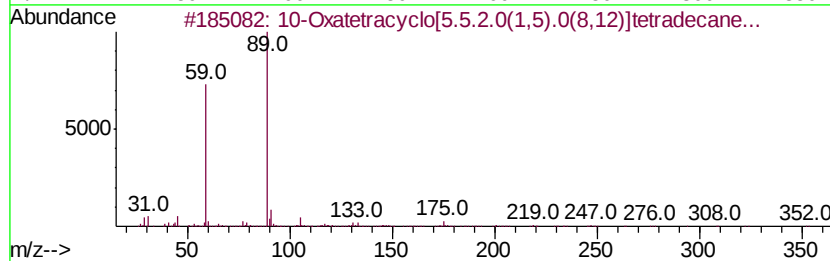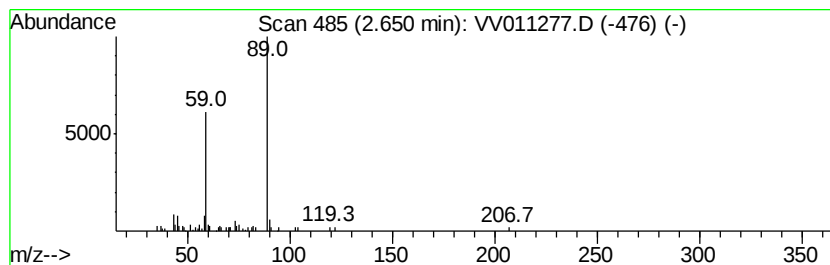

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060619\
Data File : VV011277.D
Acq On : 07 Jun 2019 07:20
Operator : SY/MD
Sample : K3228-01
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P00

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
10-Oxatetracyclo[...	2.65	0.5	ug/L	43038	1	5.66	402376	5.0