

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011311.D
 Acq On : 08 Jun 2019 03:27
 Operator : SY/MD
 Sample : K3228-12
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P13

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.219	36	40	47	rVB2	9512	10518	1.71%	0.218%
2	1.315	62	70	77	rBV	81385	76546	12.45%	1.587%
3	1.479	107	121	123	rBV10	32546	61910	10.07%	1.284%
4	1.544	137	141	150	rVB	73011	98914	16.09%	2.051%
5	2.116	310	319	330	rVB	127723	178318	29.01%	3.698%
6	2.190	337	342	350	rVB2	12820	17254	2.81%	0.358%
7	2.325	377	384	394	rVB	10029	15632	2.54%	0.324%
8	2.647	475	484	499	rVB2	28058	59937	9.75%	1.243%
9	3.939	873	886	917	rBV	92925	247793	40.31%	5.138%
10	4.396	1011	1028	1052	rBV	95202	242198	39.40%	5.022%
11	5.087	1223	1243	1263	rBV2	226105	540701	87.96%	11.212%
12	5.659	1407	1421	1446	rBV	199191	400391	65.13%	8.302%
13	6.113	1549	1562	1583	rBV2	130534	261812	42.59%	5.429%
14	7.026	1834	1846	1864	rBV	55683	101471	16.51%	2.104%
15	7.357	1933	1949	1964	rBV	250427	433069	70.45%	8.980%
16	7.662	2034	2044	2056	rBV2	33117	56611	9.21%	1.174%
17	8.132	2180	2190	2218	rBV	353227	614745	100.00%	12.747%
18	8.894	2413	2427	2452	rBV	299598	494045	80.37%	10.244%
19	10.260	2841	2852	2866	rBV	95595	152066	24.74%	3.153%
20	11.293	3161	3173	3193	rBV	236845	400764	65.19%	8.310%
21	11.672	3279	3291	3311	rVB	213968	357883	58.22%	7.421%


Sum of corrected areas: 4822578

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011311.D
Acq On : 08 Jun 2019 03:27
Operator : SY/MD
Sample : K3228-12
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P13

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

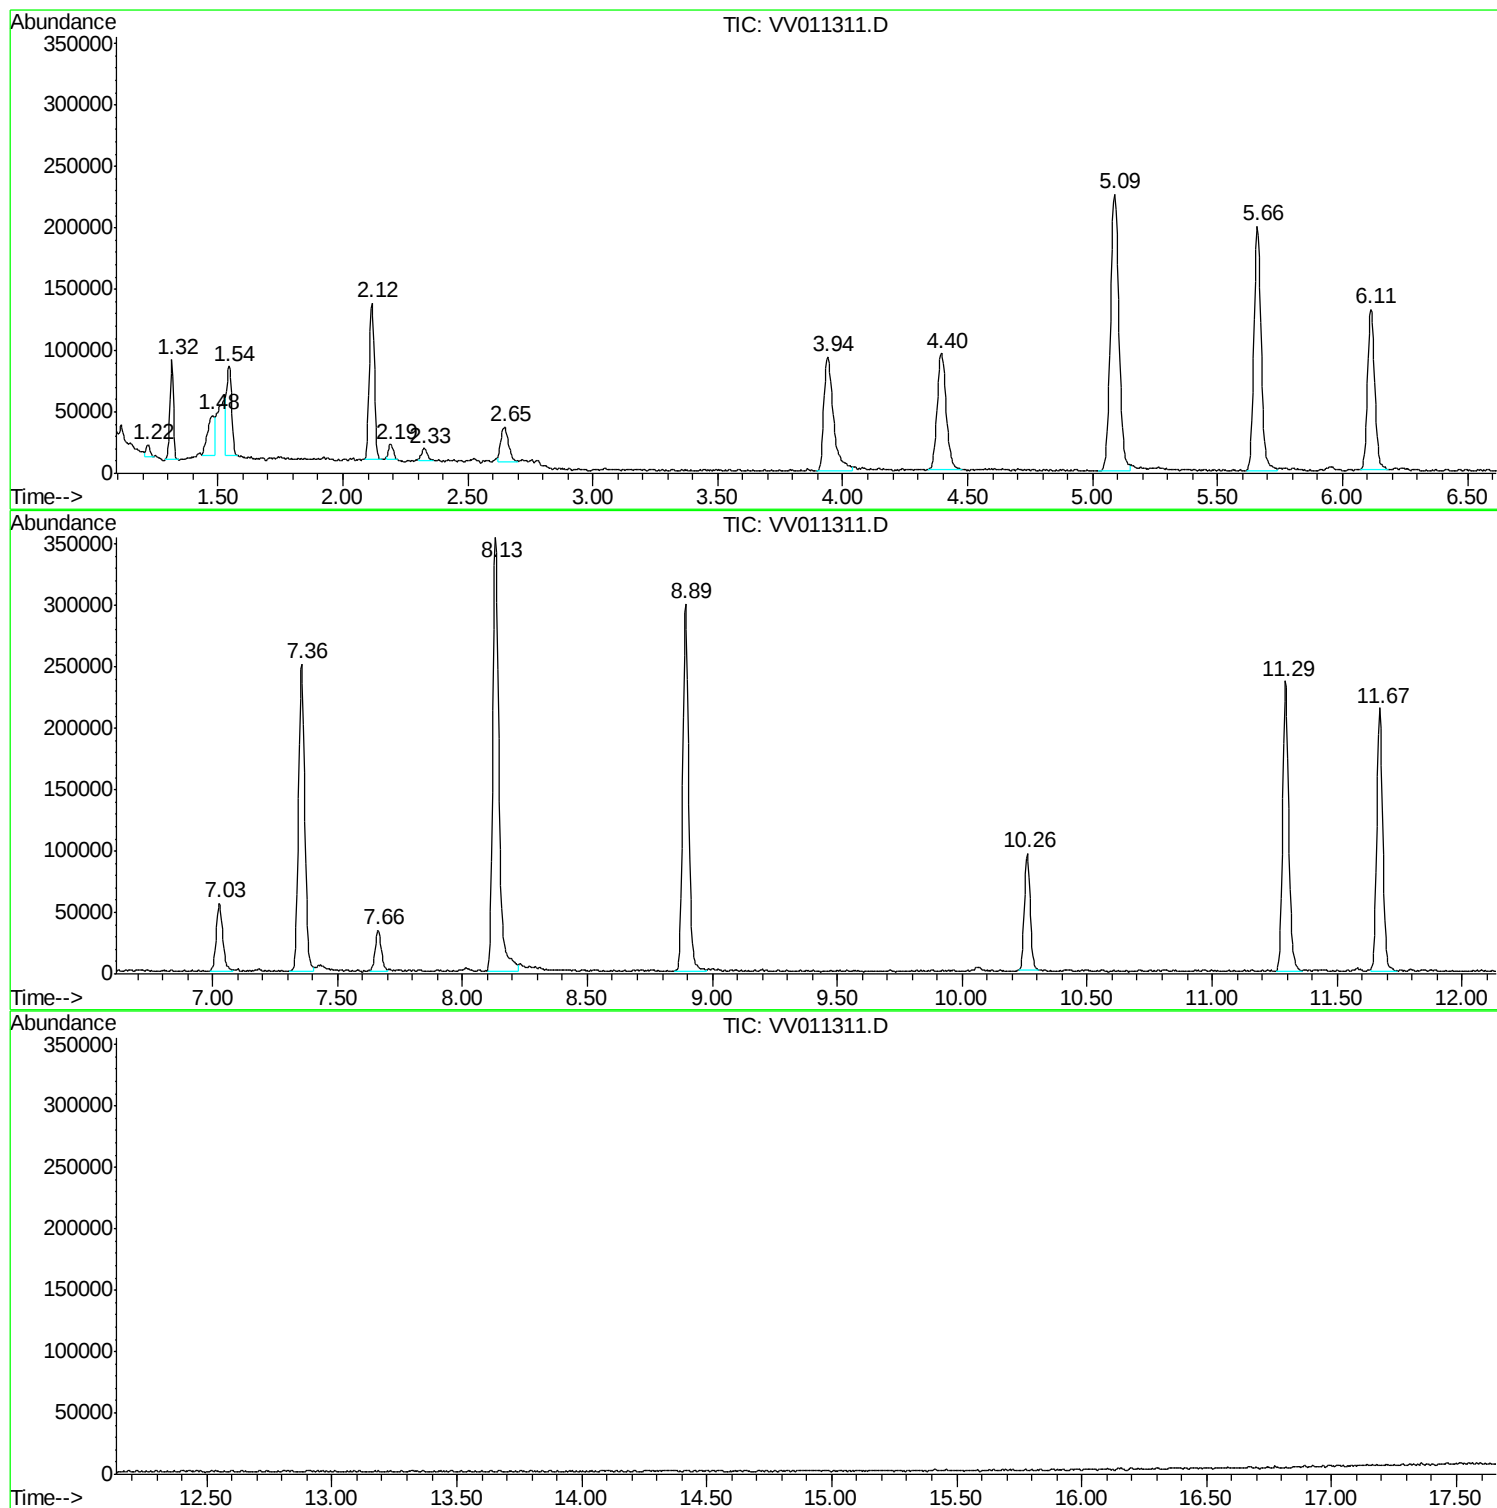

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011311.D
Acq On : 08 Jun 2019 03:27
Operator : SY/MD
Sample : K3228-12
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P13










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.48	0.77 ug/L	61910	1,4-Difluorobenzene	5.66

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Carbonochloridic acid, chloromet...	128	C2H2Cl2O2	022128-62-7	28
2			Methylene chloride	84	CH2Cl2	000075-09-2	25
3			Methvlene chloride	84	CH2Cl2	000075-09-2	14
4			2-[2-(2-Chloro-ethoxy)-ethoxy]-p...	216	C10H13ClO3	1000317-46-1	14
5			4,5-Dichloro-1,3-dioxolan-2-one	156	C3H2Cl2O3	003967-55-3	12

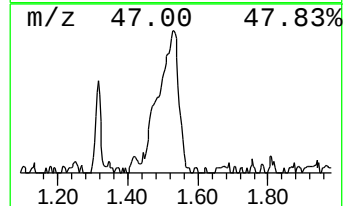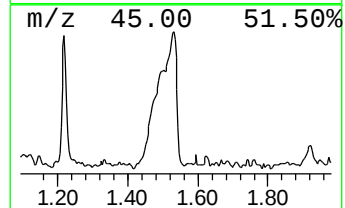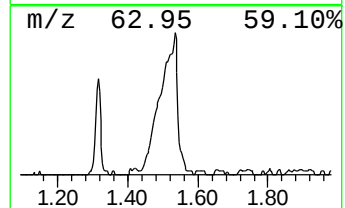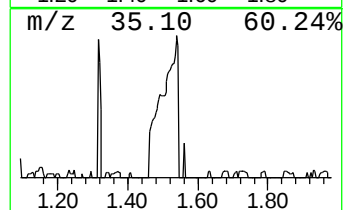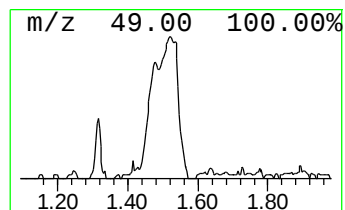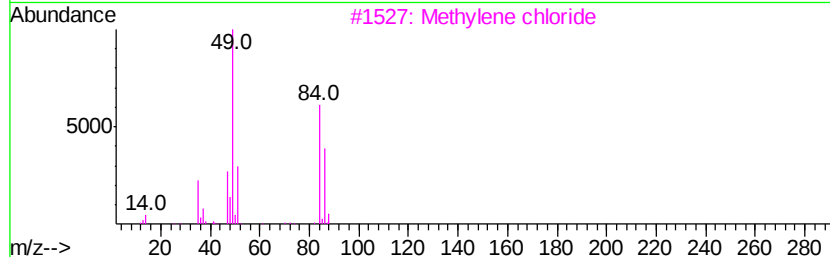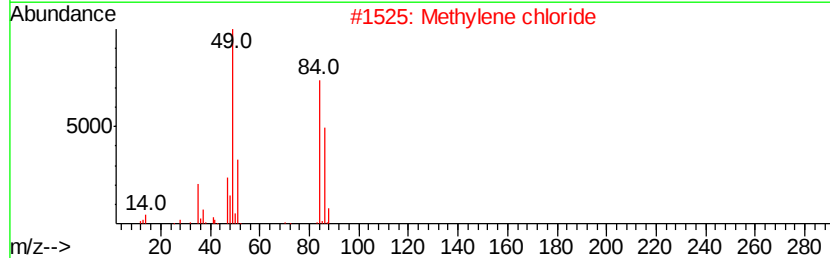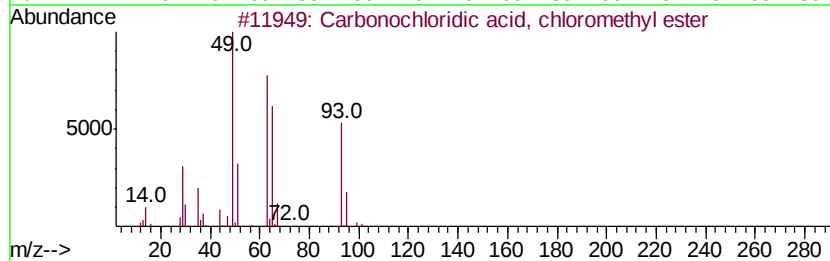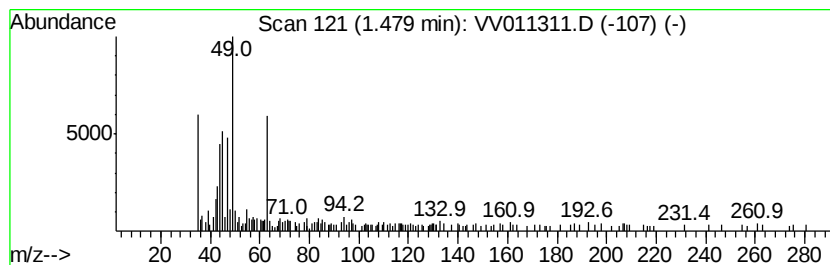

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060619\
Data File : VV011311.D
Acq On : 08 Jun 2019 03:27
Operator : SY/MD
Sample : K3228-12
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P13

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.48	0.8	ug/L	61910	1	5.66	400391	5.0