

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
 Data File : VV011312.D
 Acq On : 08 Jun 2019 03:55
 Operator : SY/MD
 Sample : K3228-13
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P14

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	61	70	77	rBV	80578	78814	12.55%	1.615%
2	1.476	108	120	122	rBV9	33909	51695	8.23%	1.059%
3	1.547	137	142	153	rVB	83385	112715	17.95%	2.309%
4	2.116	310	319	330	rVB	130014	178326	28.40%	3.654%
5	2.193	336	343	352	rVB	14267	22397	3.57%	0.459%
6	2.328	374	385	397	rBV	27445	51390	8.19%	1.053%
7	2.646	475	484	501	rVB2	21081	47523	7.57%	0.974%
8	3.942	871	887	910	rBV	95143	246142	39.20%	5.043%
9	4.396	1010	1028	1049	rBV	95208	245270	39.06%	5.025%
10	5.087	1225	1243	1263	rBV3	229233	539861	85.98%	11.061%
11	5.659	1406	1421	1438	rBV	196683	392218	62.47%	8.036%
12	6.113	1547	1562	1583	rBV	129425	265695	42.32%	5.444%
13	7.026	1835	1846	1860	rBV	54887	101707	16.20%	2.084%
14	7.357	1936	1949	1965	rBV	251725	439491	70.00%	9.005%
15	7.662	2035	2044	2061	rBV	33135	57080	9.09%	1.169%
16	8.132	2176	2190	2221	rBV	360421	627855	100.00%	12.864%
17	8.894	2412	2427	2441	rBV	293871	482089	76.78%	9.877%
18	10.058	2780	2789	2800	rBV	4726	9274	1.48%	0.190%
19	10.260	2836	2852	2865	rBV	98138	160178	25.51%	3.282%
20	11.292	3159	3173	3189	rBV	239599	400578	63.80%	8.207%
21	11.672	3277	3291	3305	rBV	227668	370436	59.00%	7.590%


Sum of corrected areas: 4880734

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011312.D
Acq On : 08 Jun 2019 03:55
Operator : SY/MD
Sample : K3228-13
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P14

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

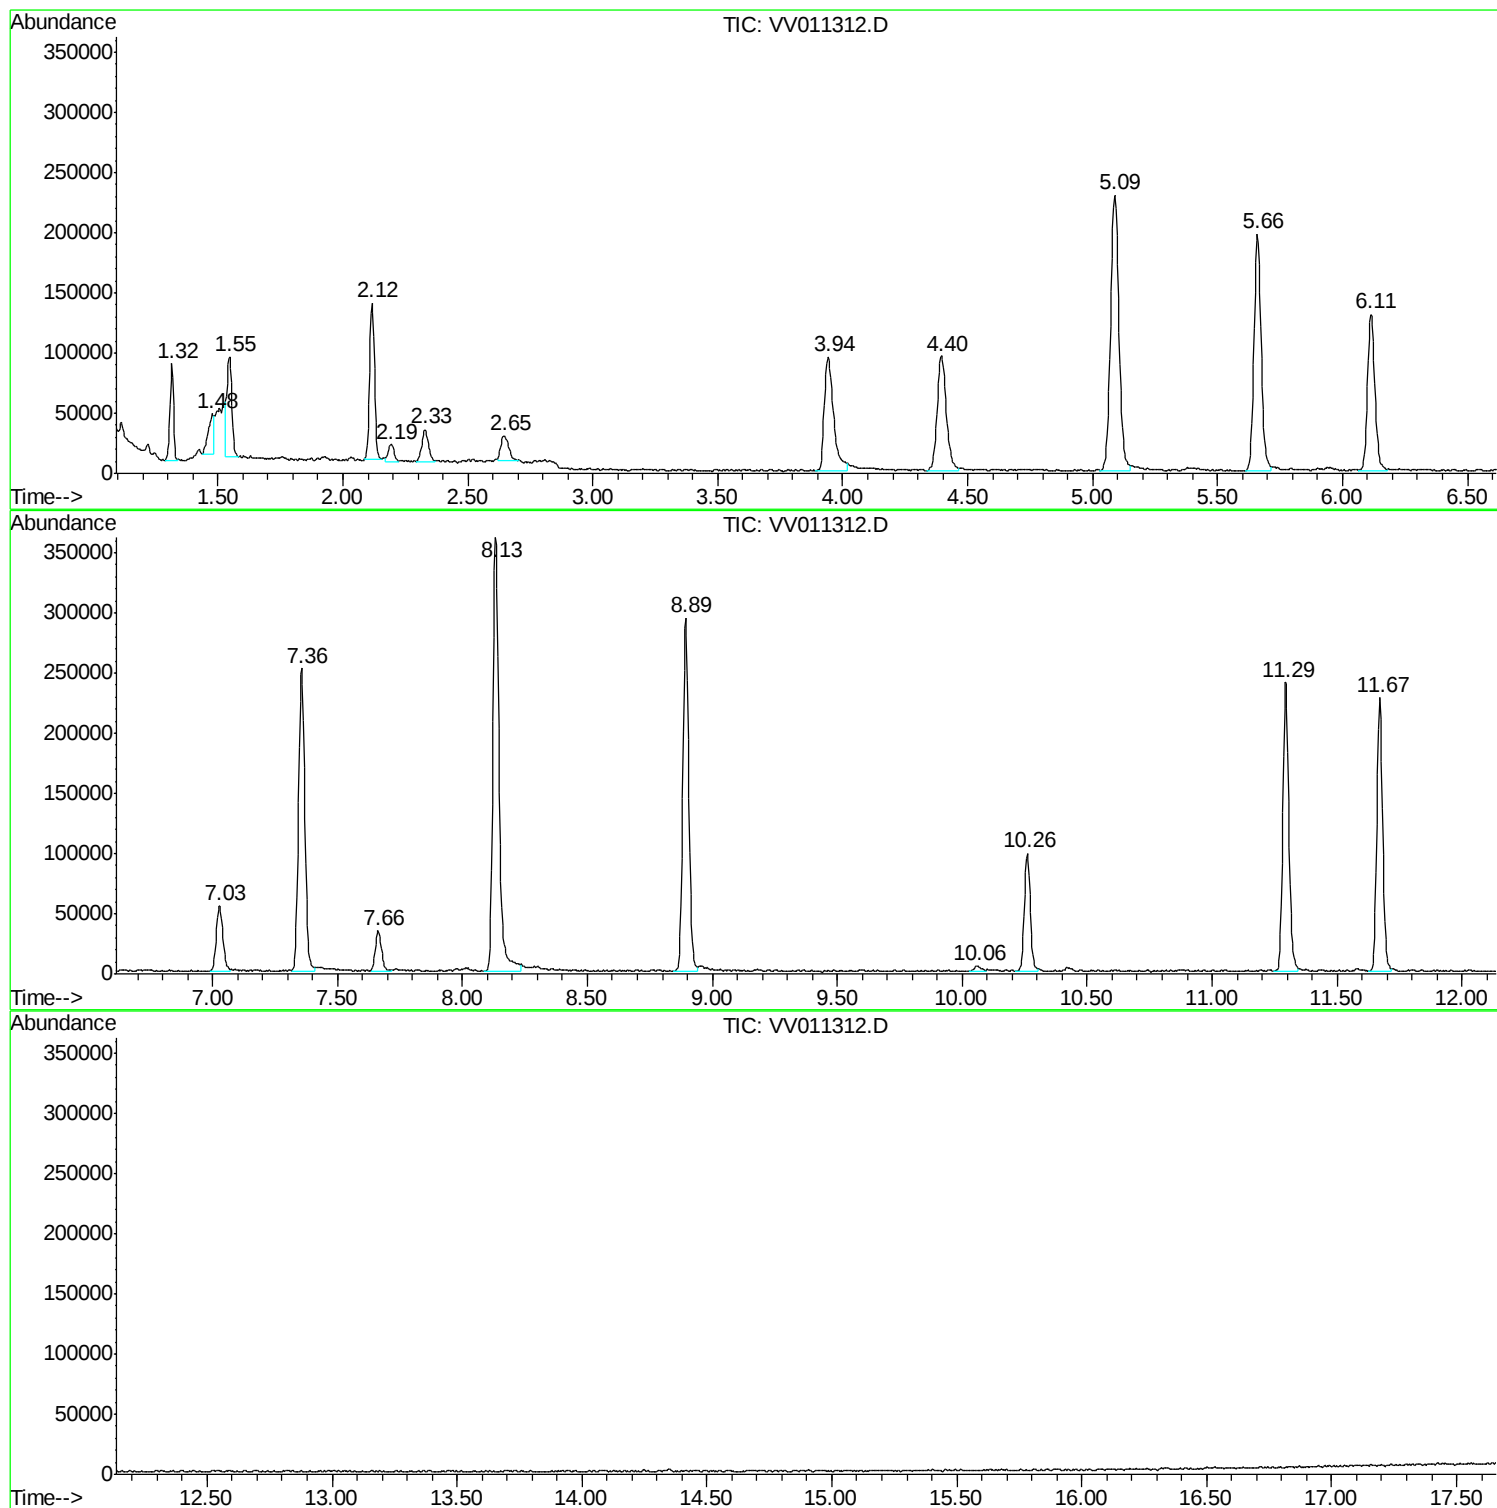

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011312.D
Acq On : 08 Jun 2019 03:55
Operator : SY/MD
Sample : K3228-13
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P14










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.48	0.66 ug/L	51695	1,4-Difluorobenzene	5.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Chloromethylphosphonic dichloride	166	CH2Cl3OP	001983-26-2	27
2		Propanenitrile, 2,2,3-trichloro-	157	C3H2Cl3N	000813-74-1	12
3		Methylene chloride	84	CH2Cl2	000075-09-2	9
4		Methylene chloride	84	CH2Cl2	000075-09-2	9
5		Benzene, 1-azido-4-nitro-	164	C6H4N4O2	001516-60-5	9

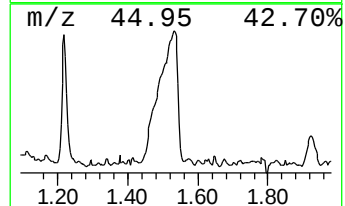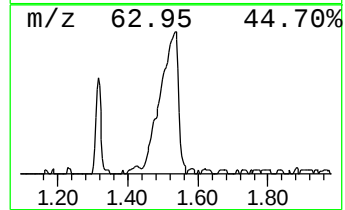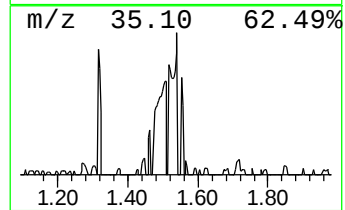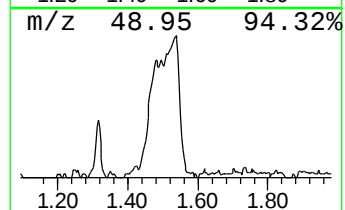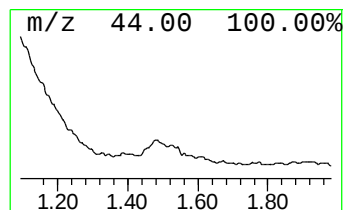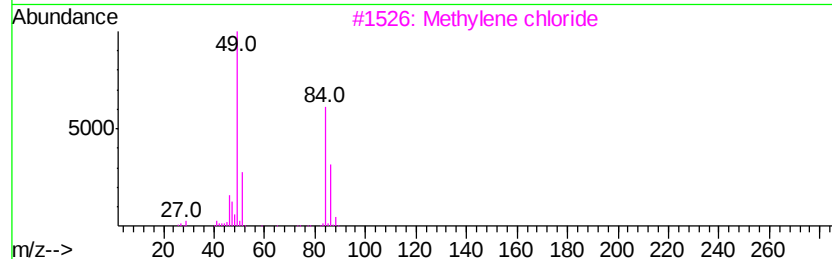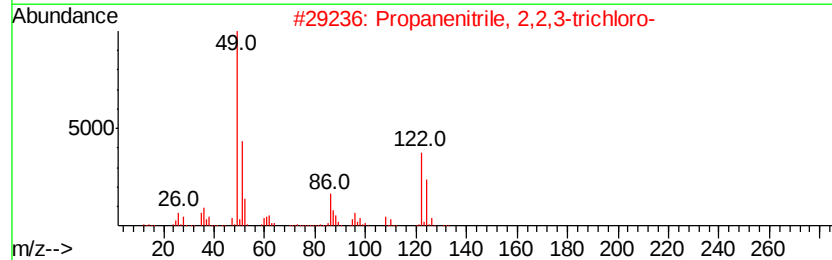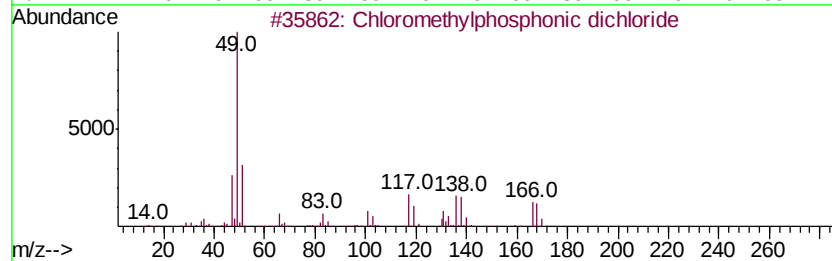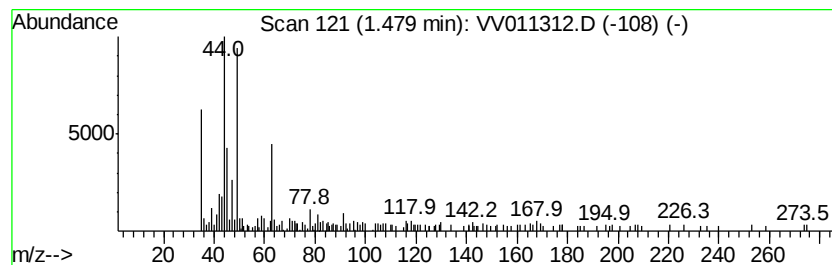

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011312.D
Acq On : 08 Jun 2019 03:55
Operator : SY/MD
Sample : K3228-13
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P14










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.33	0.66 ug/L	51390	1,4-Difluorobenzene	5.66

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	72
2			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	72
3			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	72
4			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	56
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	50

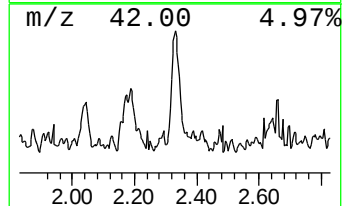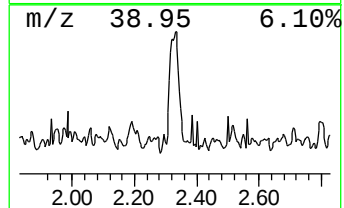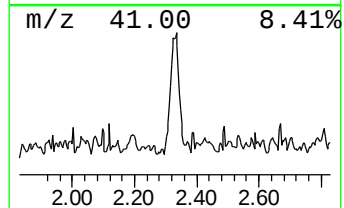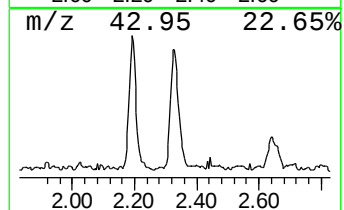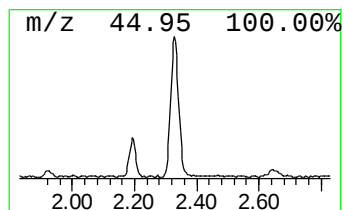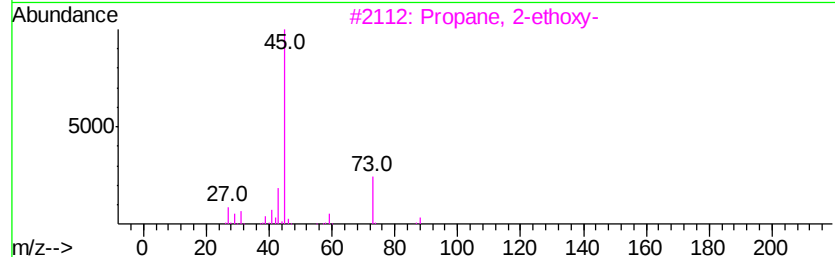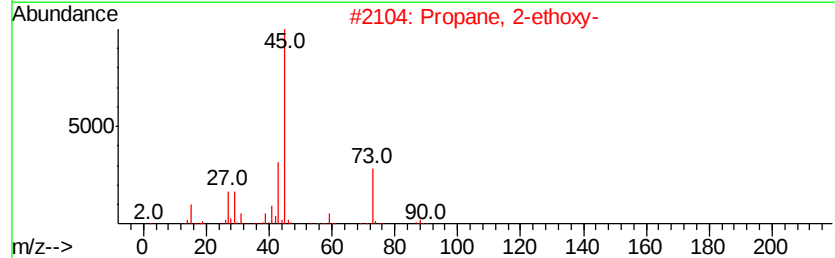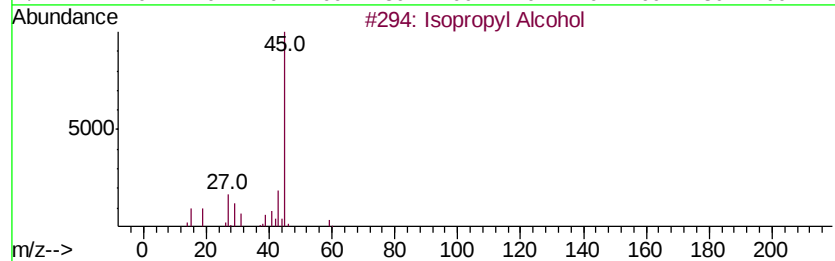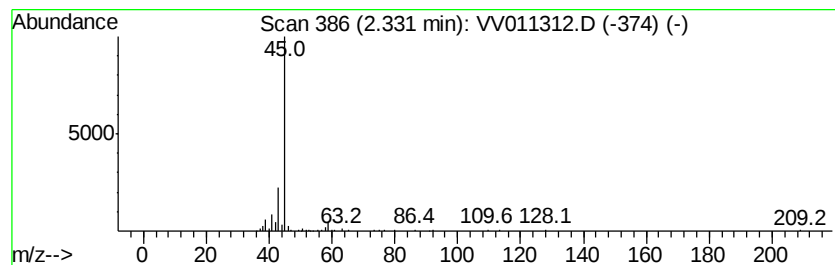

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060619\
Data File : VV011312.D
Acq On : 08 Jun 2019 03:55
Operator : SY/MD
Sample : K3228-13
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P14

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.48	0.7	ug/L	51695	1	5.66	392218	5.0
Isopropyl Alcohol	2.33	0.7	ug/L	51390	1	5.66	392218	5.0