


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060619\
Data File : VV011241.D
Acq On : 06 Jun 2019 13:03
Operator : SY/MD
Sample : BFB44
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB44

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Jun 10 17:09:19 2019

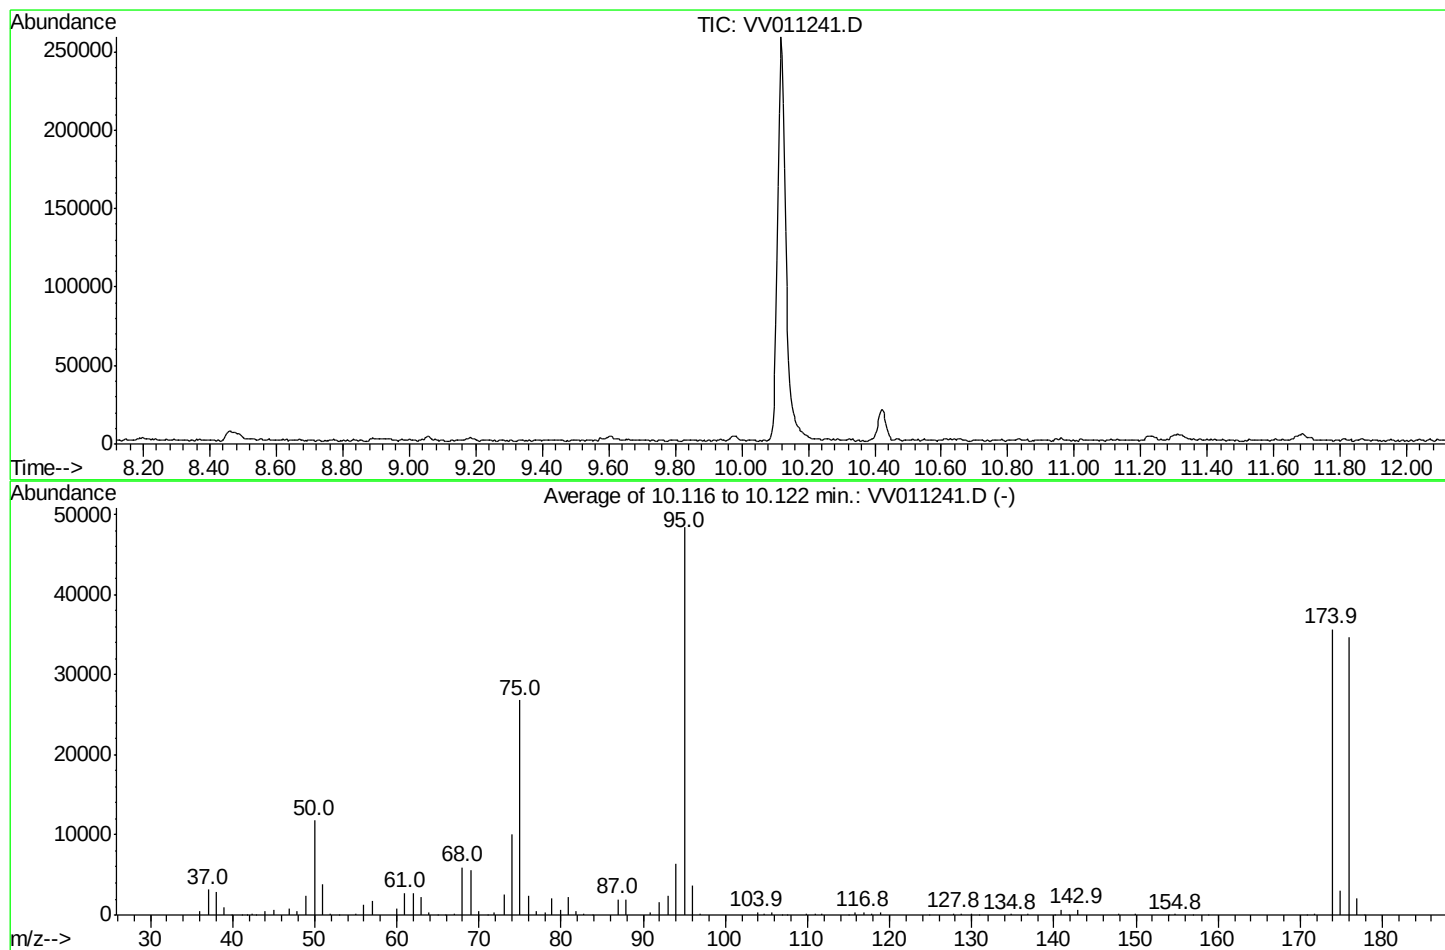

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.4	11812	PASS
75	95	30	80	55.4	26792	PASS
95	95	100	100	100.0	48376	PASS
96	95	5	9	7.6	3663	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.7	35629	PASS
175	174	5	9	8.5	3039	PASS
176	174	95	101	97.5	34733	PASS
177	176	5	9	6.2	2151	PASS

Scan 2794 (10.074 min): VV011241.D
BFB44

m/z	Abundance
35.90	115.0
37.60	128.0
38.30	142.0
39.00	143.0
39.80	258.0
41.20	120.0
43.00	126.0
43.90	492.0
46.30	140.0
48.70	127.0
66.70	122.0
78.90	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
36.00	688.0
37.00	3124.0
38.00	2950.0
39.00	1121.0
39.90	290.0
41.10	159.0
42.40	141.0
42.80	169.0
44.00	1076.0
45.00	626.0
46.90	764.0
47.90	532.0
49.00	2319.0
50.00	11796.0
50.90	3769.0
51.80	188.0
54.90	215.0
55.90	1239.0
57.00	1630.0
60.00	702.0
60.90	2753.0
62.00	2525.0
63.00	2234.0
63.90	298.0
64.90	129.0
65.90	121.0
66.70	134.0
68.00	5802.0
69.00	5436.0
70.00	434.0
71.00	113.0
71.80	359.0
73.00	2566.0
74.00	9973.0
75.00	26648.0
76.00	2555.0
77.00	393.0
78.00	285.0
78.90	2152.0
79.90	655.0
80.90	2244.0
81.80	476.0
82.70	164.0
83.80	122.0
86.90	1972.0
87.90	1842.0
90.80	245.0
91.90	1633.0
92.90	2267.0
94.00	6275.0
95.00	47112.0
96.00	3585.0
97.00	222.0
103.90	399.0
104.70	147.0
105.70	273.0
107.50	102.0
109.90	117.0
110.90	146.0
111.80	107.0
115.00	106.0
115.80	282.0
116.80	381.0
118.00	182.0
118.90	312.0
127.90	206.0
128.70	157.0
130.00	119.0
134.70	105.0
136.90	153.0
140.90	641.0
142.90	667.0
147.90	122.0
149.90	103.0
154.80	153.0
158.80	112.0
170.70	120.0
171.80	182.0
173.90	34344.0
174.90	3114.0
175.90	33080.0
176.90	2121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
35.90	662.0
37.00	3226.0
38.00	2885.0
39.00	1202.0
39.90	274.0
41.10	137.0
41.80	104.0
42.40	148.0
42.90	145.0
44.00	1044.0
45.00	659.0
46.90	846.0
47.90	547.0
48.90	2390.0
50.00	12286.0
51.00	3854.0
51.90	203.0
55.00	241.0
55.90	1294.0
57.00	1783.0
60.00	793.0
61.00	2804.0
62.00	2768.0
63.00	2373.0
63.80	277.0
65.00	120.0
65.80	116.0
67.00	191.0
68.00	6191.0
69.00	5767.0
70.00	470.0
71.00	101.0
71.80	389.0
73.00	2600.0
74.00	10461.0
75.00	27512.0
76.00	2438.0
77.00	450.0
78.00	308.0
78.90	2349.0
79.90	694.0
80.90	2317.0
81.90	511.0
82.70	171.0
83.80	112.0
87.00	1996.0
87.90	1936.0
90.90	285.0
91.90	1758.0
93.00	2456.0
94.00	6589.0
95.00	49896.0
96.00	3812.0
96.90	204.0
103.90	410.0
104.70	151.0
105.70	304.0
106.90	107.0
107.50	103.0
109.80	139.0
110.90	165.0
111.80	162.0
115.80	246.0
116.80	395.0
117.80	194.0
118.90	319.0
127.80	220.0
128.70	153.0
130.00	147.0
134.80	127.0
136.90	140.0
140.10	117.0
140.90	704.0
141.80	119.0
142.90	682.0
147.90	118.0
149.80	115.0
154.00	101.0
154.80	139.0
157.00	112.0
170.80	104.0
171.80	210.0
173.90	36904.0
174.90	3169.0
175.90	35912.0
176.90	2226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
35.90	641.0
37.00	3115.0
38.00	2583.0
39.00	1128.0
40.00	256.0
41.20	146.0
41.80	140.0
42.30	140.0
43.00	127.0
44.00	1022.0
45.00	589.0
46.90	861.0
47.90	490.0
49.00	2308.0
50.00	11354.0
51.00	3671.0
51.90	202.0
52.90	105.0
55.00	257.0
55.90	1162.0
57.00	1735.0
60.00	744.0
61.00	2766.0
62.00	2694.0
63.00	2252.0
63.80	207.0
66.90	220.0
68.00	5892.0
69.00	5603.0
70.00	417.0
71.80	415.0
73.00	2392.0
74.00	9817.0
75.00	26216.0
76.00	2140.0
76.90	420.0
78.00	259.0
78.90	2220.0
79.90	654.0
80.90	2189.0
81.90	510.0
82.70	150.0
87.00	1800.0
87.90	1828.0
90.90	313.0
91.90	1642.0
93.00	2431.0
94.00	6184.0
95.00	48120.0
96.00	3594.0
97.00	143.0
103.90	339.0
104.70	164.0
105.70	305.0
109.80	149.0
110.90	164.0
111.80	157.0
115.80	235.0
116.80	380.0
117.70	223.0
118.80	285.0
124.90	110.0
127.70	214.0
128.80	133.0
129.90	212.0
130.90	135.0
134.80	153.0
140.90	667.0
141.80	118.0
142.90	694.0
147.80	118.0
149.80	101.0
154.80	112.0
157.00	104.0
171.80	221.0
173.90	35640.0
174.90	2835.0
175.90	35208.0
176.90	2106.0
177.80	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44