


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016589.D
Acq On : 06 Jun 2020 14:52
Operator : SY/MD
Sample : L2895-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
EW0K3

Manual Integrations
APPROVED

MMDadoda
6/8/2020 3:05:12 PM

Quant Time: Jun 07 00:36:16 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 06 23:47:35 2020
Response via : Initial Calibration

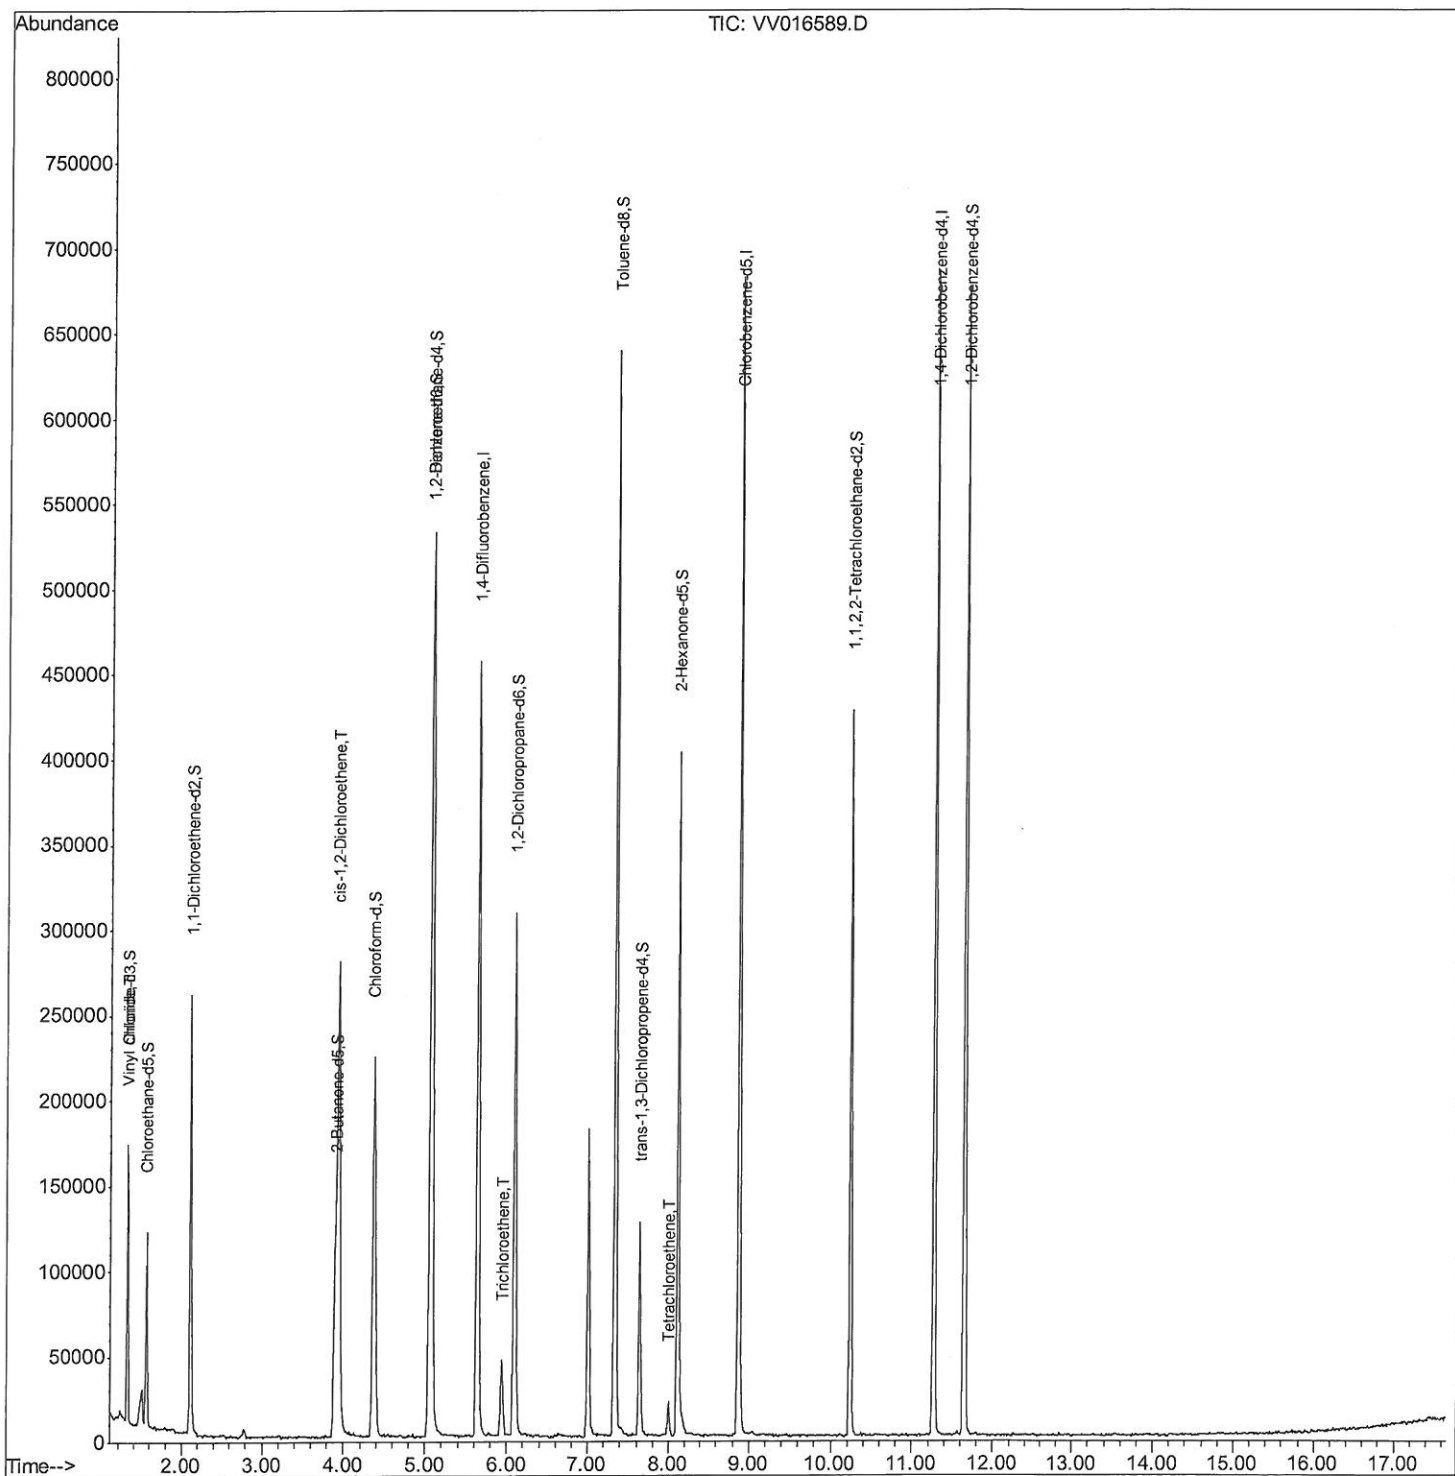

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016589.D
Acq On : 06 Jun 2020 14:52
Operator : SY/MD
Sample : L2895-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0K3

Manual Integrations
APPROVED

MMDadoda
6/8/2020 3:05:12 PM

Quant Time: Jun 06 23:50:16 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 06 23:47:35 2020
Response via : Initial Calibration

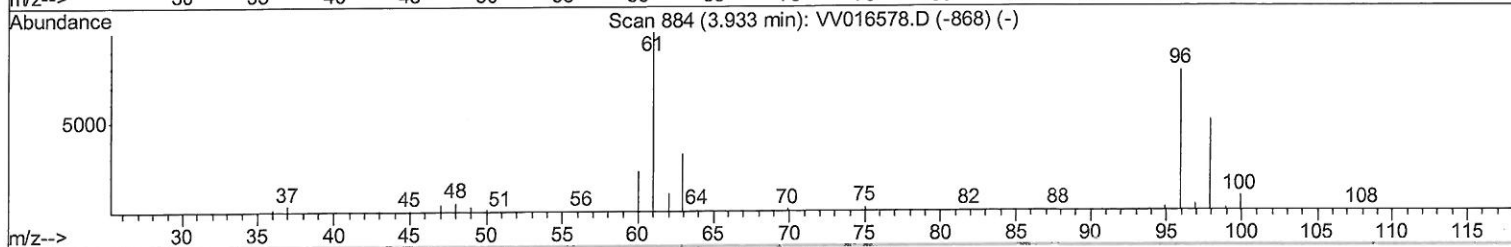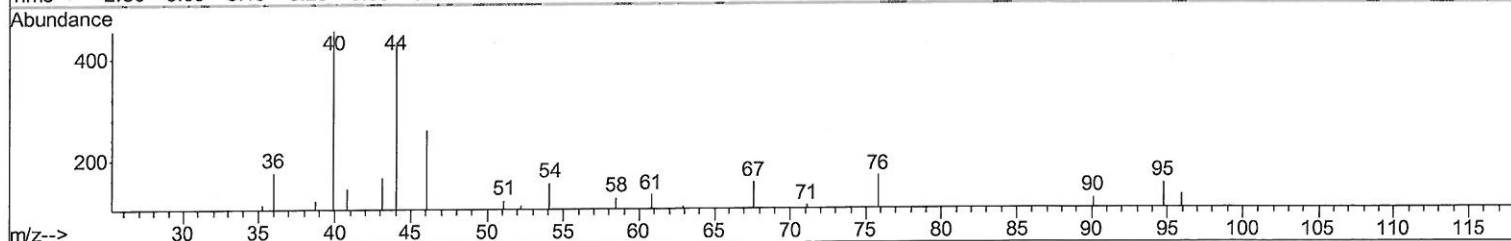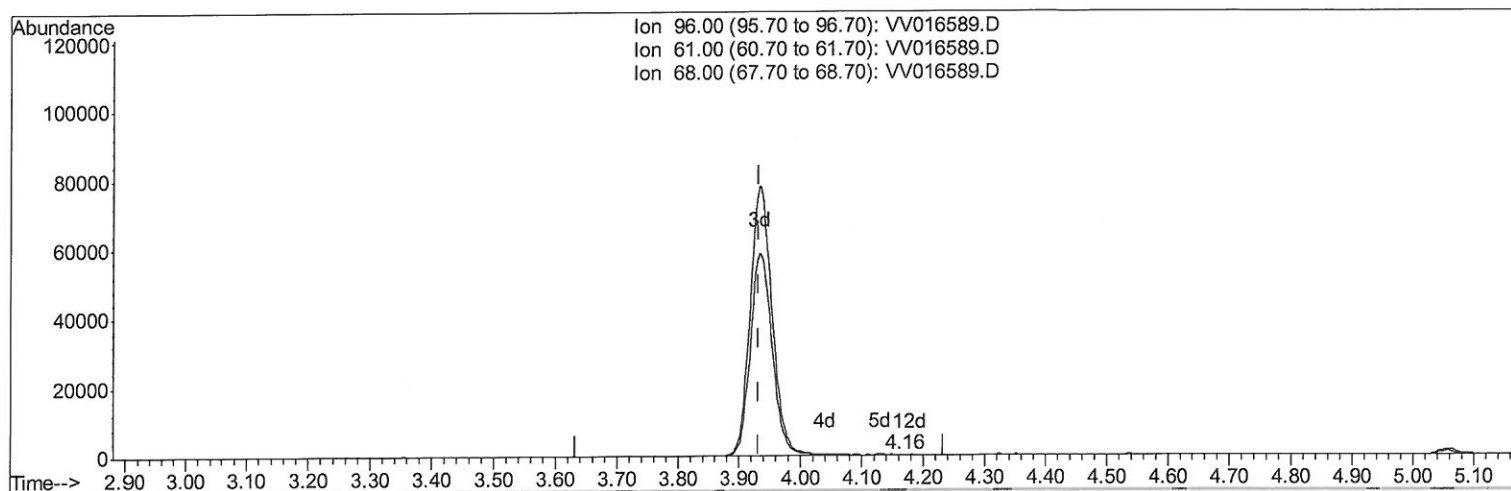

TIC: VV016589.D

(20) cis-1,2-Dichloroethene (T)

4.161min (+0.228) 0.03ug/L

response 94

Ion	Exp%	Act%
96.00	100	100
61.00	133.40	101.55
68.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016589.D
 Acq On : 06 Jun 2020 14:52
 Operator : SY/MD
 Sample : L2895-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0K3

Manual Integrations
 APPROVED

MMDadoda
 6/8/2020 3:05:12 PM

Quant Time: Jun 06 23:50:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 06 23:47:35 2020
 Response via : Initial Calibration

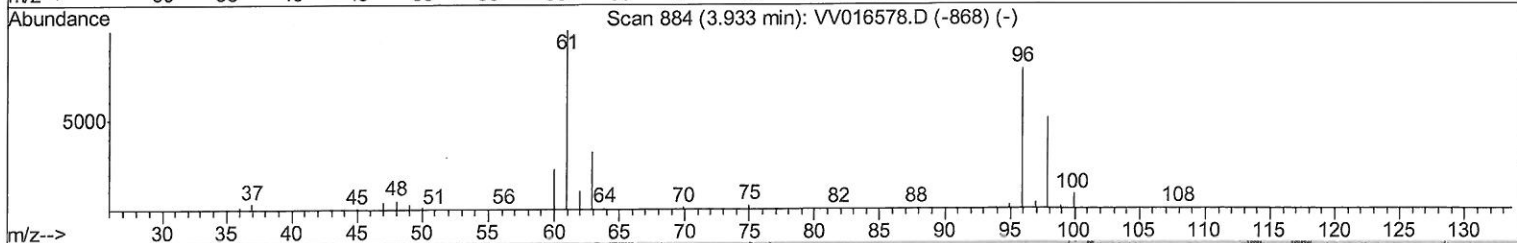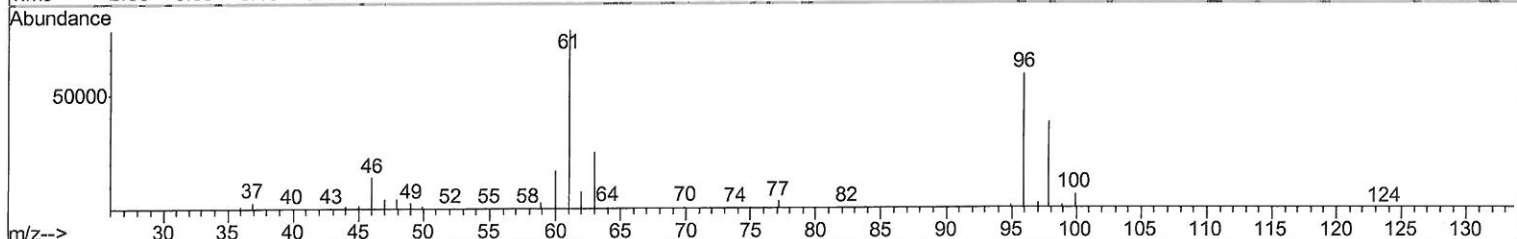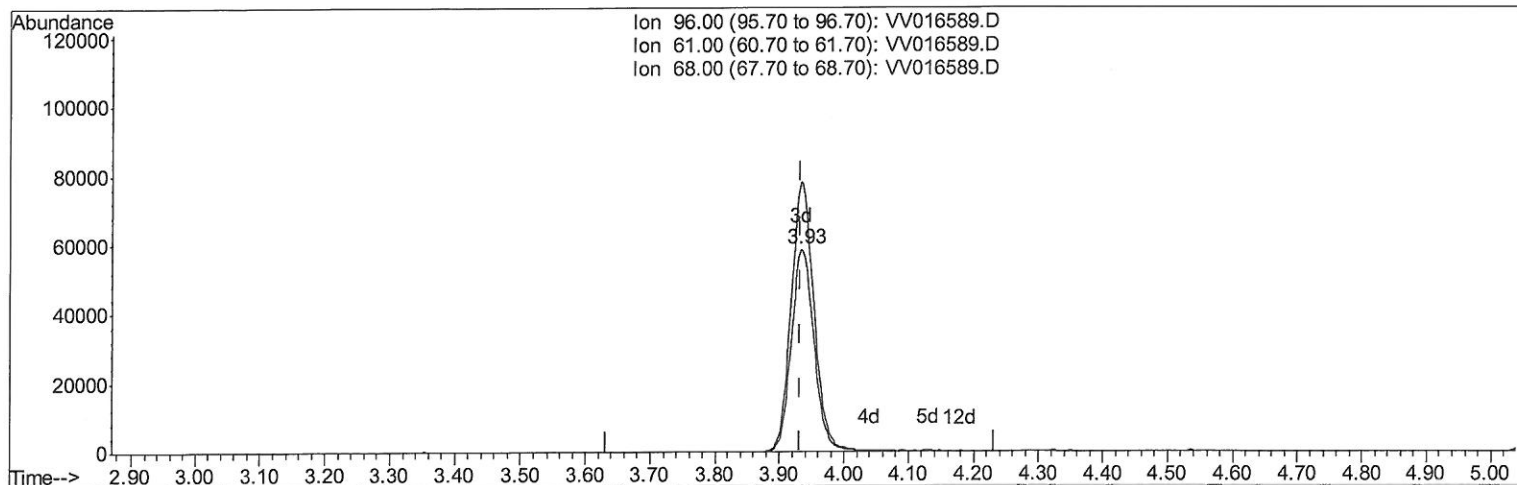

TIC: VV016589.D

(20) cis-1,2-Dichloroethene (T)

3.933min (+0.000) 50.63ug/L m

response 144735

Ion	Exp%	Act%
96.00	100	100
61.00	133.40	133.33
68.00	0.00	0.19#
0.00	0.00	0.00

7 MD
06/20 mg
06/12/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016589.D
 Acq On : 06 Jun 2020 14:52
 Operator : SY/MD
 Sample : L2895-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0K3

Manual Integrations
 APPROVED

MMDadoda
 6/8/2020 3:05:12 PM

Quant Time: Jun 07 00:36:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 06 23:47:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	378171	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	353851	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	169143	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	94601	35.32	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	70.64%
7) Chloroethane-d5	1.56	69	71835	37.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	74.30%
11) 1,1-Dichloroethene-d2	2.12	63	136461	28.74	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	57.48%#
21) 2-Butanone-d5	3.89	46	180285	105.26	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	105.26%
24) Chloroform-d	4.37	84	223563	44.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.96%
26) 1,2-Dichloroethane-d4	5.05	65	157931	46.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.84%
32) Benzene-d6	5.07	84	441436	46.57	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.14%
36) 1,2-Dichloropropane-d6	6.09	67	140528	47.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.16%
41) Toluene-d8	7.34	98	399256	46.38	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.76%
43) trans-1,3-Dichloropropene-	7.64	79	67599	46.97	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.94%
47) 2-Hexanone-d5	8.11	63	135729	107.31	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	107.31%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	190320	47.51	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.02%
64) 1,2-Dichlorobenzene-d4	11.65	152	163674	51.49	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.98%

Target Compounds					Ovalue	
5) Vinyl chloride	1.32	62	3421	1.178	ug/L	# 47
20) cis-1,2-Dichloroethene	3.93	96	144735m	50.626	ug/L	96
34) Trichloroethene	5.94	95	15236	5.580	ug/L	96
46) Tetrachloroethene	8.00	164	4424	2.101	ug/L	96

MD
 06/12/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed