

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016593.D
 Acq On : 06 Jun 2020 16:27
 Operator : SY/MD
 Sample : L2895-14
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L1

Quant Time: Jun 07 00:48:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 06 23:47:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	375336	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	353268	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	166755	50.00	ug/L	0.00


System Monitoring Compounds


4) Vinyl Chloride-d3	1.31	65	92816	34.91	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.82%
7) Chloroethane-d5	1.5					

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016593.D
Acq On : 06 Jun 2020 16:27
Operator : SY/MD
Sample : L2895-14
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L1

Quant Time: Jun 07 00:48:03 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 06 23:47:35 2020
Response via : Initial Calibration

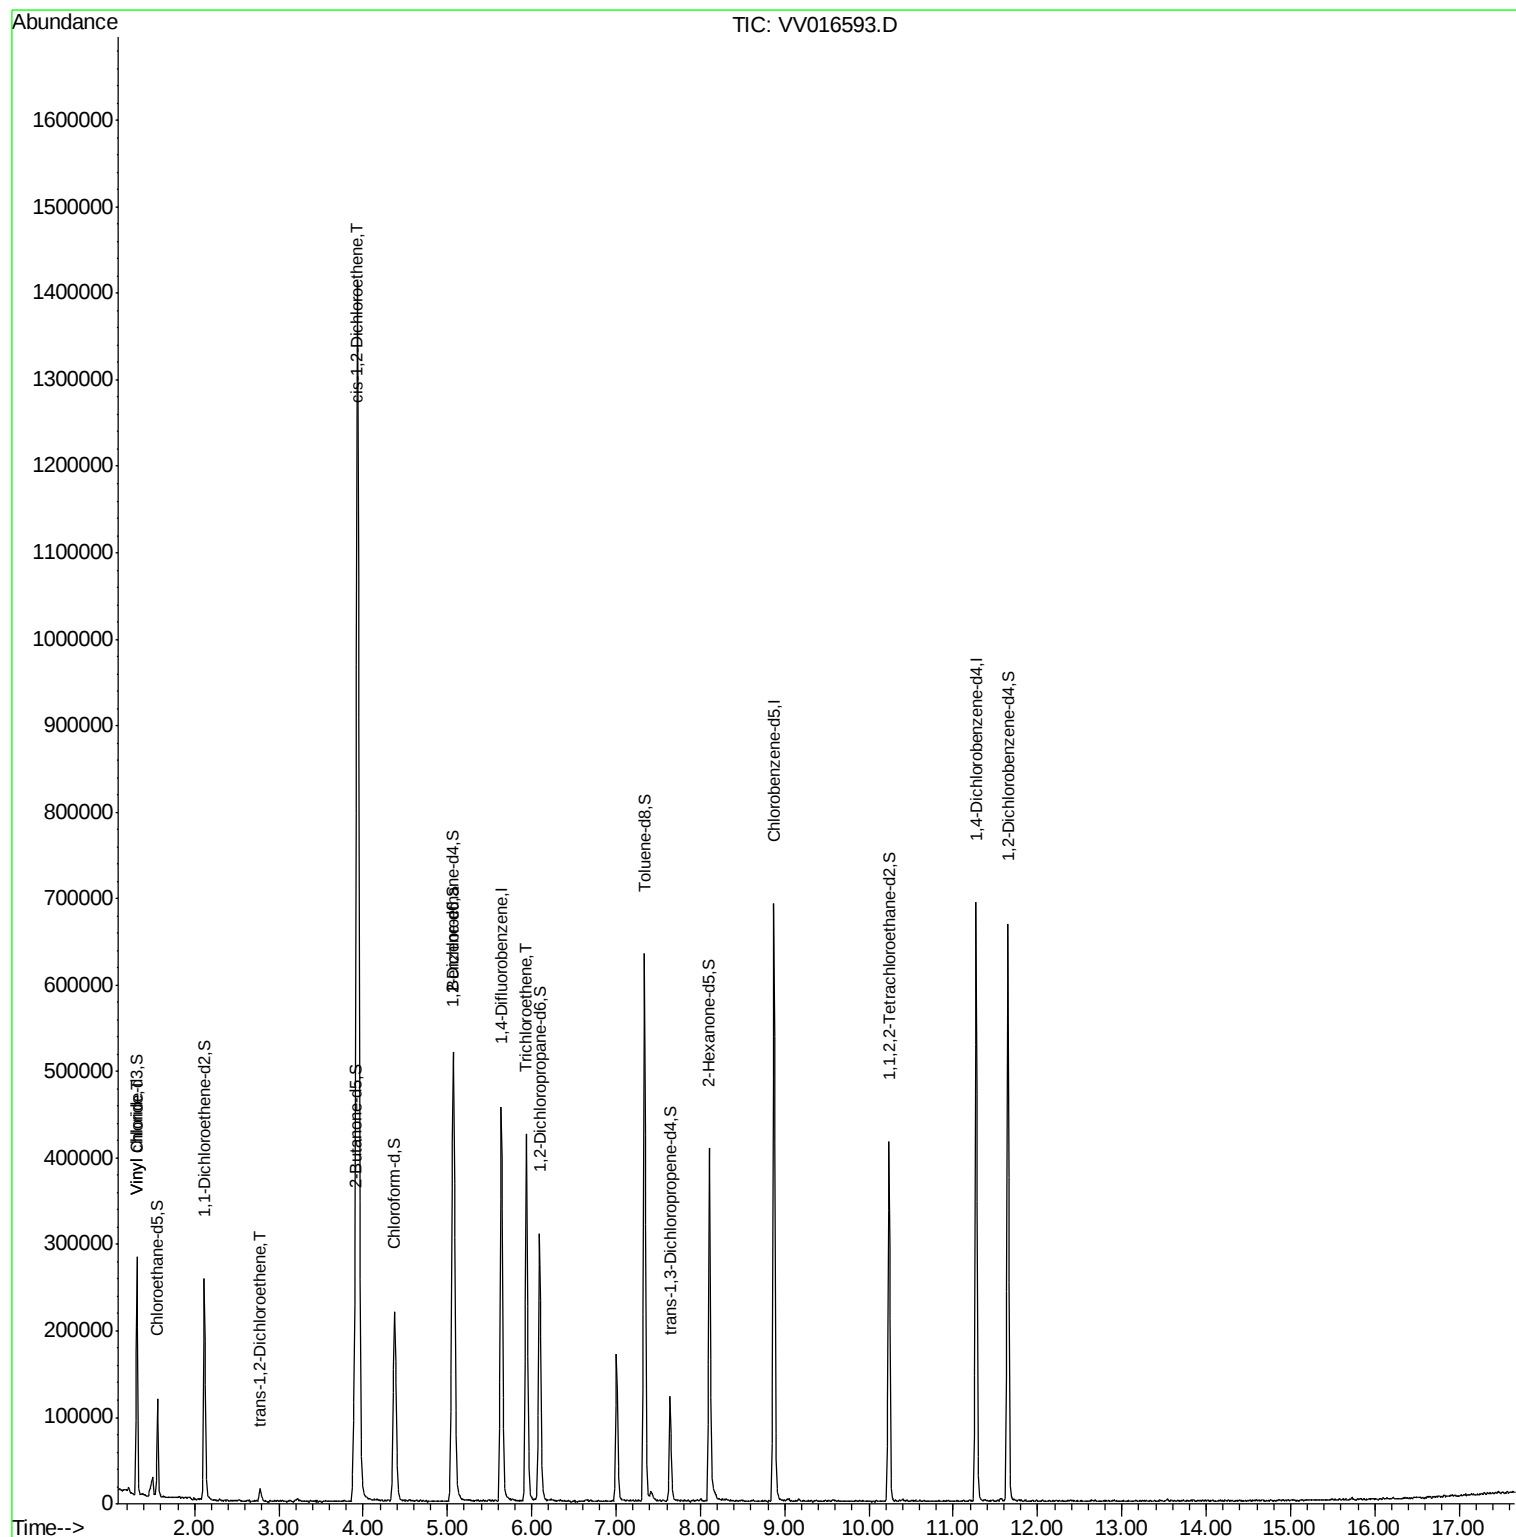

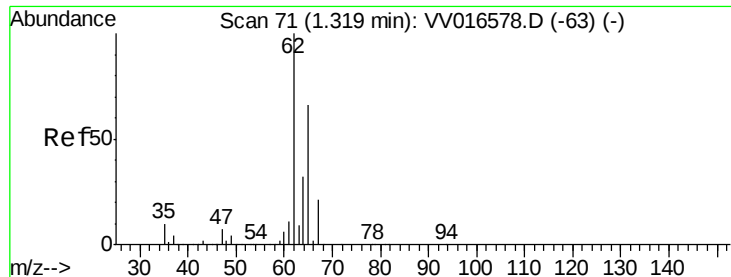

#5

Vinyl chloride

Concen: 28.054 ug/L

RT: 1.32 min Scan# 71

Delta R.T. -0.00 min

Lab File: VV016593.D

Acq: 06 Jun 2020 16:27

Instrument :

MSVOA_V

ClientSampleId :


EW0L1

Tot Ion: 62 Resp: 80878


Ion Ratio Lower Upper

62 100

64 34.5 22.7 42.1

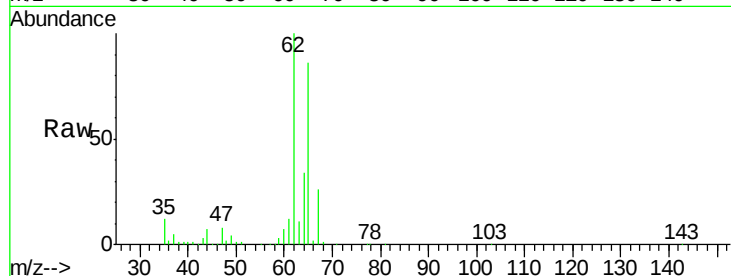

Abundance Ion 62.00 (61.70 to 62.70): VV0

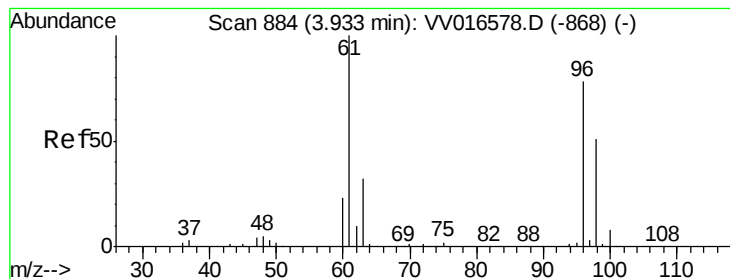

#20

cis-1,2-Dichloroethene
Concen: 270.646 ug/L
RT: 3.93 min Scan# 884
Delta R.T. -0.00 min
Lab File: VV016593.D
Acq: 06 Jun 2020 16:27

Instrument :
MSVOA_V
ClientSampled :
EW0L1

Tot Ion: 96 Resp: 767953
Ion Ratio Lower Upper
96 100
61 133.5 93.4 173.4
68 0.0 0.0 0.0

