

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016595.D
 Acq On : 06 Jun 2020 17:15
 Operator : SY/MD
 Sample : L2895-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW0L4

Quant Time: Jun 07 00:58:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 06 23:47:35 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	370139	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	344100	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	163239	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	89932	34.30	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	68.60%
7) Chloroethane-d5	1.56	69	68034	35.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	71.90%
11) 1,1-Dichloroethene-d2	2.12	63	132035	28.41	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	56.82%#
21) 2-Butanone-d5	3.89	46	177775	106.05	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.05%
24) Chloroform-d	4.37	84	218515	44.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.82%
26) 1,2-Dichloroethane-d4	5.05	65	155787	47.29	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.58%
32) Benzene-d6	5.07	84	431699	46.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.66%
36) 1,2-Dichloropropane-d6	6.09	67	140049	48.76	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.52%
41) Toluene-d8	7.34	98	387169	46.25	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.50%
43) trans-1,3-Dichloropropene-	7.64	79	62677	44.78	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.56%
47) 2-Hexanone-d5	8.11	63	131918	107.25	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	107.25%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	187193	48.06	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.12%
64) 1,2-Dichlorobenzene-d4	11.65	152	161011	52.49	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.98%


Target Compounds					Ovalue
13) Acetone	2.17	43	1985	1.267 ug/L	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016595.D
Acq On : 06 Jun 2020 17:15
Operator : SY/MD
Sample : L2895-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW0L4

Quant Time: Jun 07 00:58:00 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 06 23:47:35 2020
Response via : Initial Calibration

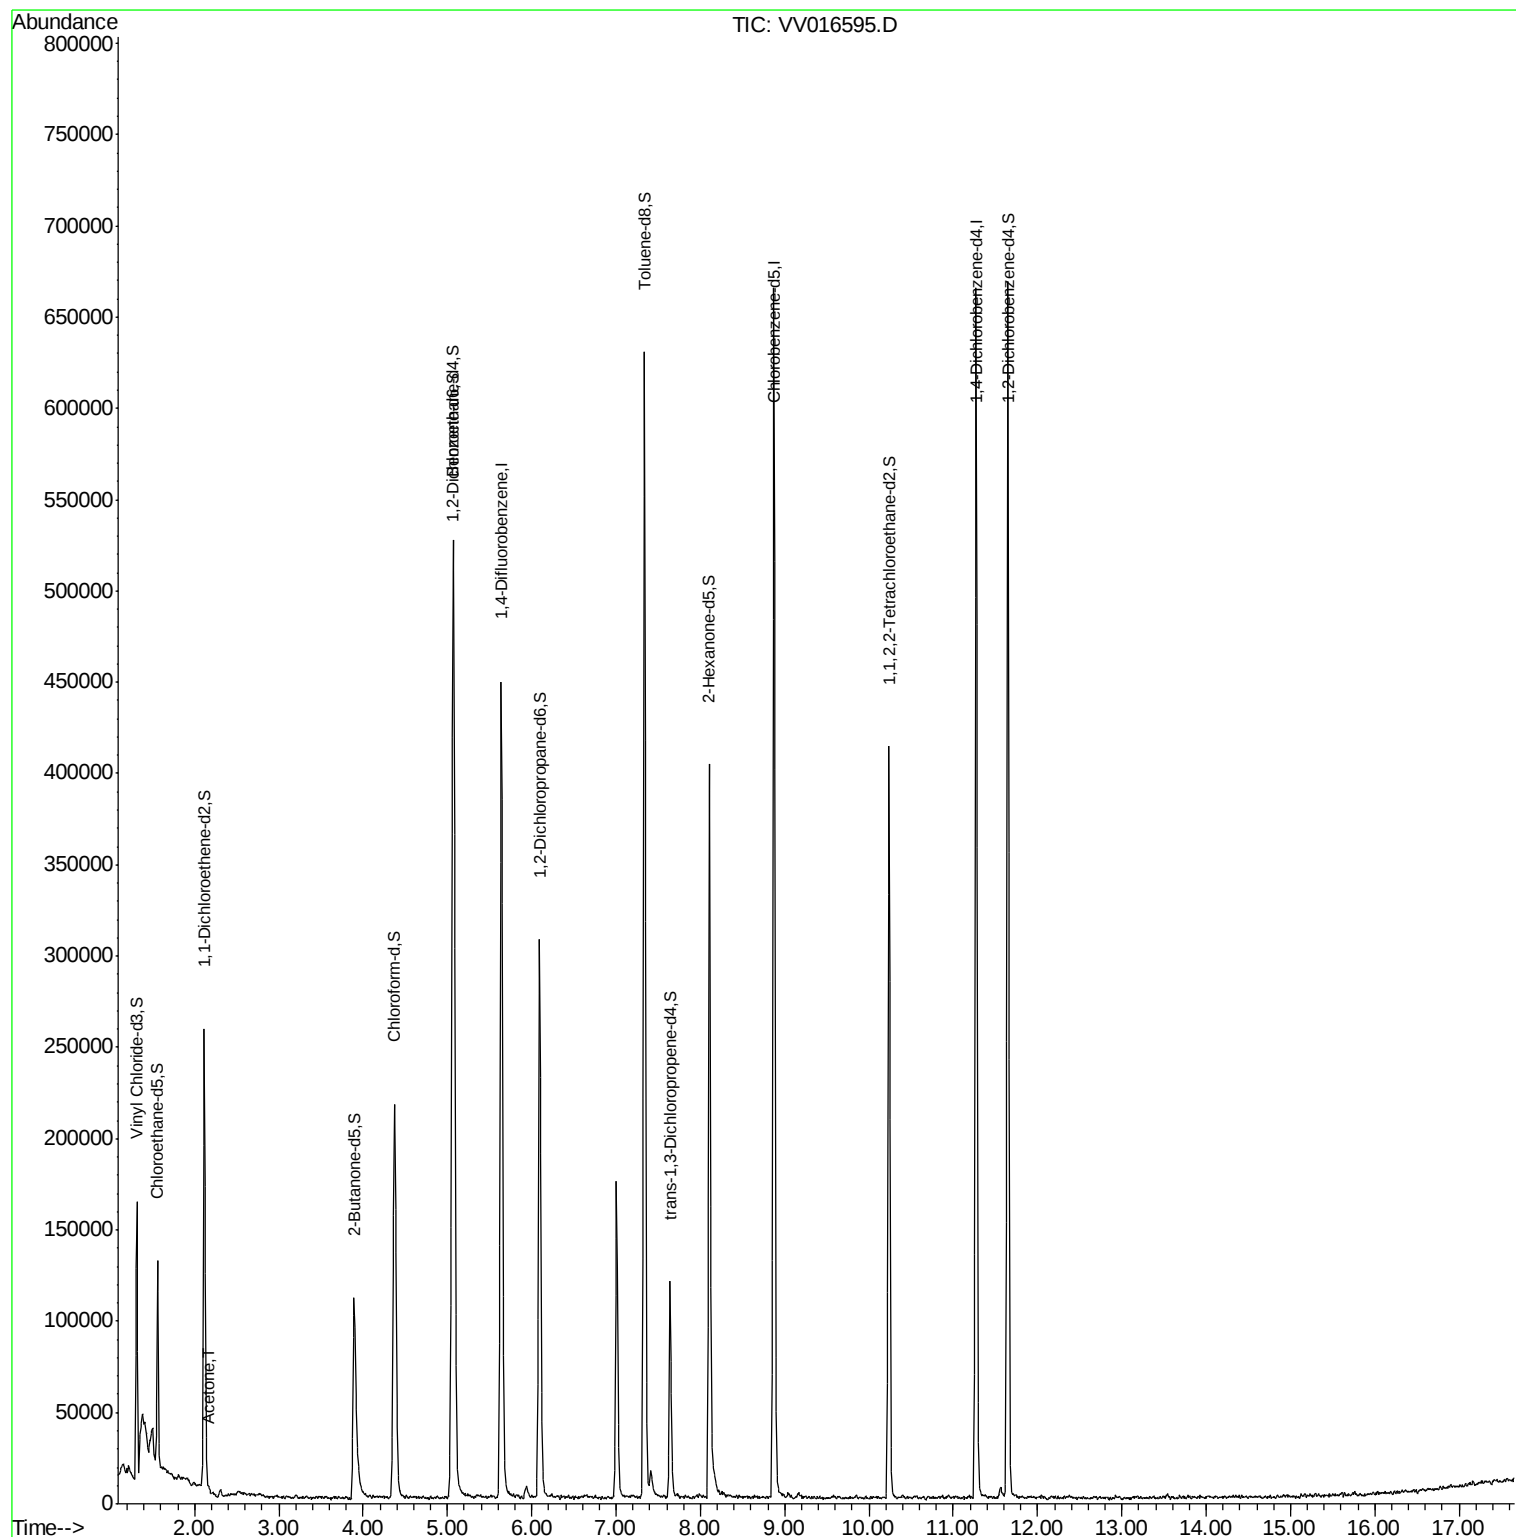

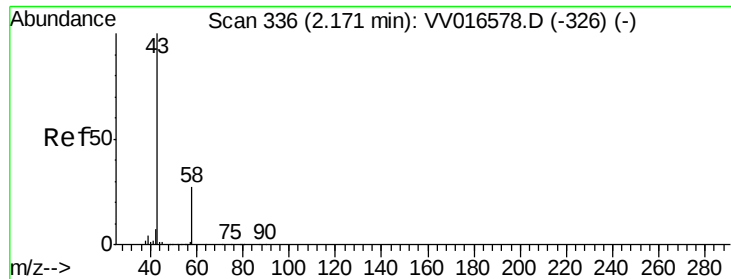

#13

Acetone

Concen: 1.267 ug/L

RT: 2.17 min Scan# 336

Delta R.T. -0.00 min

Lab File: VV016595.D

Acq: 06 Jun 2020 17:15

Instrument :

MSVOA_V

ClientSampleId :


EW0L4

Tot Ion: 43 Resp: 1985

Ion Ratio Lower Upper

43 100

58 55.5 0.0 57.2

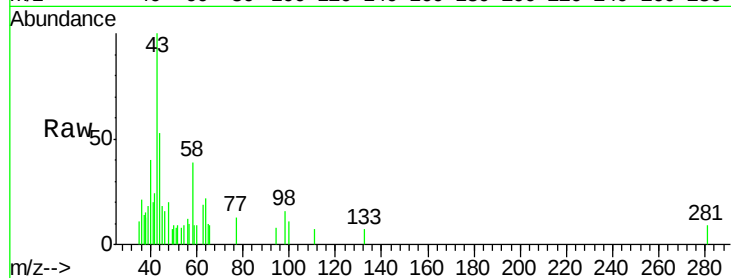

Abundance Ion 43.00 (42.70 to 43.70): VV0

Ion 58.00 (57.70 to 58.70): VV0

