

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016579.D
 Acq On : 06 Jun 2020 10:50
 Operator : SY/MD
 Sample : VV0606WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	82	rVB	211808	218158	13.15%	1.758%
2	1.569	143	149	163	rVB	157759	183177	11.04%	1.476%
3	2.119	310	320	334	rBV	337799	498489	30.05%	4.018%
4	2.377	398	400	403	rBV3	1396	682	0.04%	0.005%
5	2.698	496	500	502	rBV4	1477	1144	0.07%	0.009%
6	2.926	567	571	574	rBV4	1014	901	0.05%	0.007%
7	3.052	606	610	611	rBV3	739	550	0.03%	0.004%
8	3.196	652	655	662	rBV8	1583	1725	0.10%	0.014%
9	3.286	680	683	685	rBV2	1055	781	0.05%	0.006%
10	3.396	713	717	718	rBV2	630	521	0.03%	0.004%
11	3.495	743	748	751	rBV7	1858	1437	0.09%	0.012%
12	3.560	763	768	770	rBV6	1222	1165	0.07%	0.009%
13	3.679	803	805	809	rVB4	886	586	0.04%	0.005%
14	3.704	809	813	815	rBV5	1248	991	0.06%	0.008%
15	3.727	818	820	824	rVV4	1484	872	0.05%	0.007%
16	3.746	824	826	830	rVB4	940	579	0.03%	0.005%
17	3.782	836	837	842	rVB3	874	579	0.03%	0.005%
18	3.891	860	871	905	rVV	140434	382265	23.05%	3.081%
19	4.283	989	993	997	rBV6	1791	1727	0.10%	0.014%
20	4.370	1006	1020	1041	rBV	260921	627609	37.84%	5.059%
21	4.598	1089	1091	1094	rBV3	1036	612	0.04%	0.005%
22	4.785	1147	1149	1153	rBV5	1143	783	0.05%	0.006%
23	4.823	1159	1161	1163	rBV3	1333	765	0.05%	0.006%
24	4.868	1172	1175	1177	rVB3	1478	770	0.05%	0.006%
25	4.929	1188	1194	1196	rBV6	648	645	0.04%	0.005%
26	5.068	1217	1237	1265	rBV2	641461	1658737	100.00%	13.369%
27	5.351	1320	1325	1328	rBV6	2023	1869	0.11%	0.015%
28	5.531	1377	1381	1385	rBV6	1303	1187	0.07%	0.010%
29	5.582	1393	1397	1400	rBV5	1171	1119	0.07%	0.009%
30	5.637	1400	1414	1438	rVV	500448	1004752	60.57%	8.098%
31	6.090	1543	1555	1577	rBV	365732	732172	44.14%	5.901%
32	6.447	1662	1666	1668	rBV3	1546	1127	0.07%	0.009%
33	6.569	1703	1704	1708	rVB3	976	554	0.03%	0.004%
34	6.589	1708	1710	1713	rBV3	807	585	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016579.D
 Acq On : 06 Jun 2020 10:50
 Operator : SY/MD
 Sample : VV0606WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.788	1769	1772	1774	rBV4	743	544	0.03%	0.004%
36	6.804	1775	1777	1779	rBV3	1063	548	0.03%	0.004%
37	6.913	1808	1811	1812	rBV3	1394	613	0.04%	0.005%
38	6.942	1816	1820	1821	rBV4	929	670	0.04%	0.005%
39	7.007	1828	1840	1858	rBV	189960	345010	20.80%	2.781%
40	7.335	1931	1942	1960	rBV	755472	1294920	78.07%	10.437%
41	7.489	1988	1990	1992	rBV3	1141	550	0.03%	0.004%
42	7.640	2028	2037	2054	rBV	134987	226606	13.66%	1.826%
43	7.862	2102	2106	2108	rBV3	1465	1266	0.08%	0.010%
44	8.003	2146	2150	2154	rBV7	1934	1785	0.11%	0.014%
45	8.106	2170	2182	2213	rBV	470554	815838	49.18%	6.576%
46	8.373	2262	2265	2266	rBV2	1376	711	0.04%	0.006%
47	8.871	2408	2420	2437	rBV	753616	1203587	72.56%	9.701%
48	9.241	2533	2535	2538	rBV4	1138	753	0.05%	0.006%
49	9.328	2560	2562	2566	rBV5	1145	838	0.05%	0.007%
50	9.405	2584	2586	2589	rBV4	1037	676	0.04%	0.005%
51	9.431	2592	2594	2599	rVB3	1320	971	0.06%	0.008%
52	9.482	2605	2610	2614	rVB6	920	963	0.06%	0.008%
53	9.511	2614	2619	2624	rVB7	1377	1348	0.08%	0.011%
54	9.537	2624	2627	2631	rVB4	1419	897	0.05%	0.007%
55	9.563	2631	2635	2636	rBV4	2352	1591	0.10%	0.013%
56	9.698	2676	2677	2679	rBV2	1122	609	0.04%	0.005%
57	9.733	2686	2688	2689	rBV3	1274	567	0.03%	0.005%
58	9.904	2738	2741	2745	rVB4	1498	969	0.06%	0.008%
59	10.061	2786	2790	2793	rBV5	1506	1224	0.07%	0.010%
60	10.148	2814	2817	2826	rVB9	1175	1452	0.09%	0.012%
61	10.199	2829	2833	2834	rBV2	1171	822	0.05%	0.007%
62	10.238	2834	2845	2861	rVV	486059	764705	46.10%	6.164%
63	10.566	2940	2947	2950	rVV7	2470	2724	0.16%	0.022%
64	10.656	2973	2975	2977	rBV3	1472	785	0.05%	0.006%
65	10.765	3007	3009	3013	rBV4	1848	1376	0.08%	0.011%
66	10.839	3030	3032	3035	rVB2	1640	718	0.04%	0.006%
67	10.891	3046	3048	3054	rBV6	969	819	0.05%	0.007%
68	10.932	3057	3061	3062	rBV4	2569	1839	0.11%	0.015%
69	11.022	3082	3089	3091	rBV8	1423	1239	0.07%	0.010%
70	11.151	3126	3129	3132	rBV4	1184	992	0.06%	0.008%
71	11.203	3135	3145	3150	rBV9	4002	6258	0.38%	0.050%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060620\
 Data File : VV016579.D
 Acq On : 06 Jun 2020 10:50
 Operator : SY/MD
 Sample : VV0606WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.270	3154	3166	3187	rVV	743998	1132205	68.26%	9.126%
73	11.531	3243	3247	3250	rBV6	1098	1020	0.06%	0.008%
74	11.646	3268	3283	3303	rBV	769475	1207298	72.78%	9.731%
75	11.756	3314	3317	3319	rBV4	937	701	0.04%	0.006%
76	11.833	3339	3341	3343	rBV2	1409	813	0.05%	0.007%
77	11.862	3346	3350	3353	rVB5	1507	1215	0.07%	0.010%
78	11.891	3356	3359	3362	rBV4	855	675	0.04%	0.005%
79	11.955	3374	3379	3381	rBV6	989	710	0.04%	0.006%
80	11.974	3381	3385	3389	rVV5	1475	1521	0.09%	0.012%
81	11.993	3389	3391	3393	rVV3	1413	860	0.05%	0.007%
82	12.016	3397	3398	3403	rVB3	1214	820	0.05%	0.007%
83	12.045	3404	3407	3411	rVB4	1458	1053	0.06%	0.008%
84	12.145	3436	3438	3439	rBV	1128	557	0.03%	0.004%
85	12.238	3464	3467	3469	rBV4	1258	824	0.05%	0.007%
86	12.283	3479	3481	3486	rBV5	1640	1050	0.06%	0.008%
87	12.457	3531	3535	3541	rVV9	1330	1327	0.08%	0.011%
88	12.566	3565	3569	3572	rBV6	1305	1295	0.08%	0.010%
89	12.672	3592	3602	3610	rVV10	6683	10495	0.63%	0.085%
90	12.891	3667	3670	3671	rBV3	1203	584	0.04%	0.005%
91	13.129	3741	3744	3747	rVB5	1277	1052	0.06%	0.008%
92	13.157	3747	3753	3755	rBV4	1462	1626	0.10%	0.013%
93	13.170	3755	3757	3761	rVV5	1381	954	0.06%	0.008%
94	13.190	3761	3763	3766	rVV3	881	526	0.03%	0.004%
95	13.286	3785	3793	3804	rBV8	8650	15354	0.93%	0.124%
96	13.492	3855	3857	3859	rBV3	1213	651	0.04%	0.005%
97	13.736	3928	3933	3936	rBV5	1502	1281	0.08%	0.010%
98	14.495	4167	4169	4172	rBV2	1198	599	0.04%	0.005%
99	14.553	4185	4187	4192	rVB6	1932	1272	0.08%	0.010%
100	15.003	4324	4327	4329	rBV4	2147	1249	0.08%	0.010%


Sum of corrected areas: 12406985

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060620\
Data File : VV016579.D
Acq On : 06 Jun 2020 10:50
Operator : SY/MD
Sample : VV0606WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

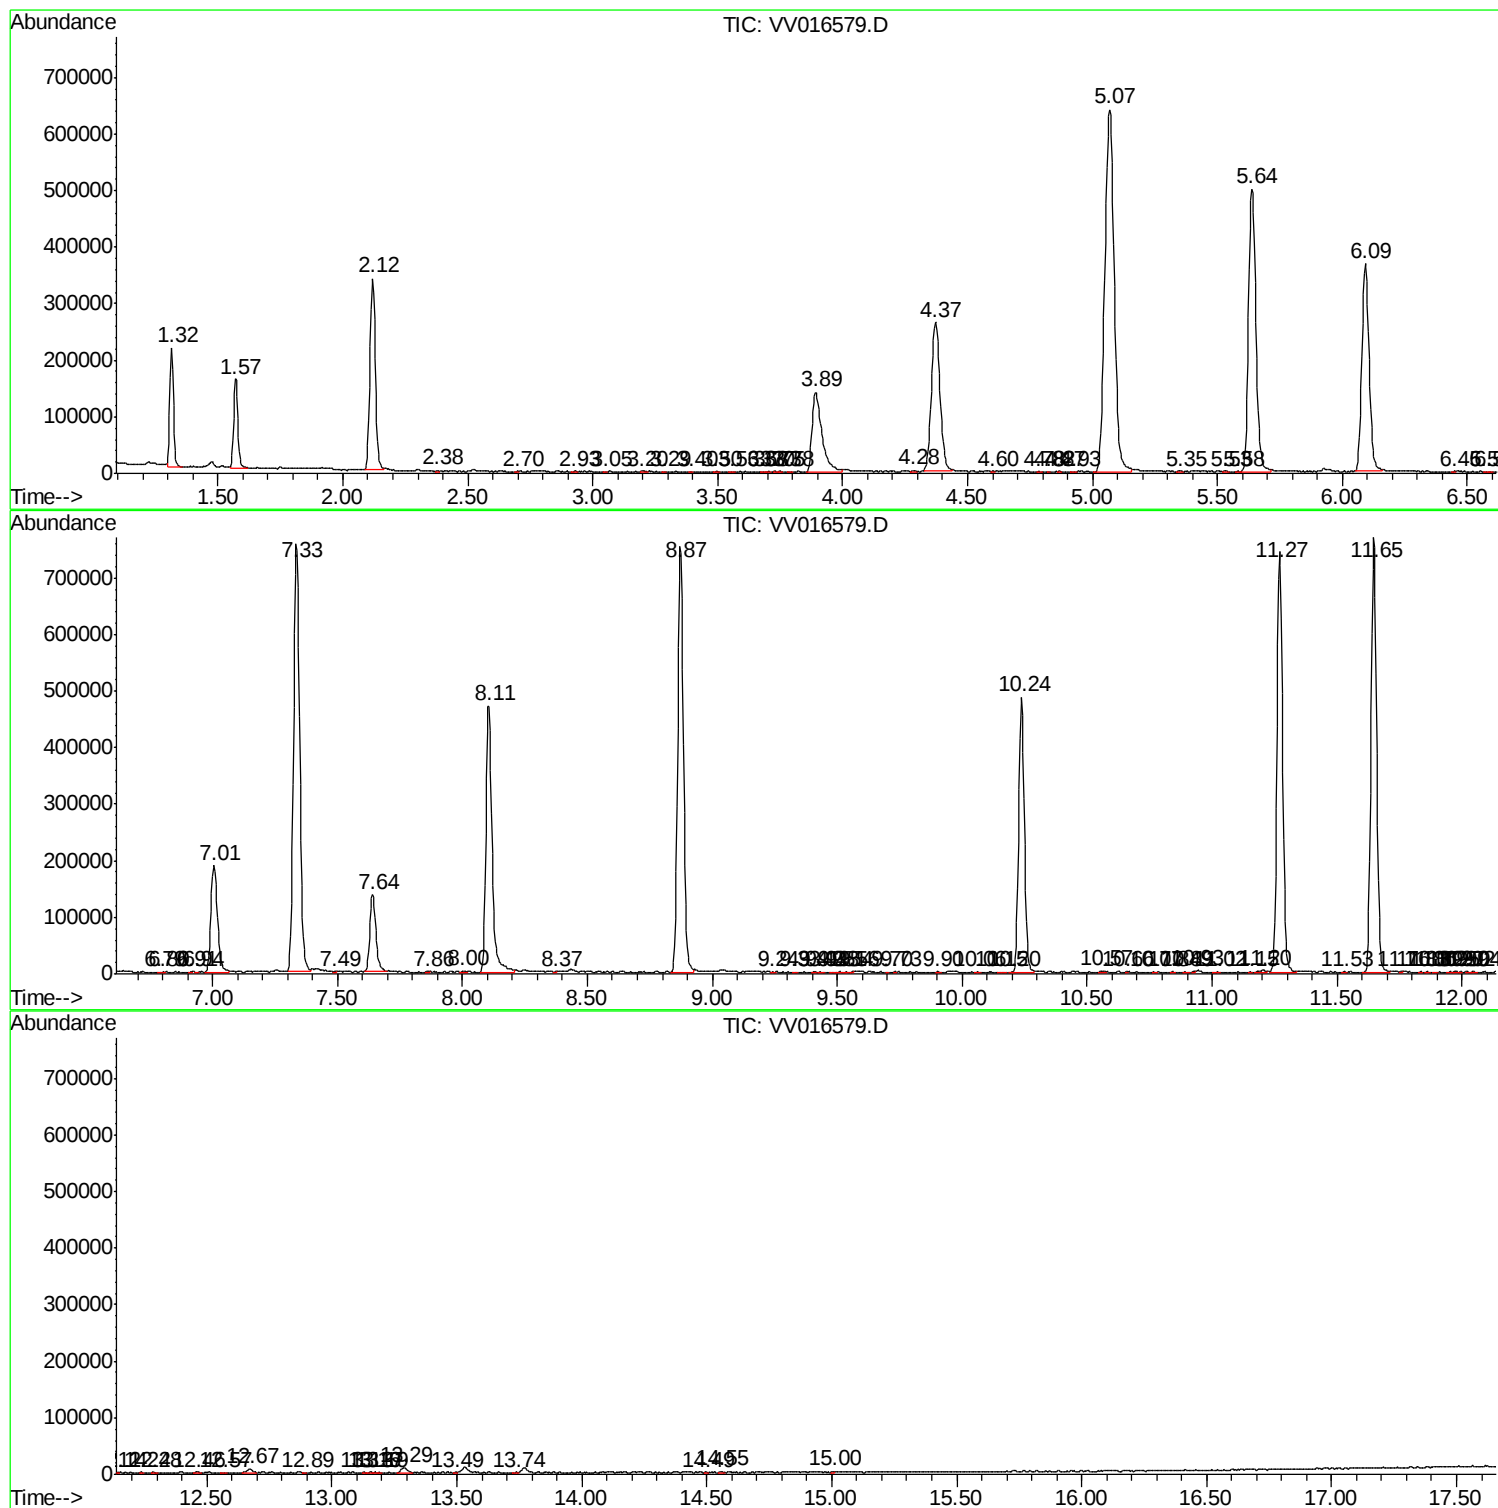

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016579.D
Acq On : 06 Jun 2020 10:50
Operator : SY/MD
Sample : VV0606WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060620\
Data File : VV016579.D
Acq On : 06 Jun 2020 10:50
Operator : SY/MD
Sample : VV0606WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc